
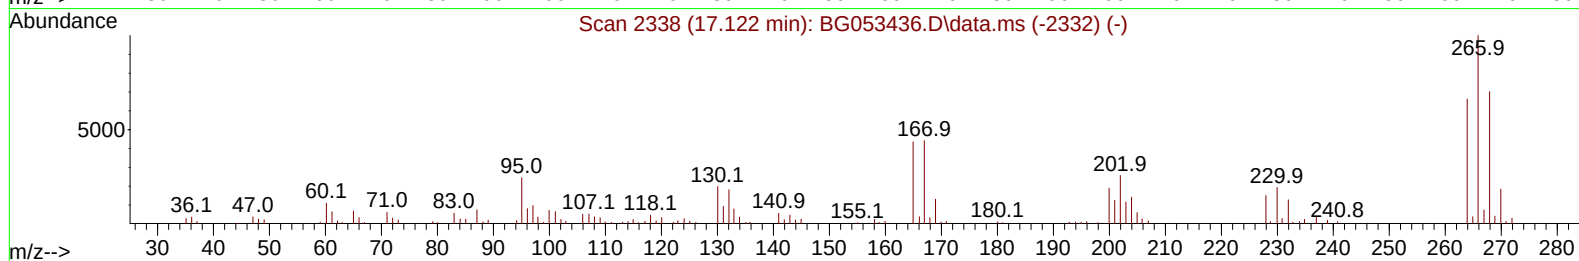
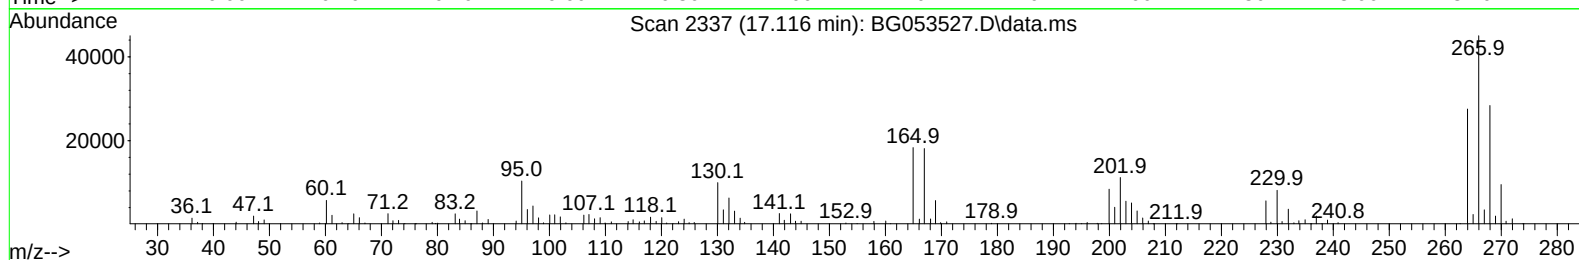


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051222\
Data File : BG053527.D
Acq On : 12 May 2022 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:09:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

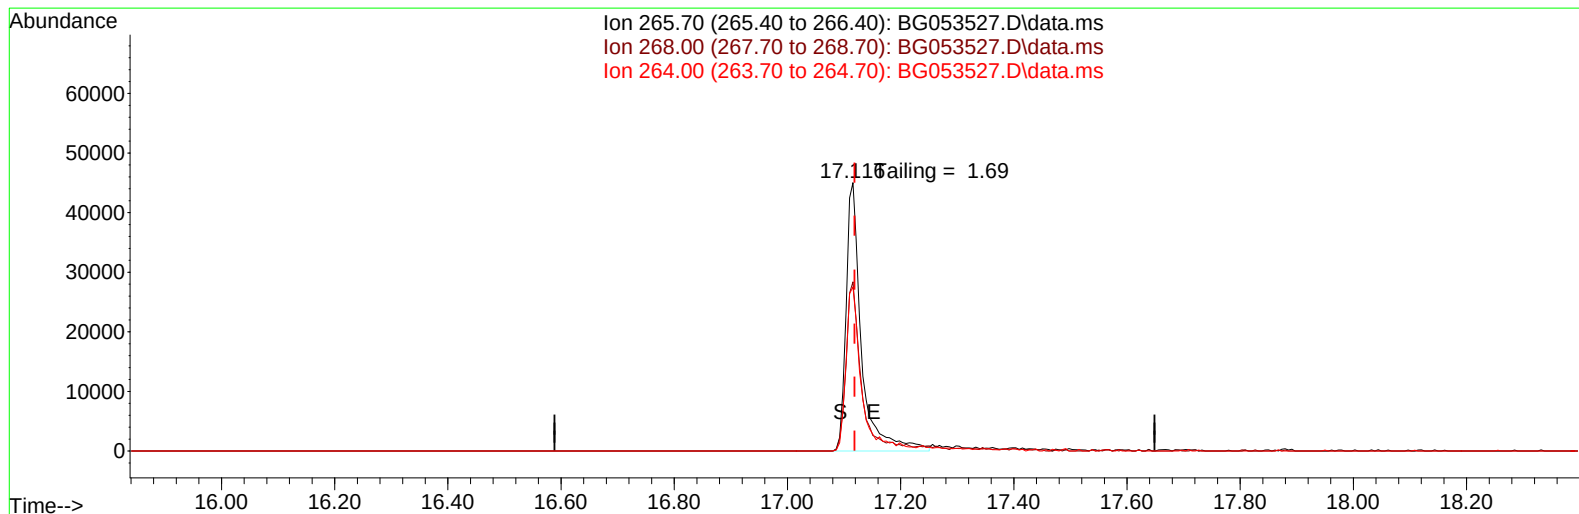

TIC: BG053527.D\data.ms

(70) Pentachlorophenol (C)




17.116min (-0.003) 42819.96 ng

response 85481

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.00
264.00	66.20	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051222\
Data File : BG053527.D
Acq On : 12 May 2022 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:09:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

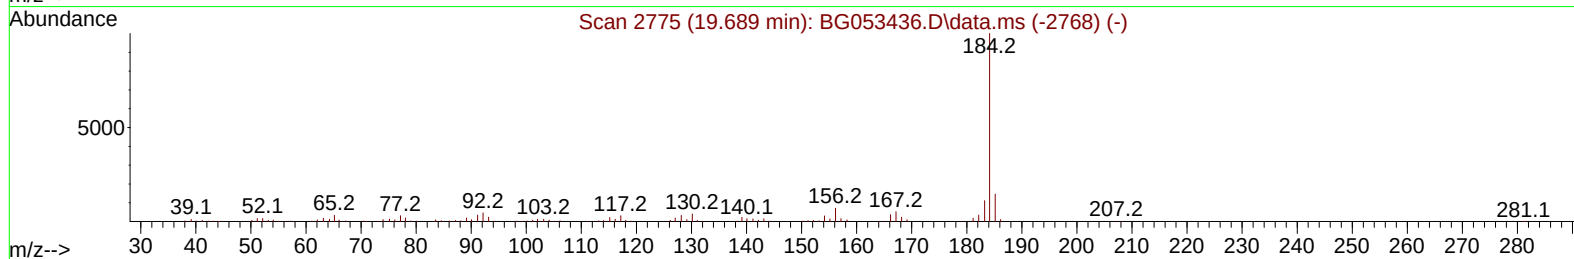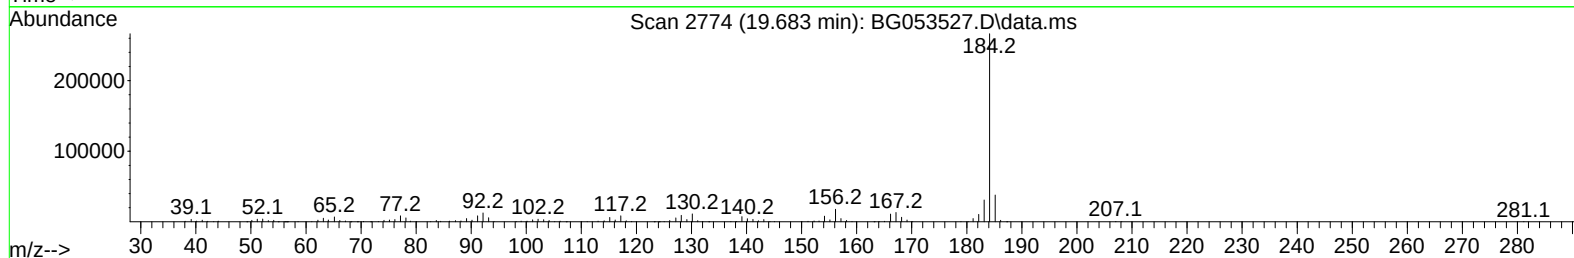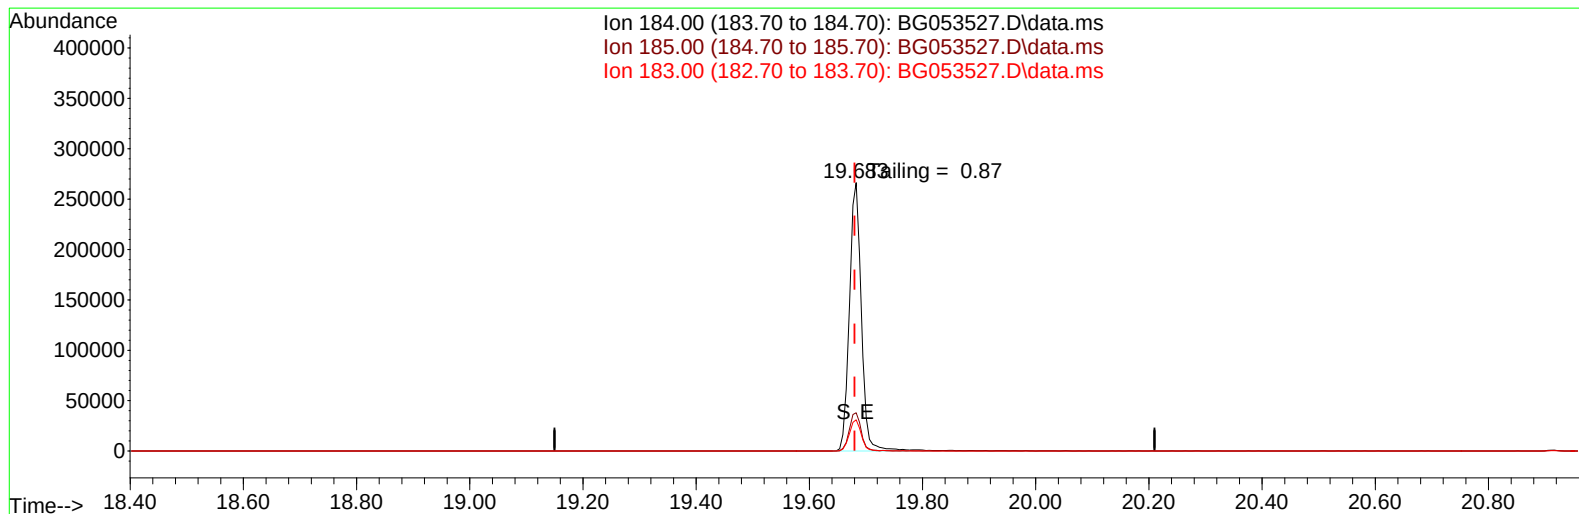

TIC: BG053527.D\data.ms

(77) Benzidine

19.683min (+ 0.003) 0.00 ng

response 389000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.24
183.00	11.10	11.67
0.00	0.00	0.00