
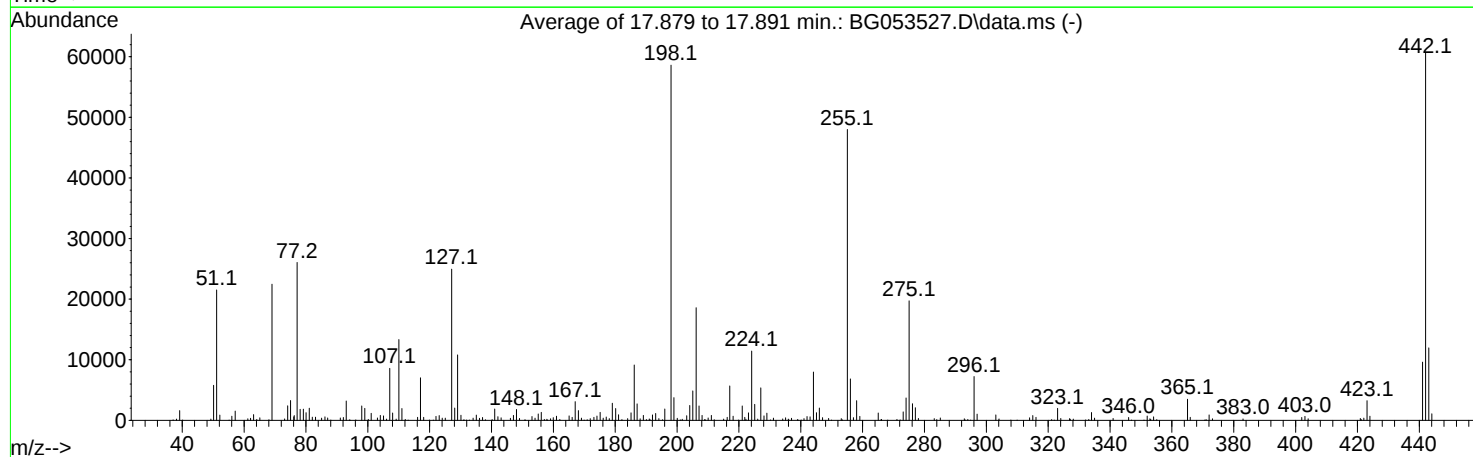


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051222\
 Data File : BG053527.D
 Acq On : 12 May 2022 9:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

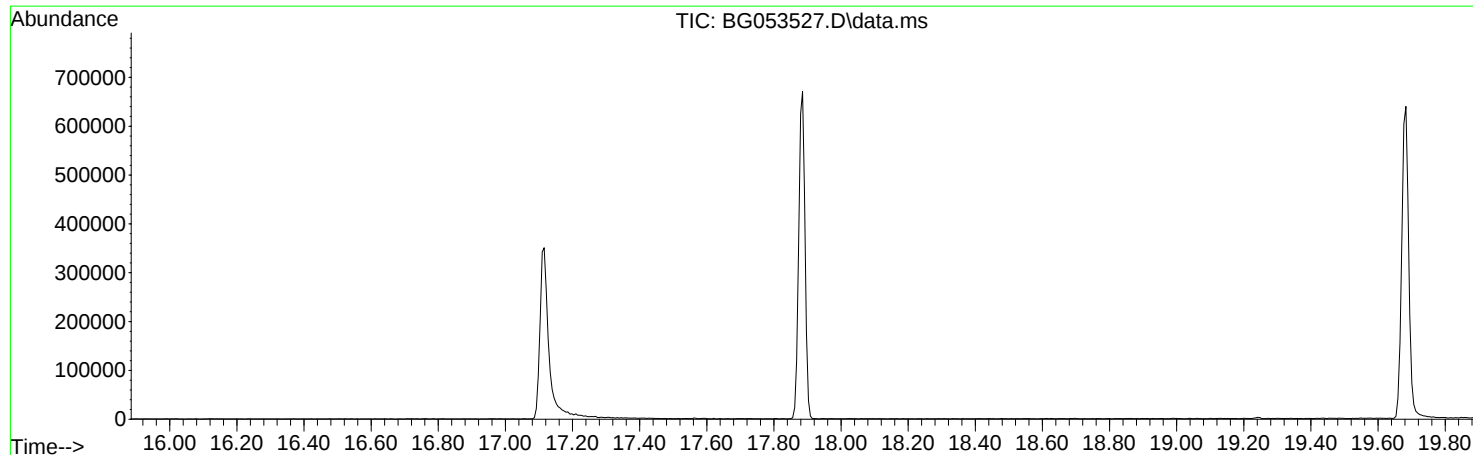

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	21522	PASS
68	69	0.00	2	0.5	116	PASS
69	198	0.00	100	38.3	22457	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	24944	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58616	PASS
199	198	5	9	6.4	3756	PASS
275	198	10	60	33.6	19723	PASS
365	198	1	100	5.9	3484	PASS
441	198	0.01	100	16.4	9611	PASS
442	442	50	100	100.0	60696	PASS
443	442	15	24	19.7	11951	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2022	BNA_G	<u>BG053527.D</u>
Compound Name	Response	Retention Time
DDT	206172	20.916
DDD	6779	20.47
DDE	247	19.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7026	213198	3.30

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051222\
Data File : BG053527.D
Acq On : 12 May 2022 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 07:09:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

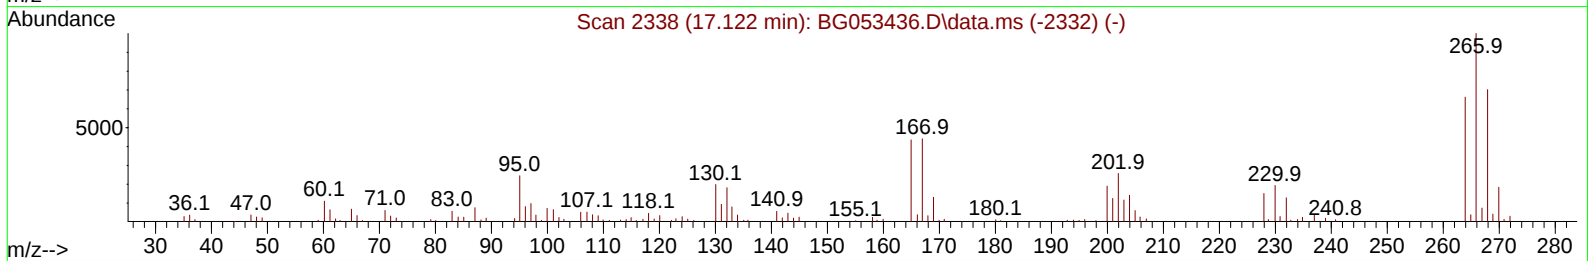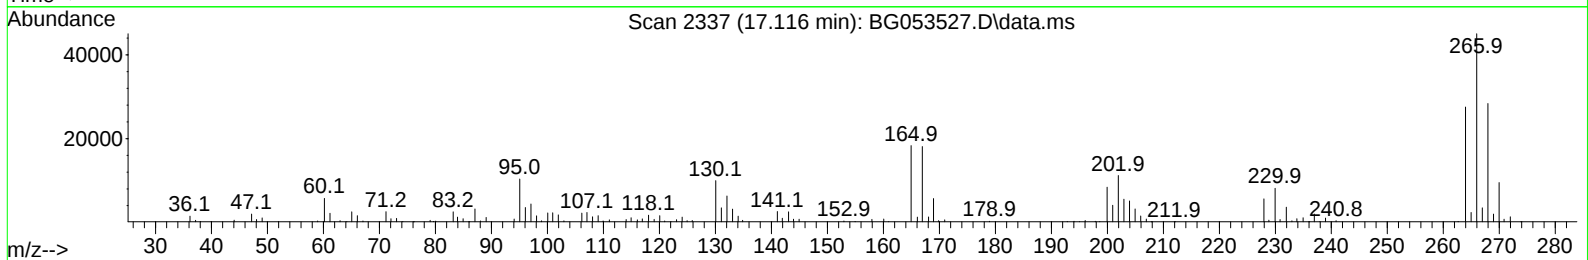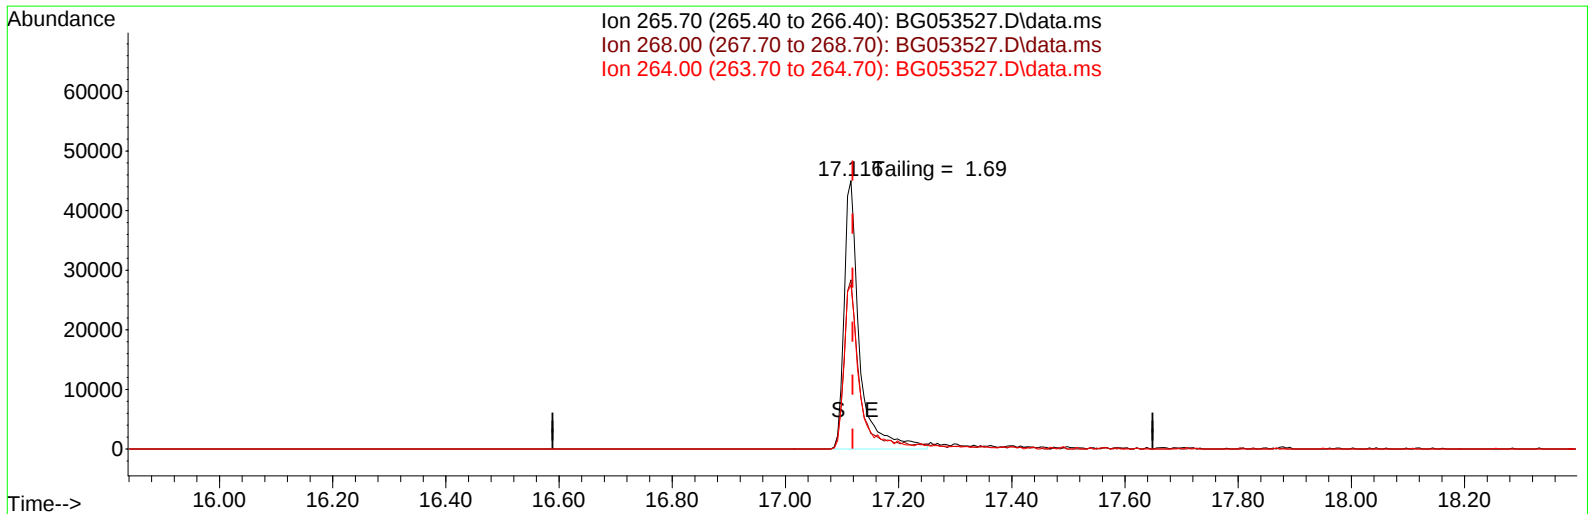

TIC: BG053527.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.003) 42819.96 ng




response 85481

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.00
264.00	66.20	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051222\
Data File : BG053527.D
Acq On : 12 May 2022 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 07:09:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

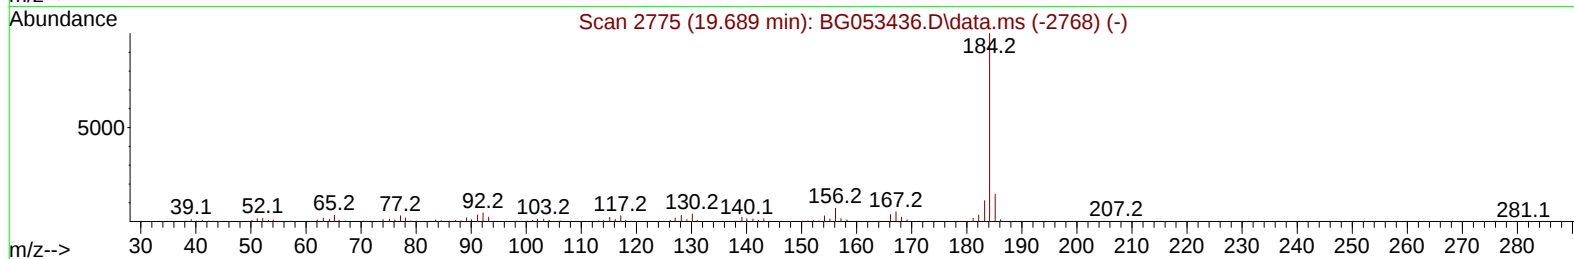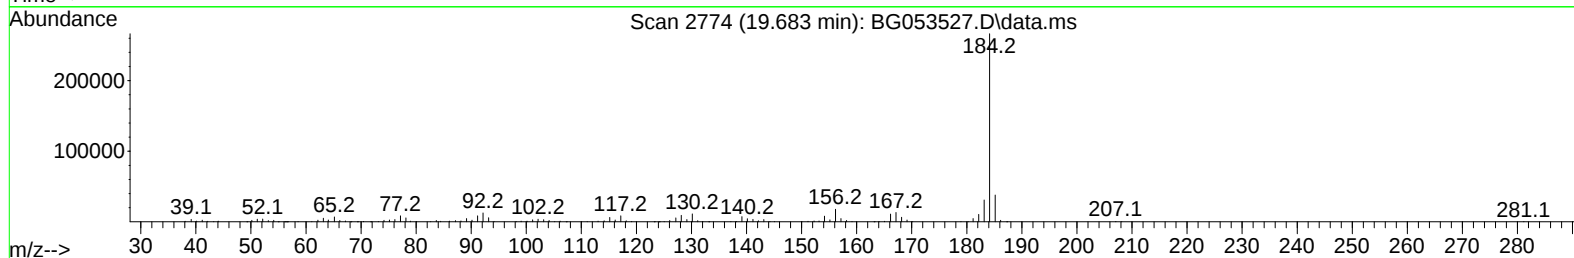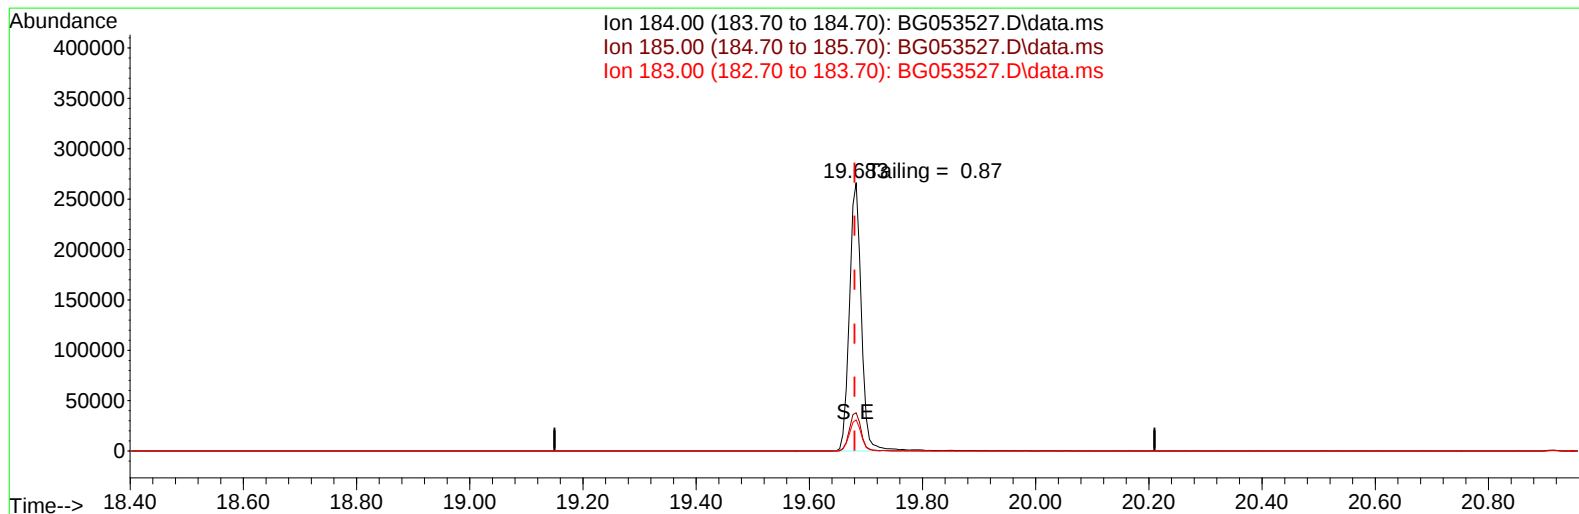

TIC: BG053527.D\data.ms

(77) Benzidine

19.683min (+ 0.003) 0.00 ng

response 389000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.24
183.00	11.10	11.67
0.00	0.00	0.00