
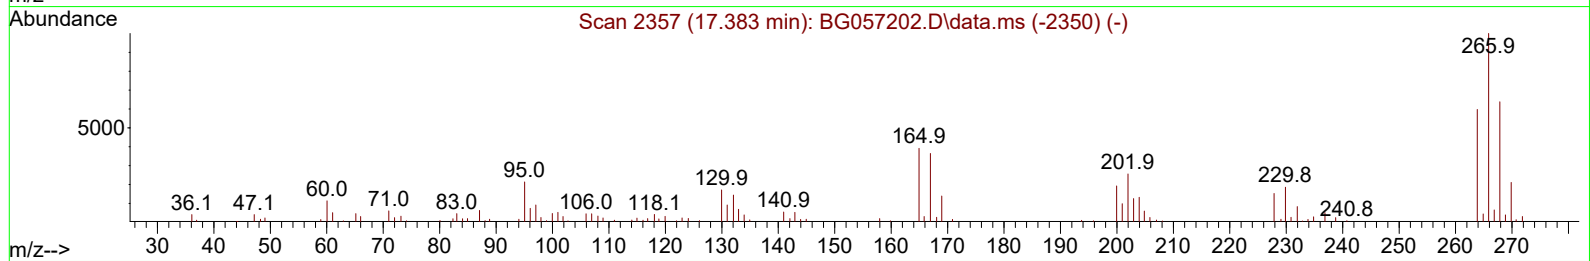
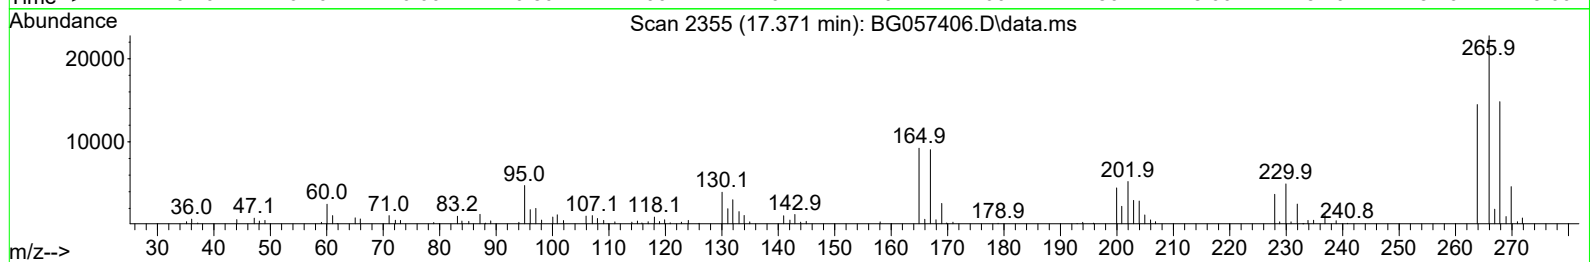


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
Data File : BG057406.D
Acq On : 12 May 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:04:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

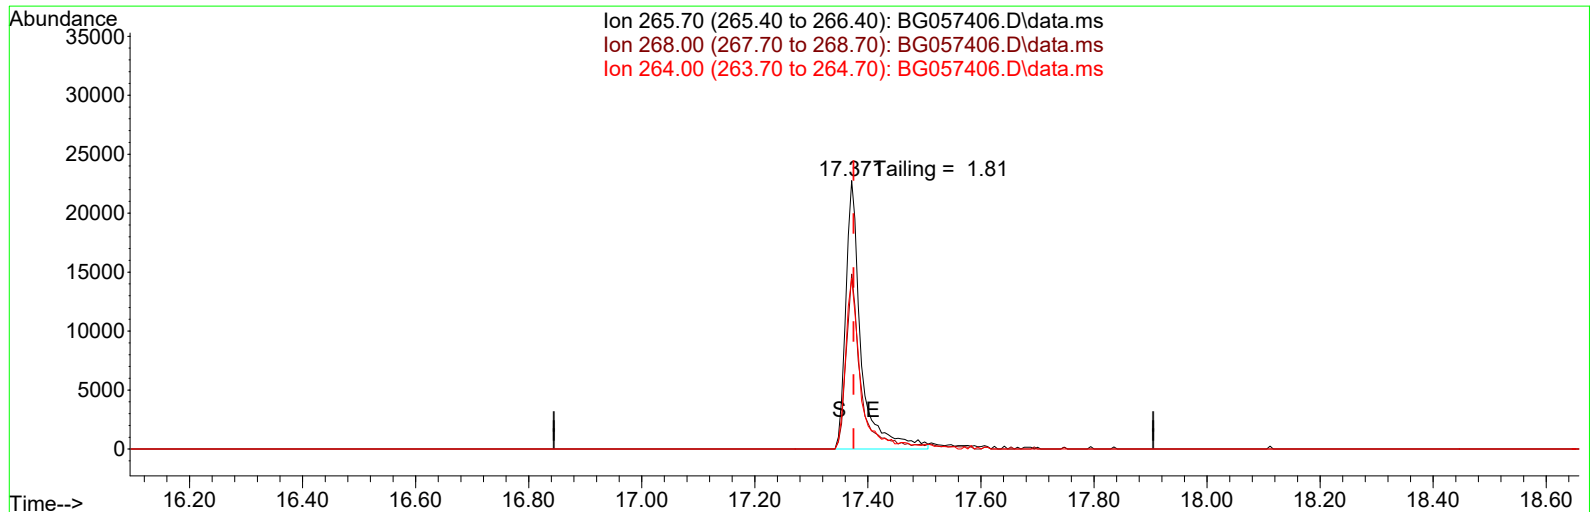

TIC: BG057406.D\data.ms

(70) Pentachlorophenol (C)




17.371min (-0.004) 47979.14 ng

response 42315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.16
264.00	59.70	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
 Data File : BG057406.D
 Acq On : 12 May 2023 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:04:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 12 22:04:03 2023
 Response via : Initial Calibration

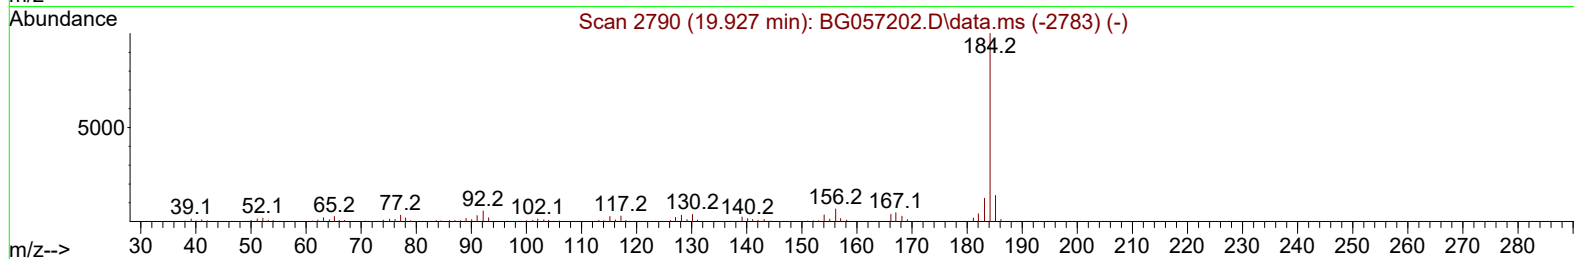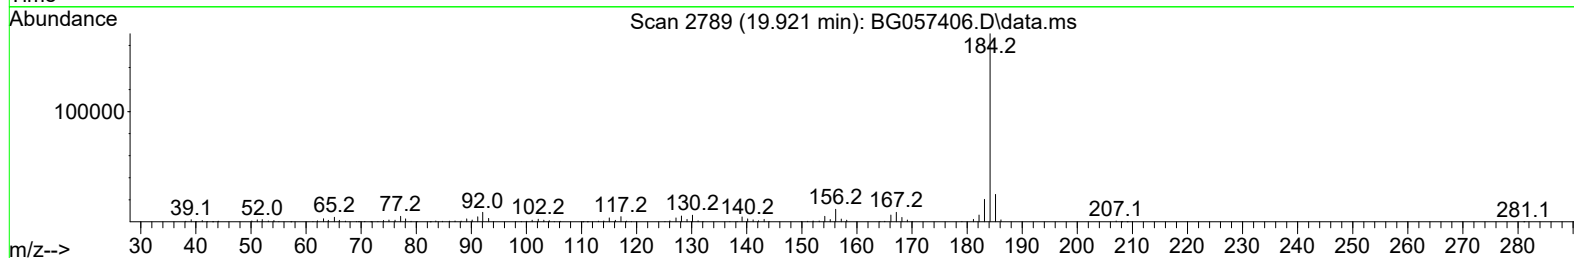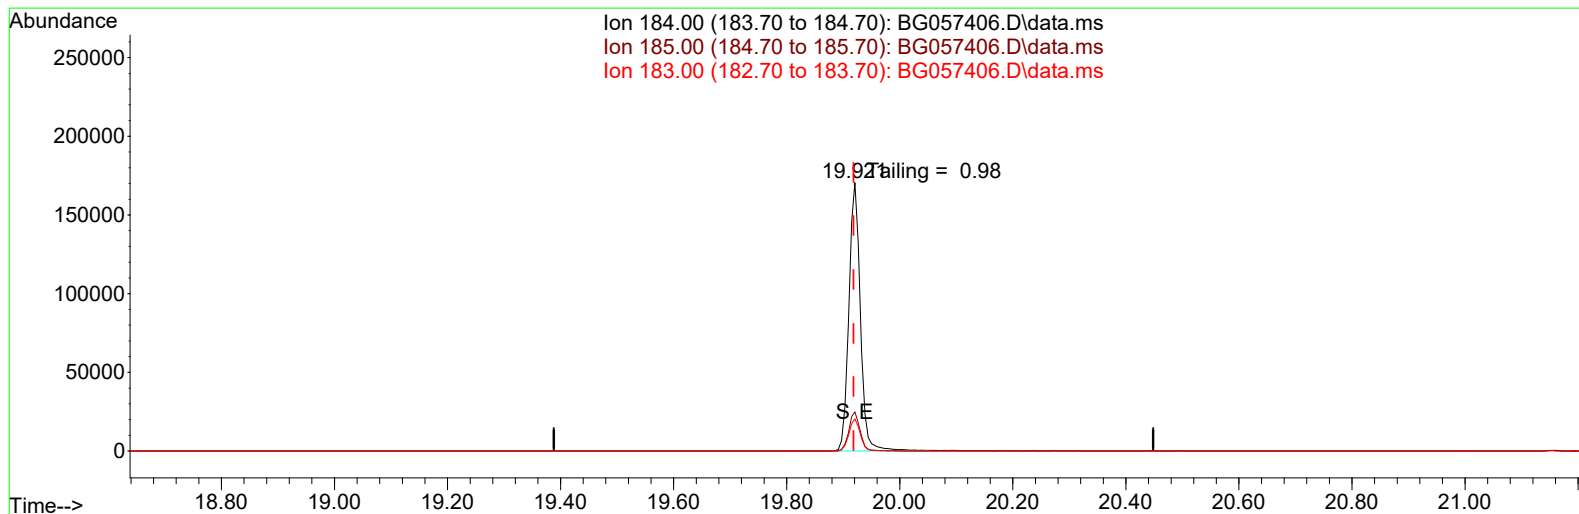

TIC: BG057406.D\data.ms

(77) Benzidine

19.921min (+ 0.002) 0.00 ng

response 242021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.62
183.00	12.40	12.00
0.00	0.00	0.00