
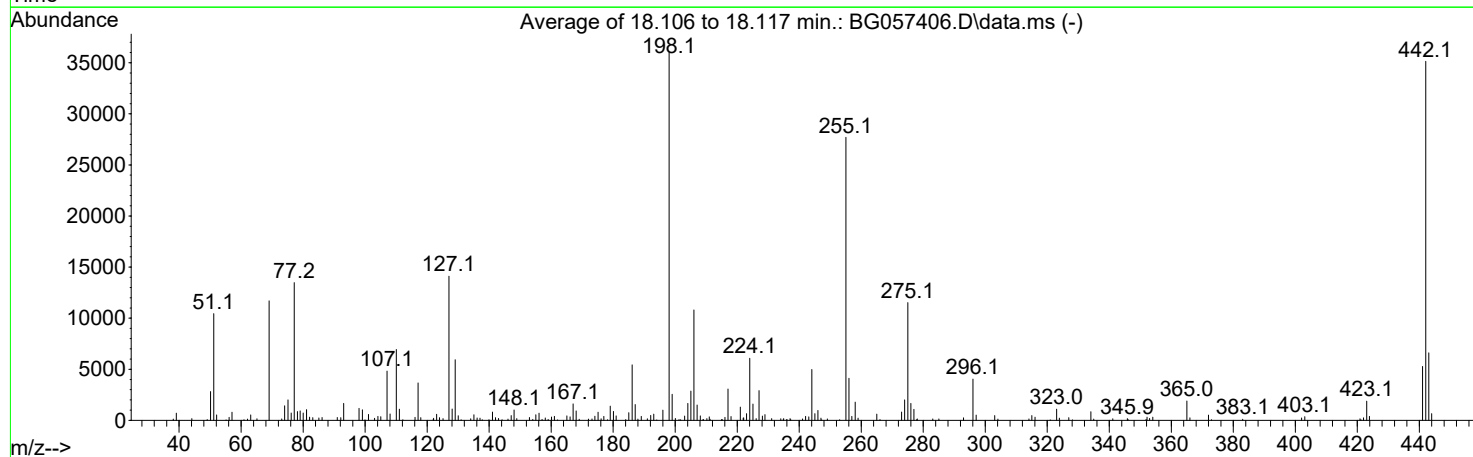


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
Data File : BG057406.D
Acq On : 12 May 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 12 22:04:03 2023

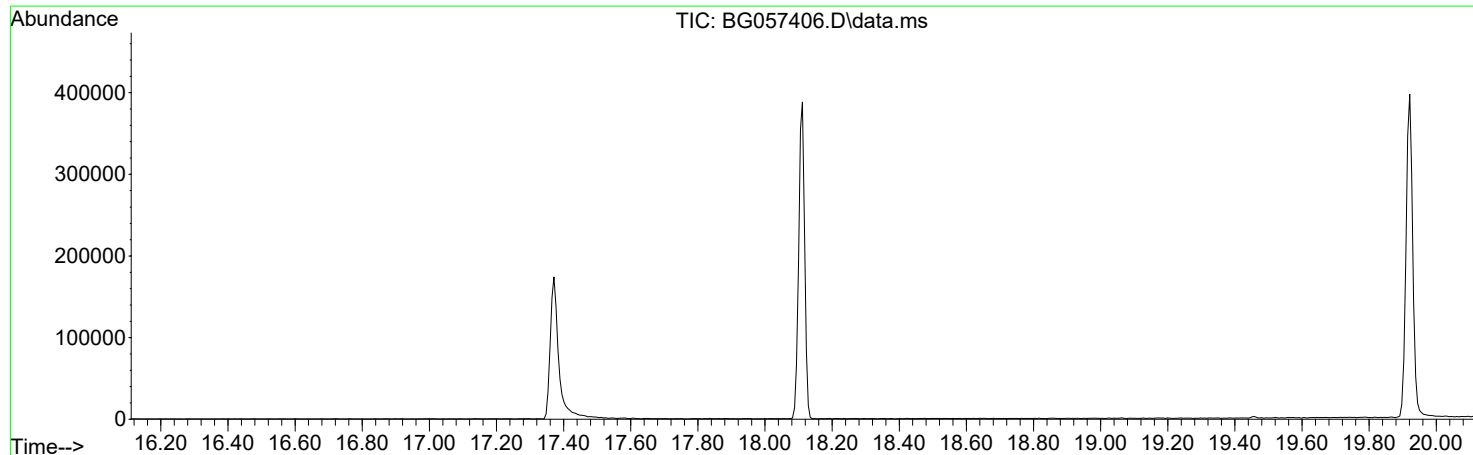

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	10440	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.5	11693	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.2	14109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36005	PASS
199	198	5	9	7.1	2560	PASS
275	198	10	60	32.0	11521	PASS
365	198	1	100	5.3	1899	PASS
441	198	0.01	100	14.7	5275	PASS
442	442	50	100	100.0	35141	PASS
443	442	15	24	18.8	6610	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2023	BNA_G	BG057406.D
Compound Name	Response	Retention Time
DDT	122629	21.154
DDD	1711	20.749
DDE	0	20.193
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1711	124340	1.38

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
Data File : BG057406.D
Acq On : 12 May 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 04:04:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

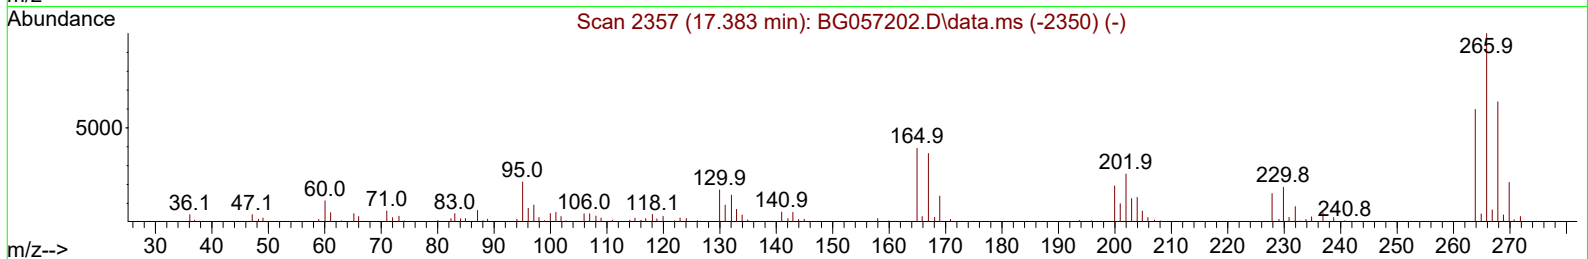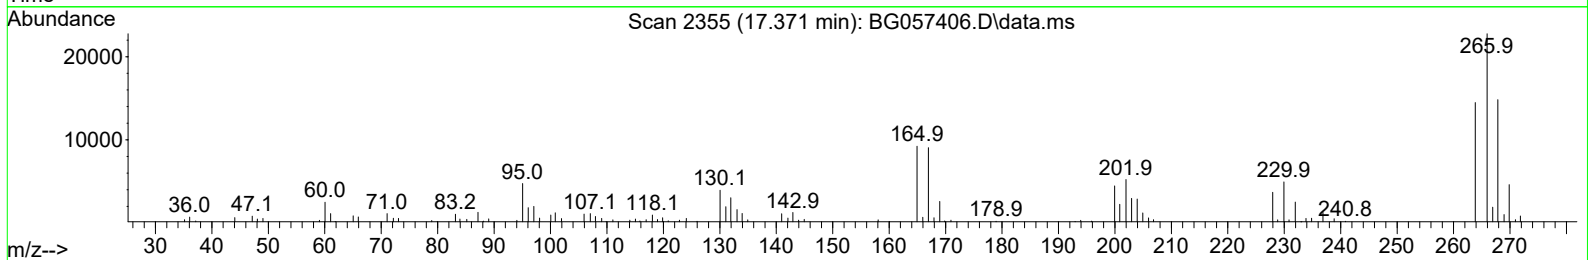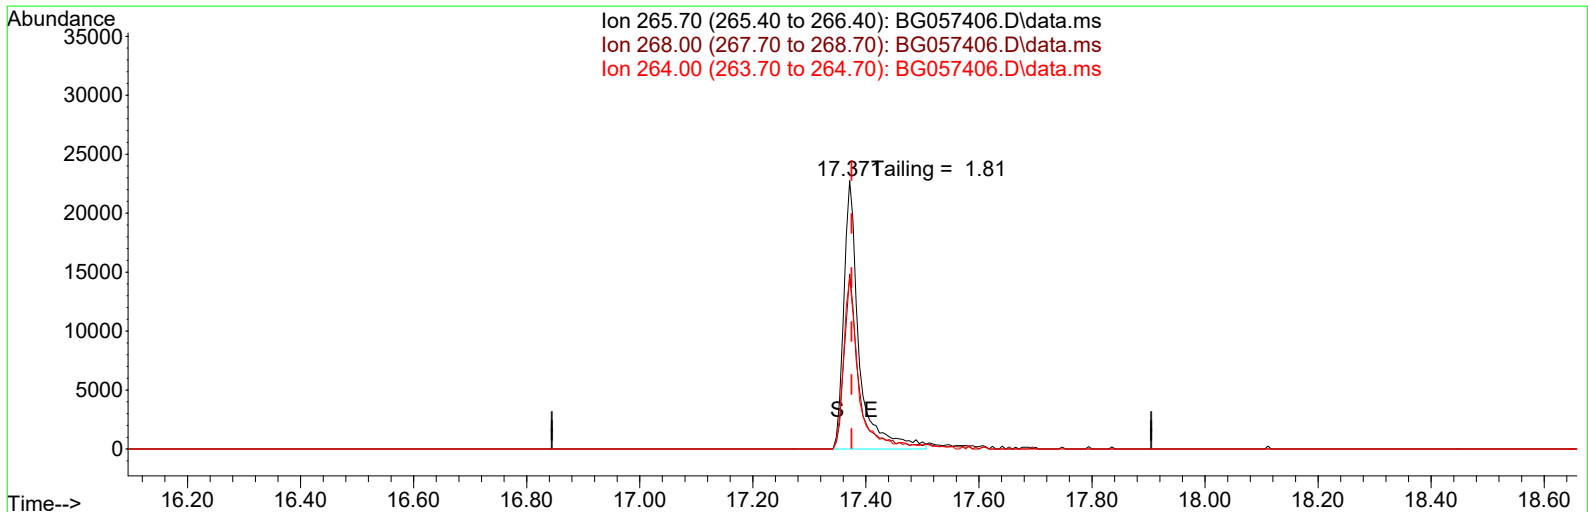

TIC: BG057406.D\data.ms

(70) Pentachlorophenol (C)

17.371min (-0.004) 47979.14 ng




response 42315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.16
264.00	59.70	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
 Data File : BG057406.D
 Acq On : 12 May 2023 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 13 04:04:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 12 22:04:03 2023
 Response via : Initial Calibration

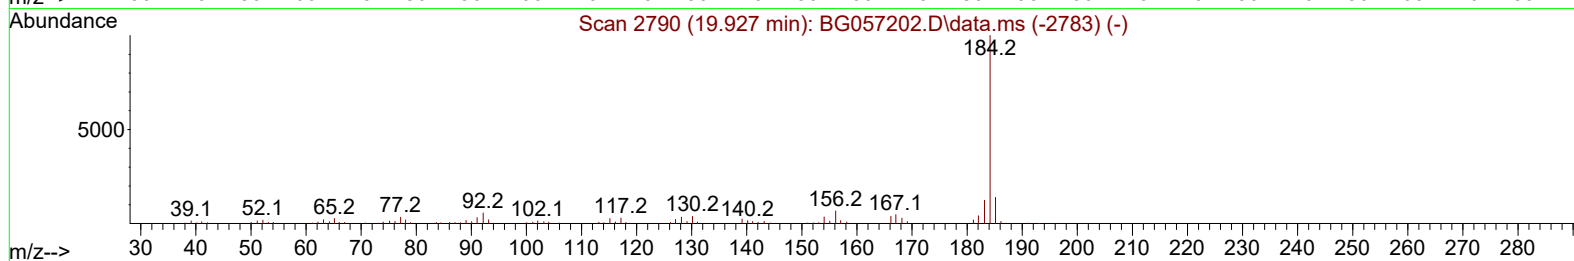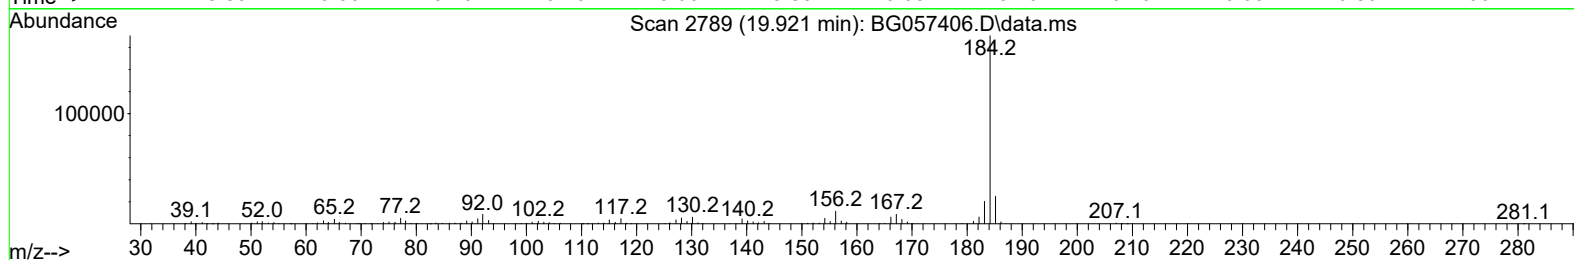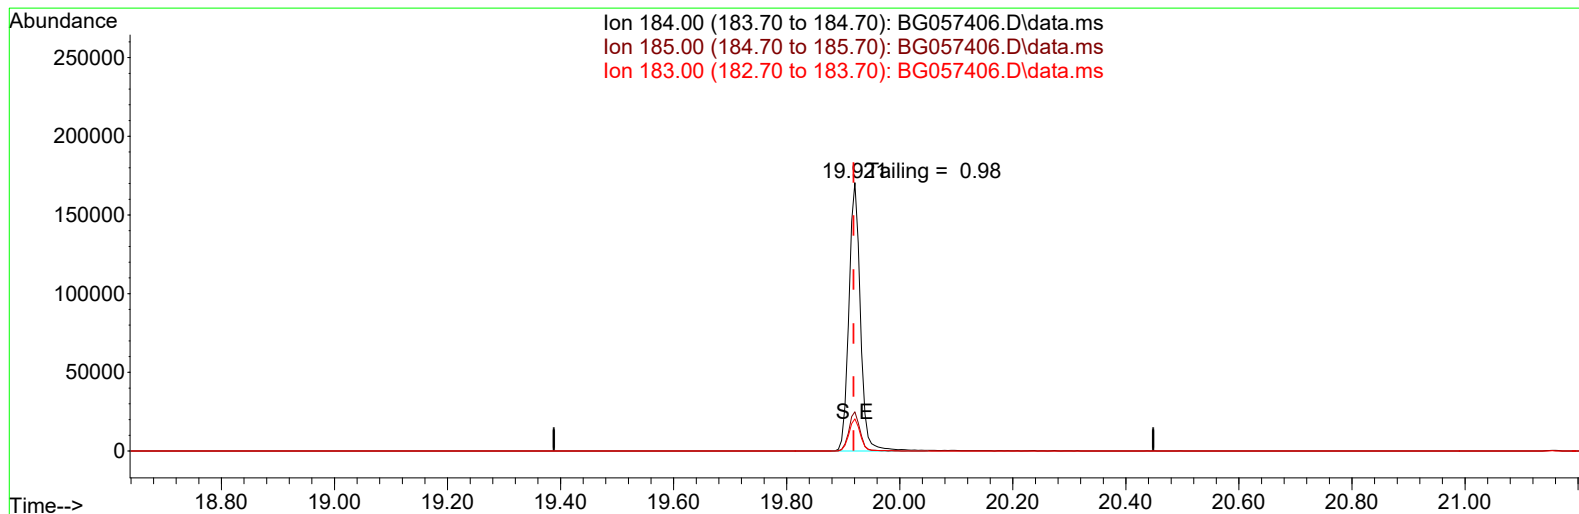

TIC: BG057406.D\data.ms

(77) Benzidine

19.921min (+ 0.002) 0.00 ng

response 242021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.62
183.00	12.40	12.00
0.00	0.00	0.00