
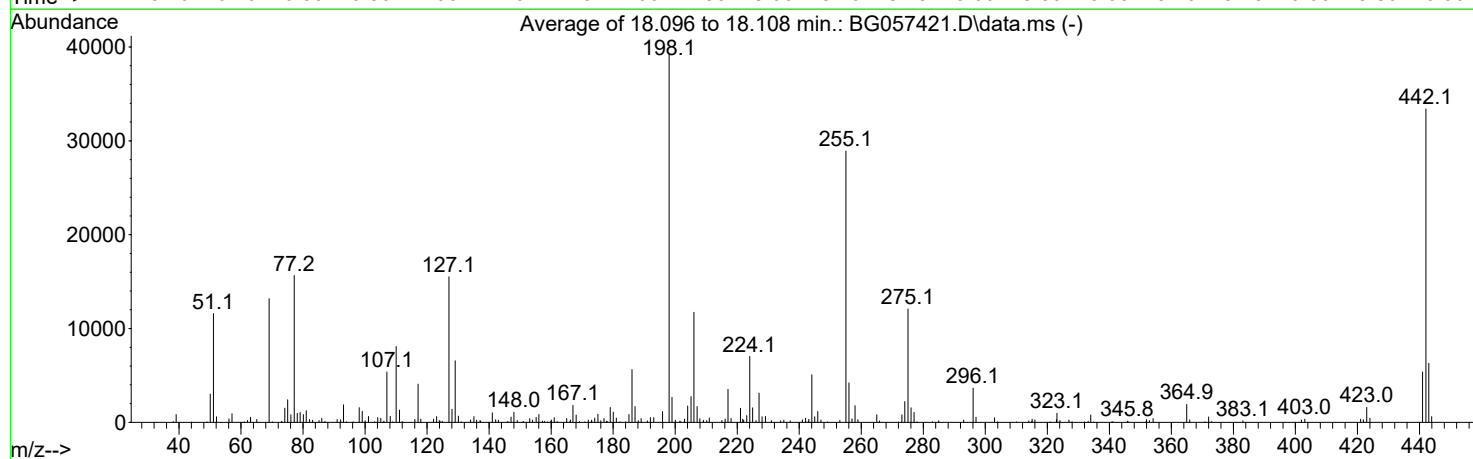


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
Data File : BG057421.D
Acq On : 12 May 2023 23:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 12 22:04:03 2023

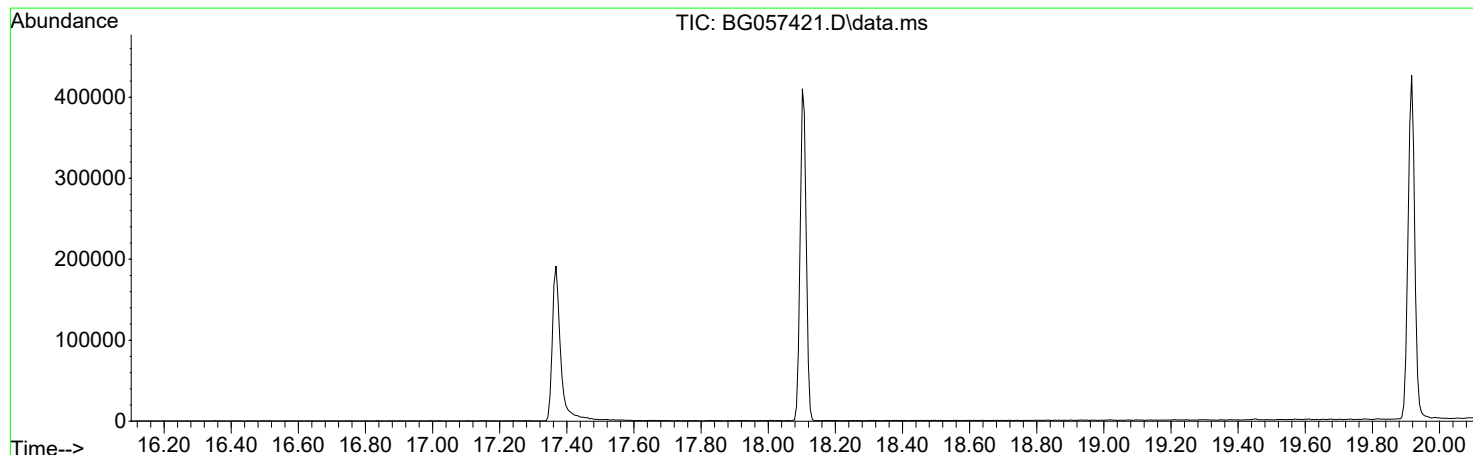

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	11595	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.6	13176	PASS
70	69	0.00	2	0.4	51	PASS
127	198	10	80	39.6	15513	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39203	PASS
199	198	5	9	6.8	2665	PASS
275	198	10	60	30.8	12084	PASS
365	198	1	100	4.9	1917	PASS
441	198	0.01	100	13.7	5371	PASS
442	442	50	100	100.0	33411	PASS
443	442	15	24	18.8	6290	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2023	BNA_G	BG057421.D
Compound Name	Response	Retention Time
DDT	133037	21.151
DDD	3561	20.692
DDE	194	20.193
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3755	136792	2.75

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
Data File : BG057421.D
Acq On : 12 May 2023 23:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 04:06:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

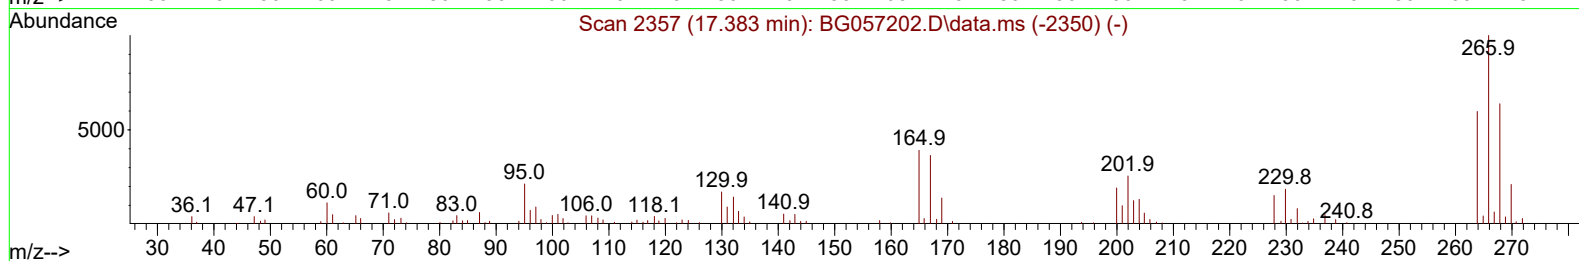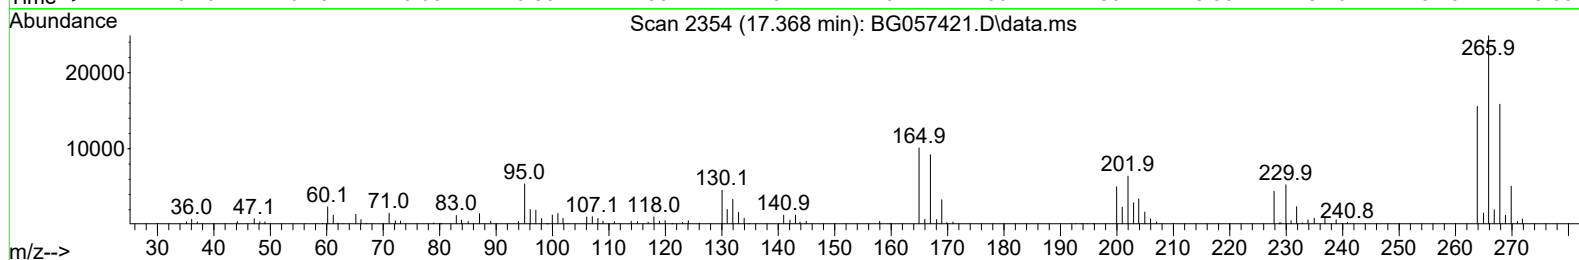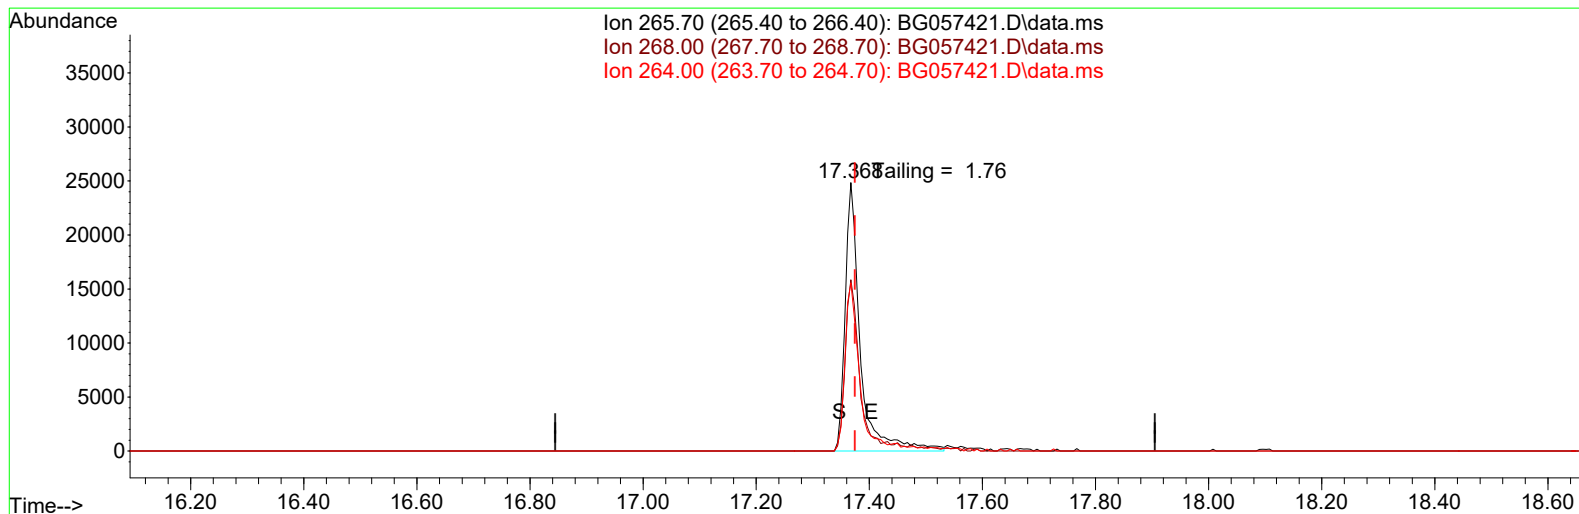

TIC: BG057421.D\data.ms

(70) Pentachlorophenol (C)

17.368min (-0.007) 27024.52 ng




response 46375

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.77
264.00	59.70	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051223\
Data File : BG057421.D
Acq On : 12 May 2023 23:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 04:06:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

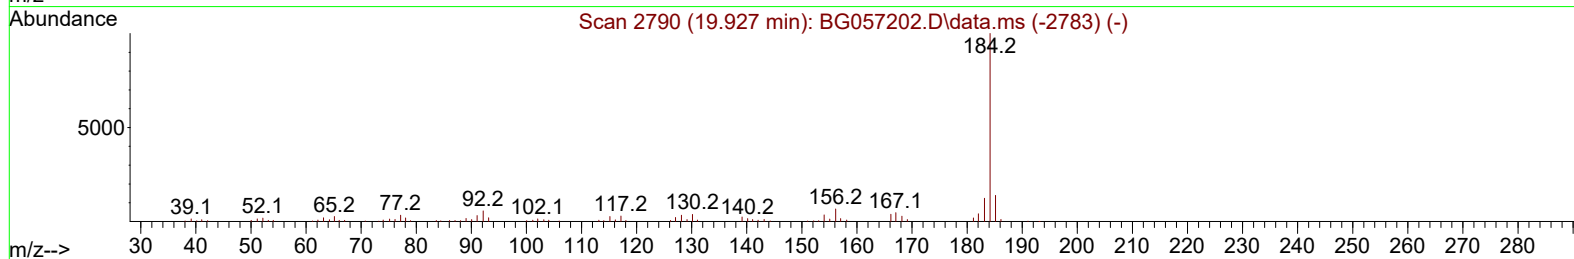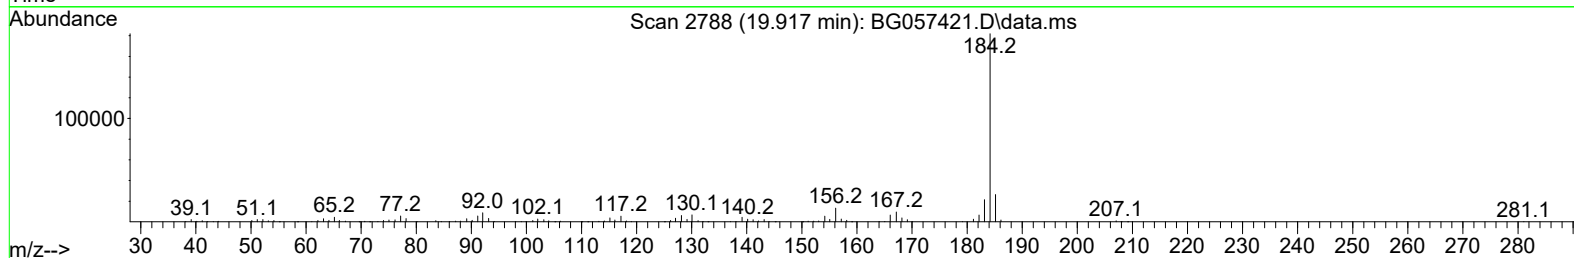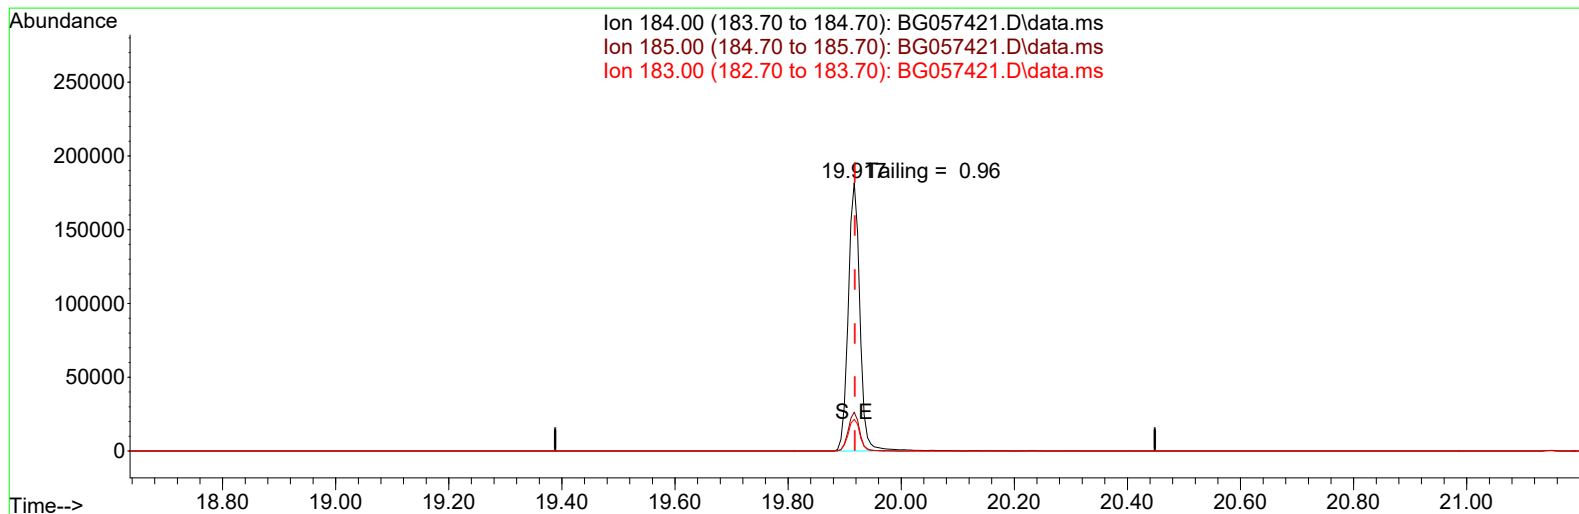

TIC: BG057421.D\data.ms

(77) Benzidine

19.917min (-0.001) 0.00 ng

response 260047

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.52
183.00	12.40	11.84
0.00	0.00	0.00