


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051315\
 Data File : BG017118.D
 Acq On : 13 May 2015 22:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

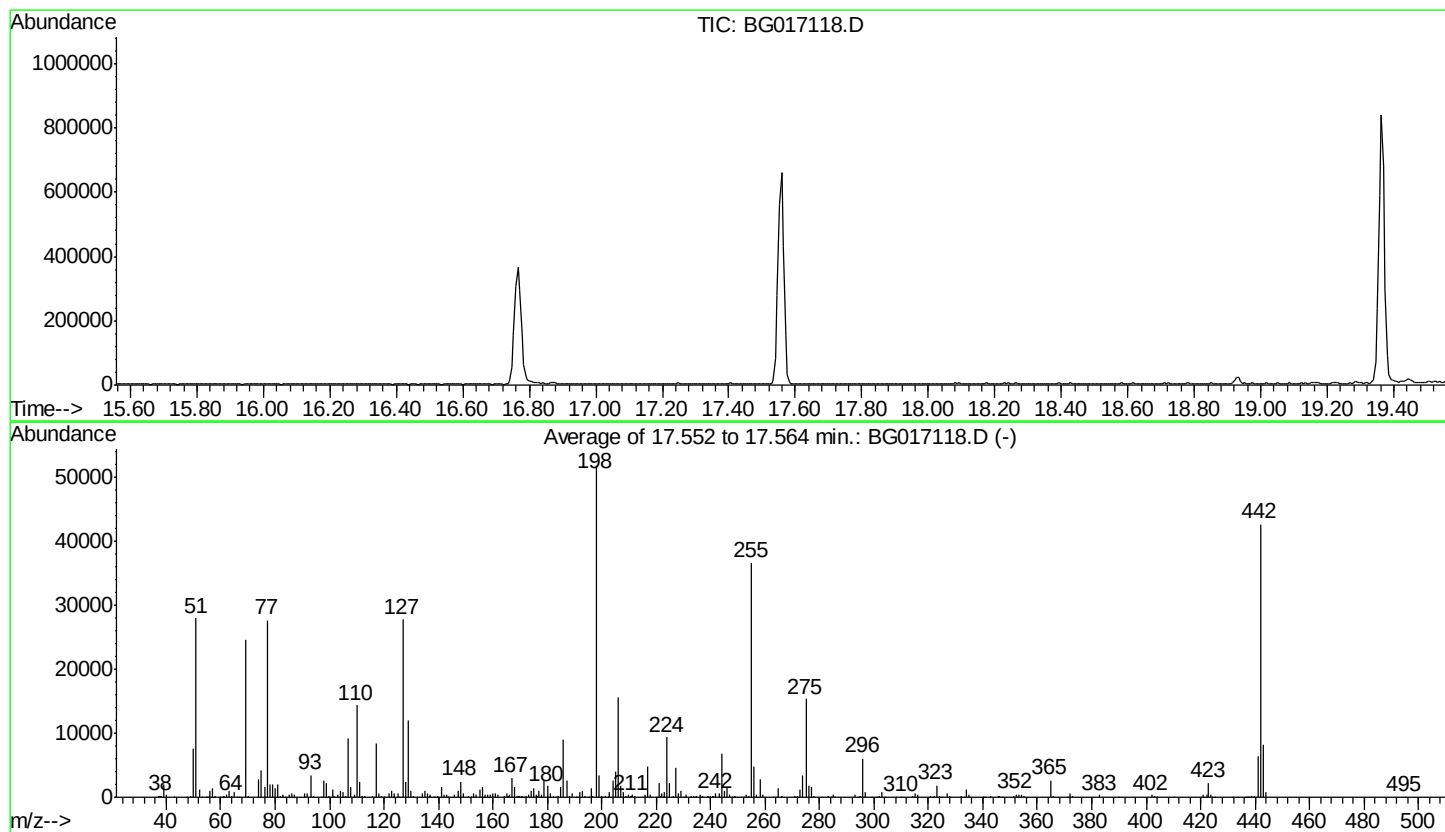

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.9	27909	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.6	24637	PASS
70	69	0.00	2	0.8	189	PASS
127	198	10	80	53.6	27738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51736	PASS
199	198	5	9	6.5	3362	PASS
275	198	10	60	29.6	15305	PASS
365	198	1	100	5.2	2699	PASS
441	442	0.01	24	15.2	6486	PASS
442	198	50	100	82.3	42586	PASS
443	442	15	24	19.1	8117	PASS