
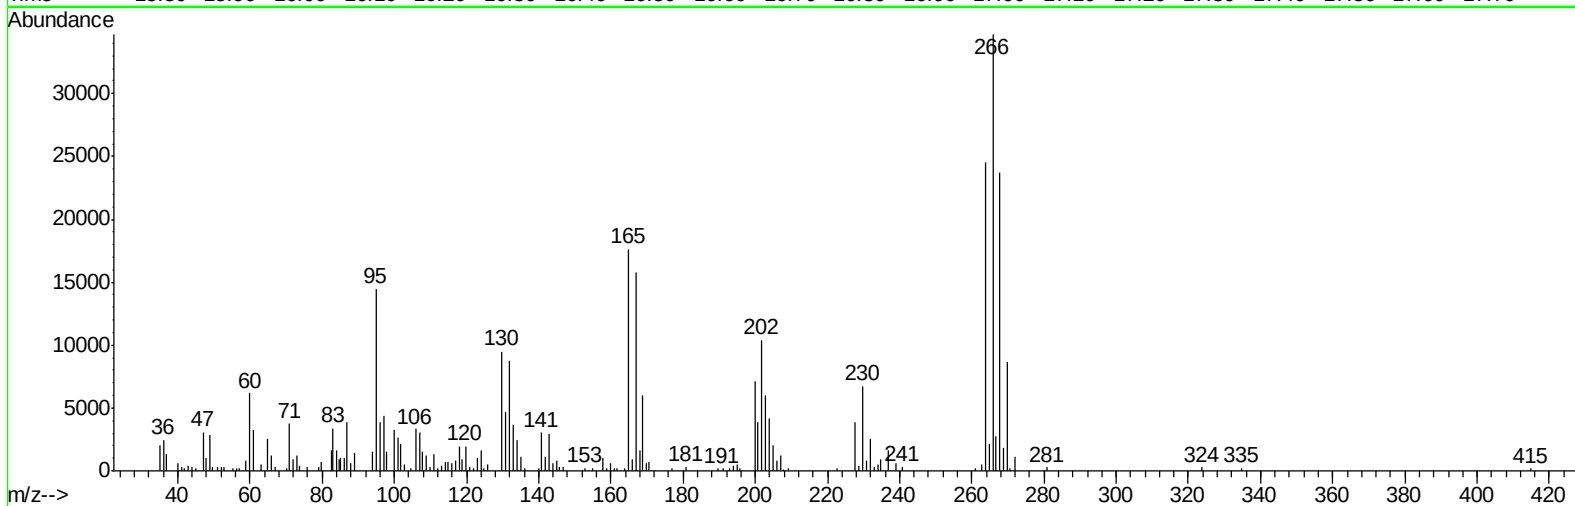


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051315\
Data File : BG017100.D
Acq On : 13 May 2015 11:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:43:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 03:58:31 2015
Response via : Initial Calibration

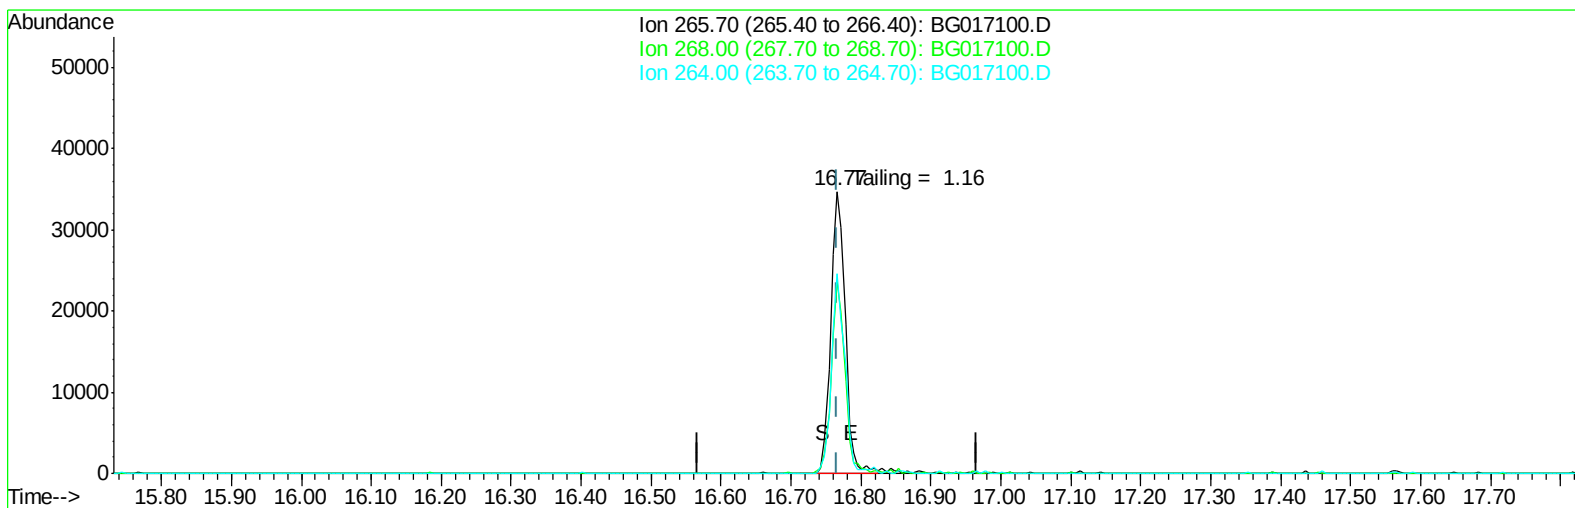

TIC: BG017100.D

(69) Pentachlorophenol (C)



16.766min (-0.000) 12865.06ng

response 49172

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	68.30
264.00	61.70	70.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051315\
Data File : BG017100.D
Acq On : 13 May 2015 11:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:43:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 03:58:31 2015
Response via : Initial Calibration

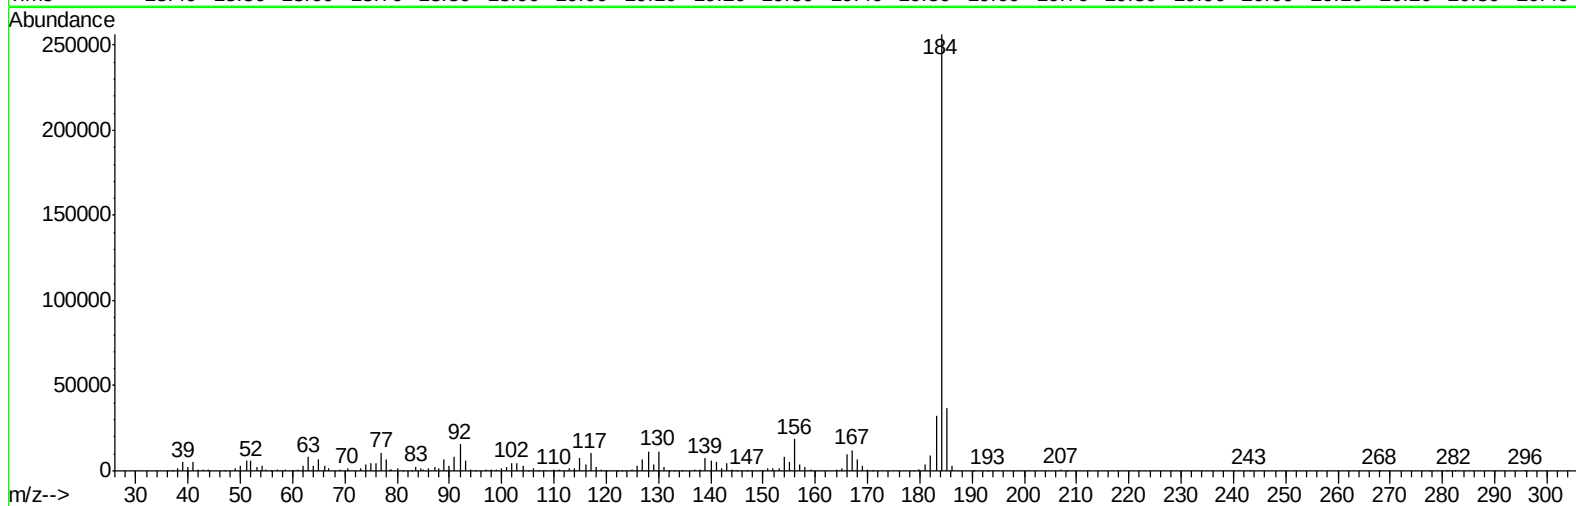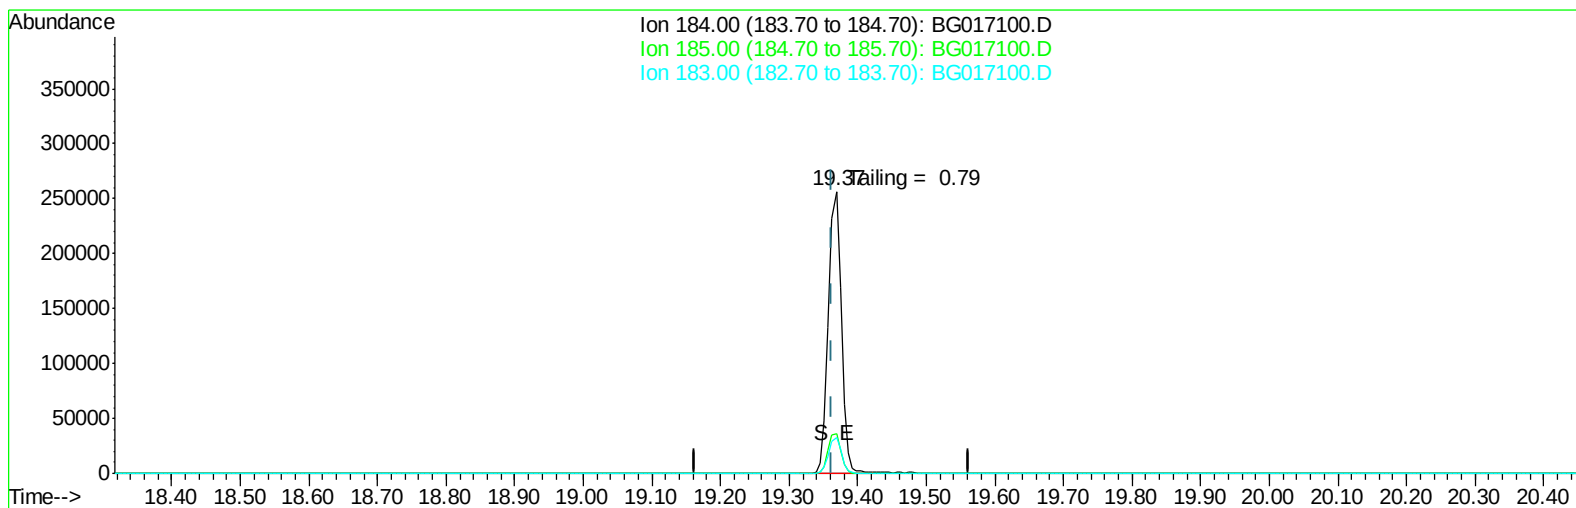

TIC: BG017100.D

(76) Benzidine

19.369min (+0.005) 189525.48ng

response 334150

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.33
183.00	14.30	12.66
0.00	0.00	0.00