
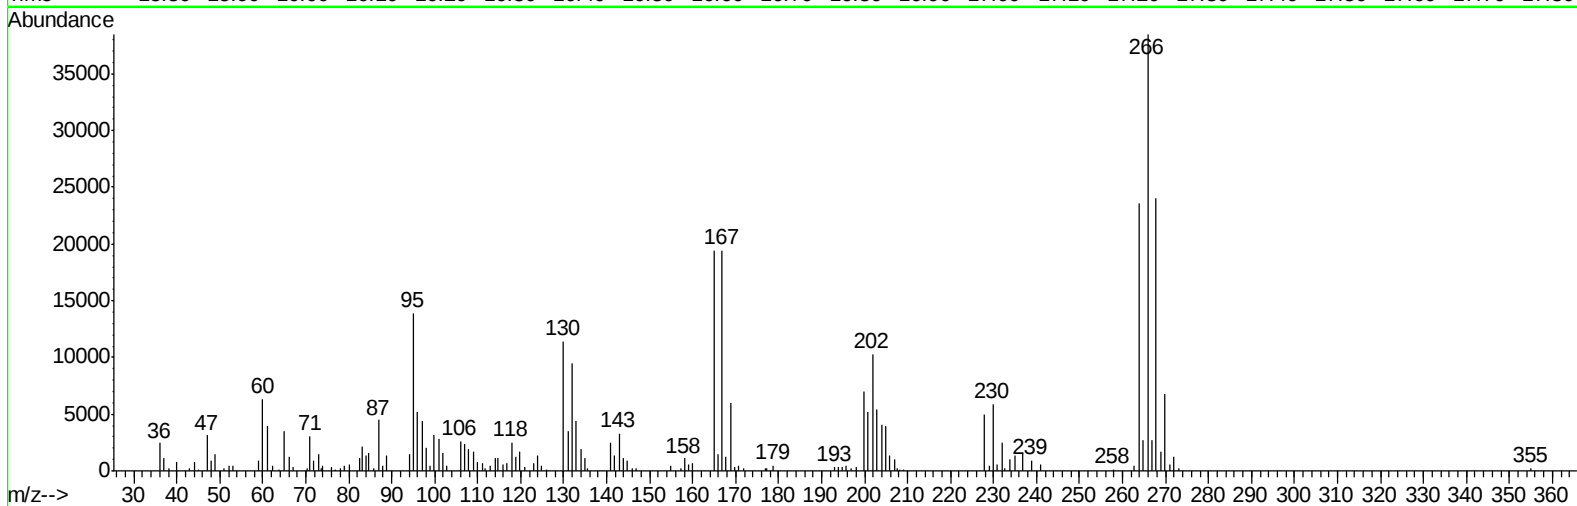


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051315\
Data File : BG017118.D
Acq On : 13 May 2015 22:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:44:25 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 03:58:31 2015
Response via : Initial Calibration

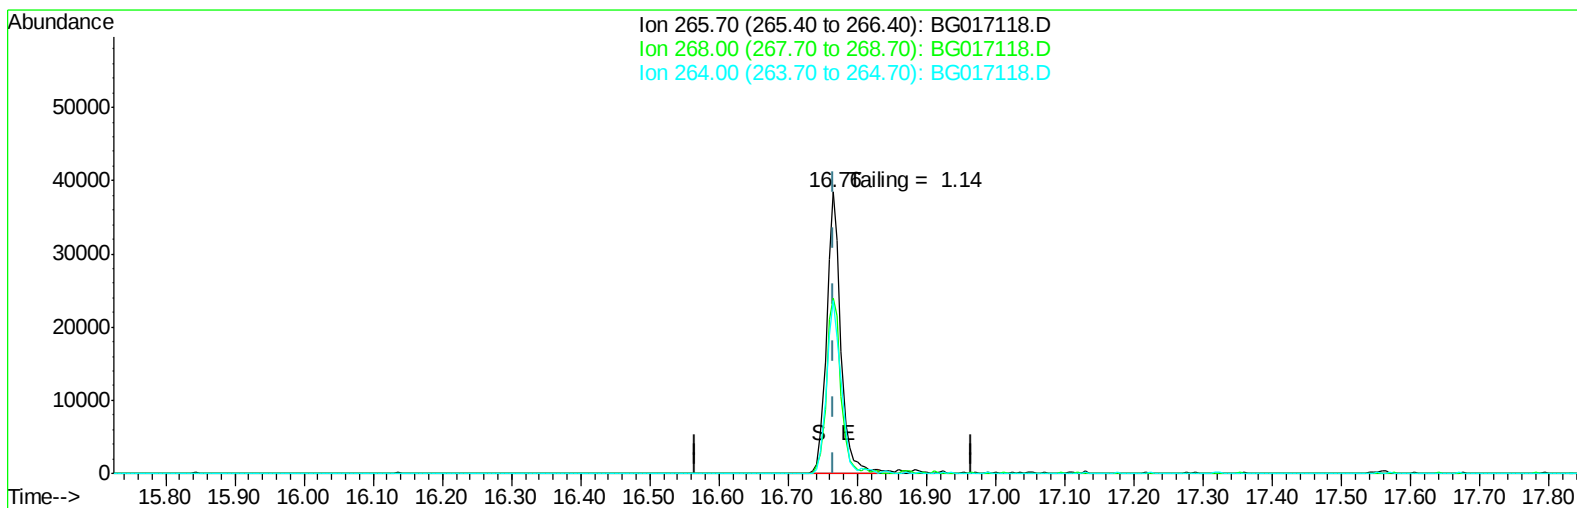

TIC: BG017118.D

(69) Pentachlorophenol (C)



16.765min (-0.001) 18591.76ng

response 54898

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	62.43
264.00	61.70	61.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051315\
Data File : BG017118.D
Acq On : 13 May 2015 22:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:44:25 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 03:58:31 2015
Response via : Initial Calibration

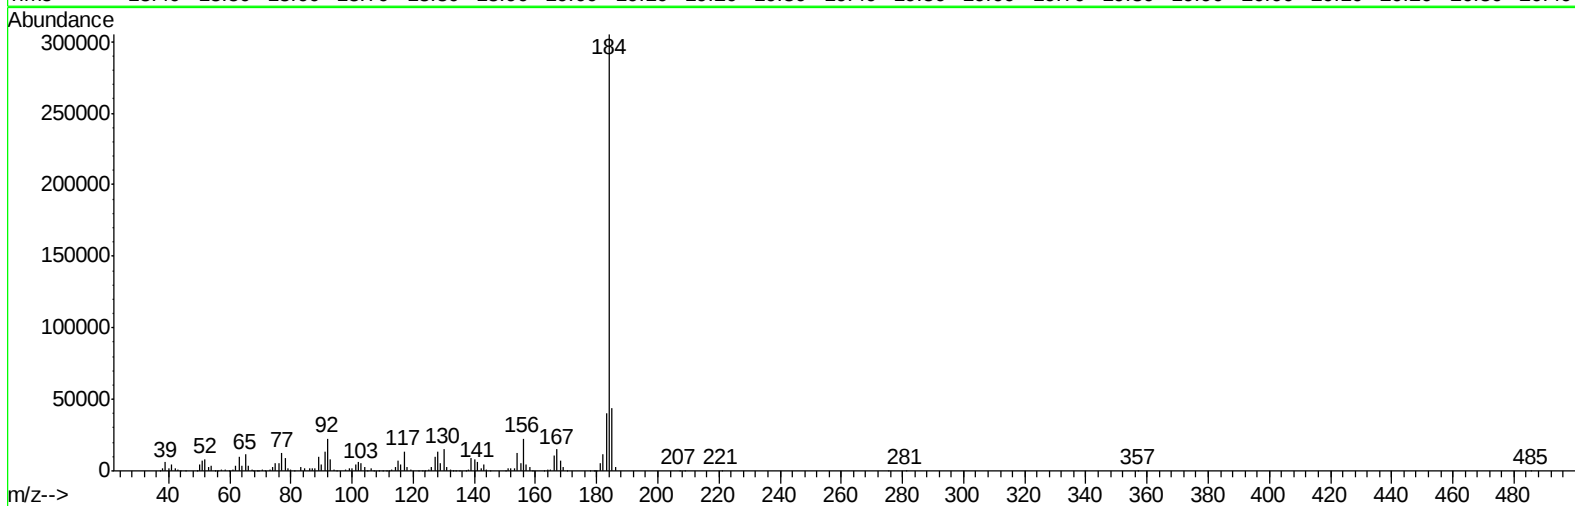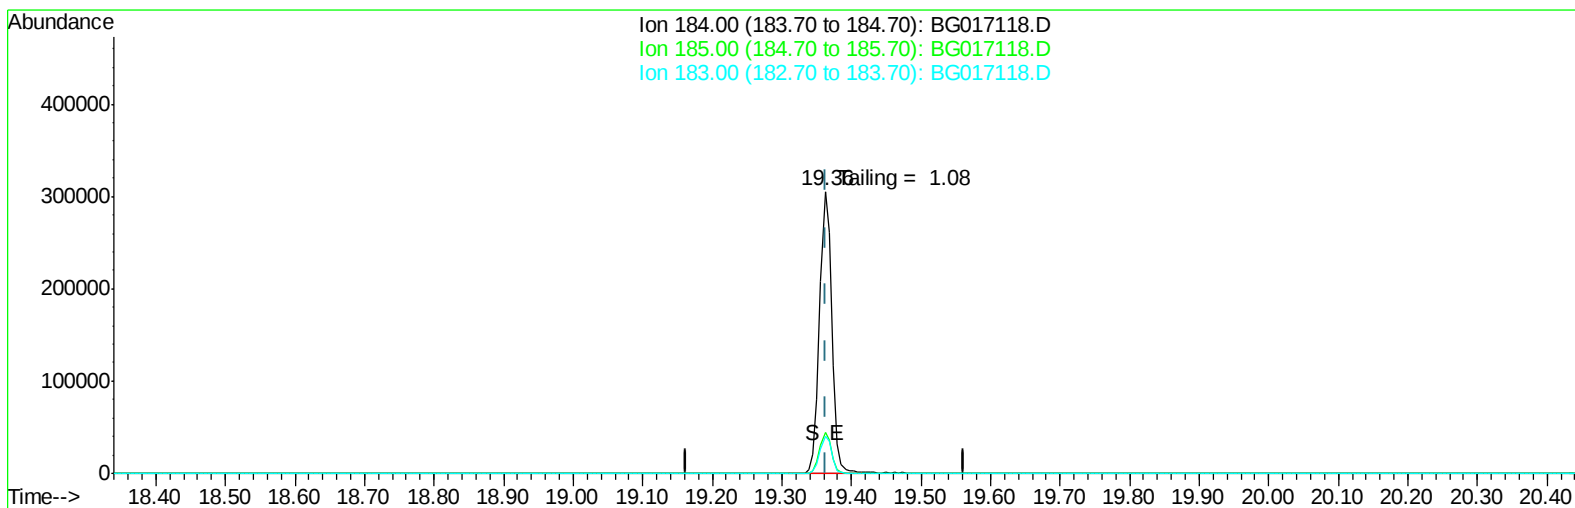

TIC: BG017118.D

(76) Benzidine

19.362min (-0.001) 110034.71ng

response 366446

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.39
183.00	14.30	13.07
0.00	0.00	0.00