


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051315\
 Data File : BG017100.D
 Acq On : 13 May 2015 11:07
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

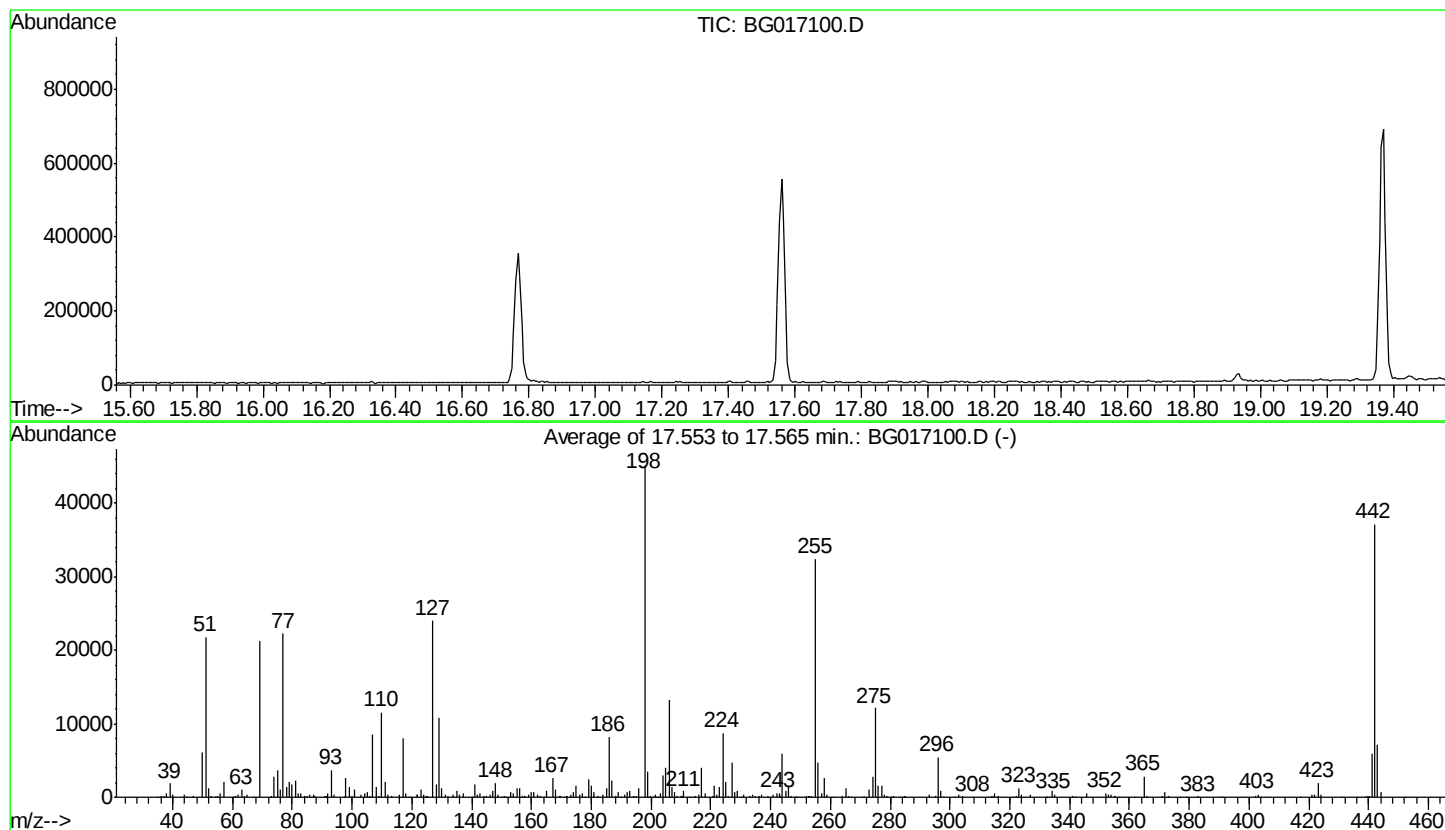

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	21841	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.2	21312	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	23968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45122	PASS
199	198	5	9	7.9	3565	PASS
275	198	10	60	27.0	12177	PASS
365	198	1	100	6.3	2824	PASS
441	442	0.01	24	15.8	5878	PASS
442	198	50	100	82.3	37146	PASS
443	442	15	24	19.4	7195	PASS