


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG051319\
 Data File : BG040910.D
 Acq On : 13 May 2019 14:22
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

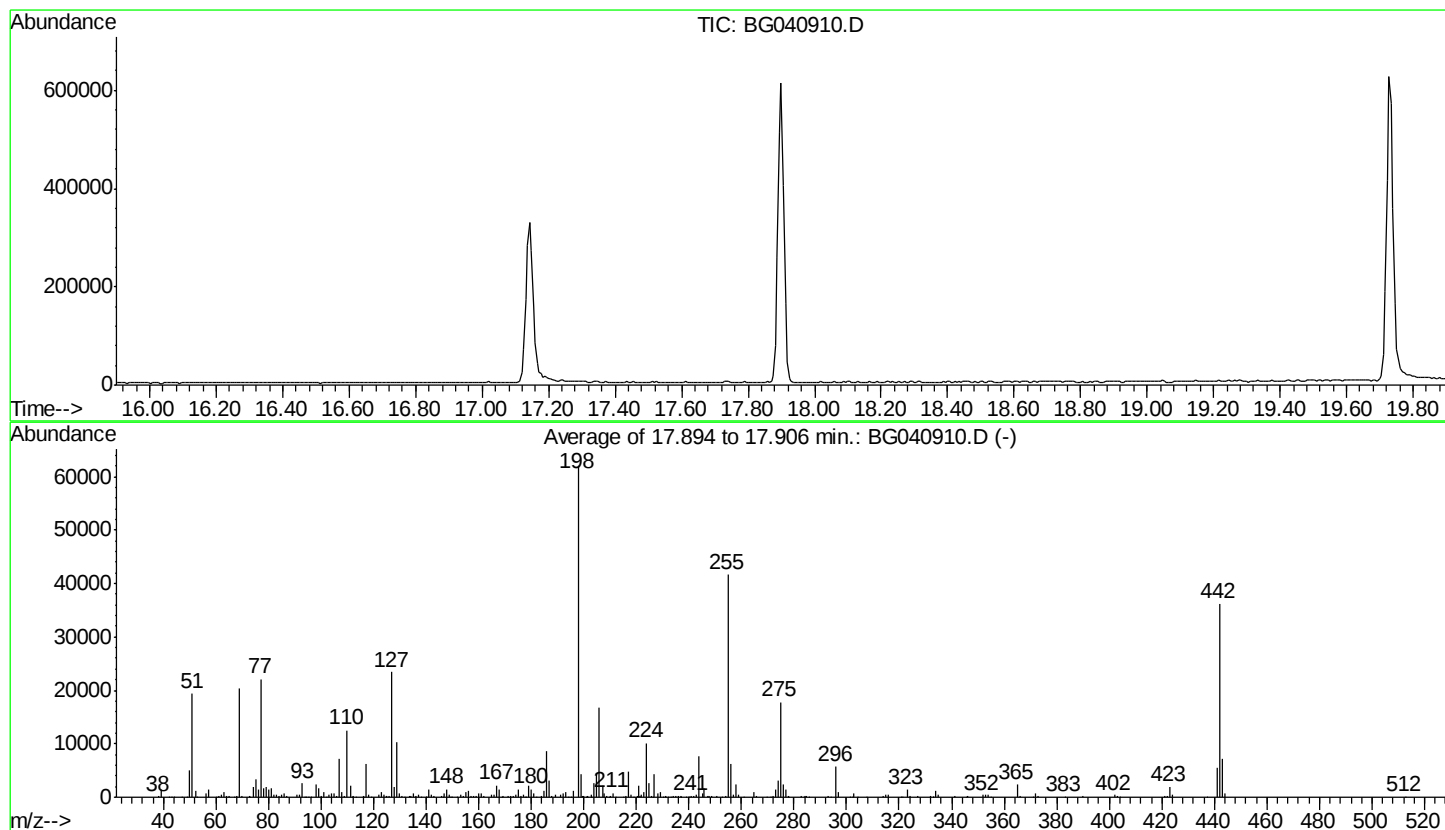

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	19330	PASS
68	69	0.00	2	0.9	180	PASS
69	198	0.00	100	32.8	20337	PASS
70	69	0.00	2	1.0	210	PASS
127	198	10	80	37.8	23456	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62053	PASS
199	198	5	9	7.1	4408	PASS
275	198	10	60	28.7	17806	PASS
365	198	1	100	3.7	2303	PASS
441	198	0.01	100	8.7	5399	PASS
442	198	50	100	58.5	36282	PASS
443	442	15	24	19.8	7179	PASS