


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG051319\
 Data File : BG040926.D
 Acq On : 14 May 2019 1:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

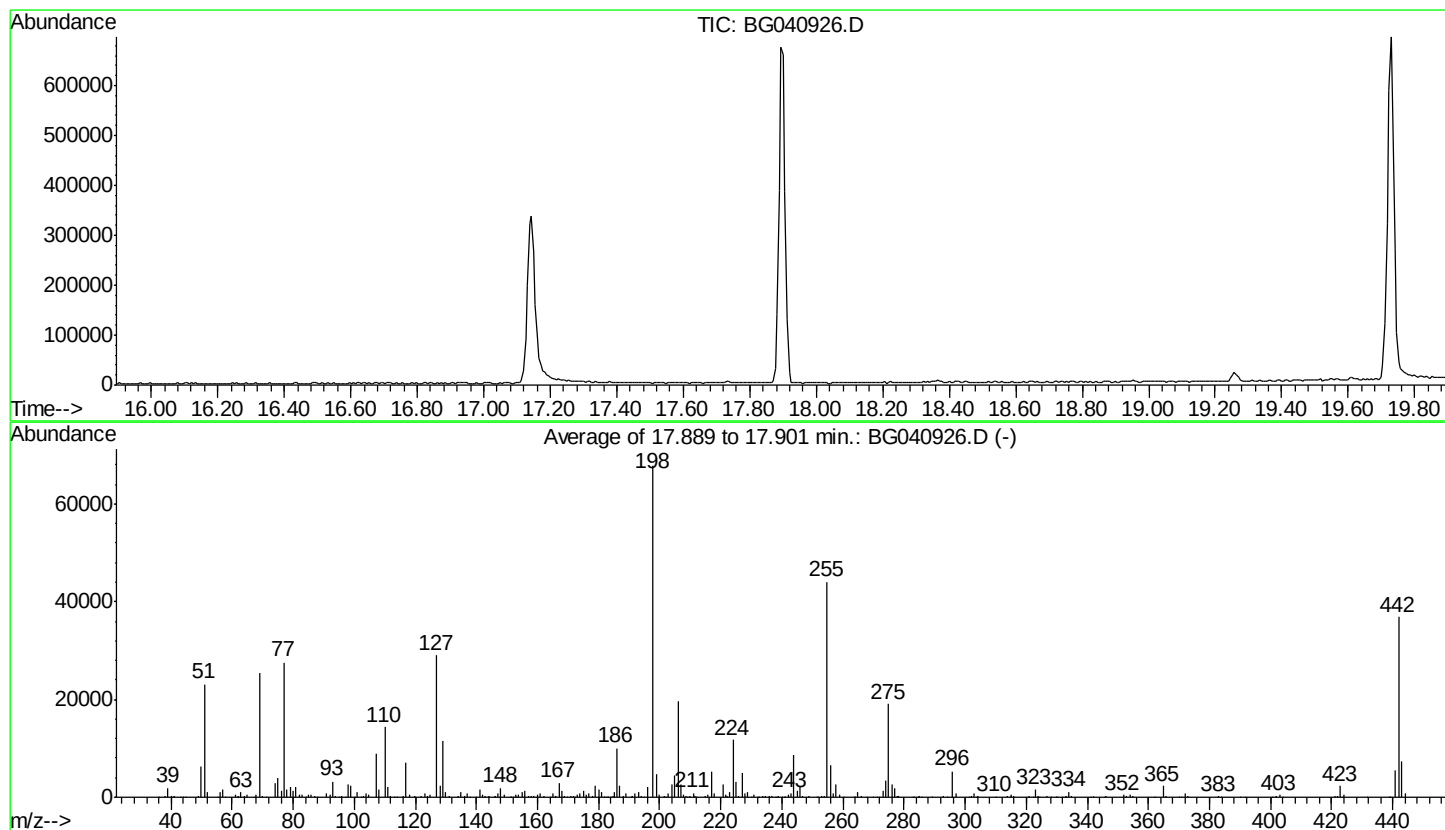

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	23120	PASS
68	69	0.00	2	1.9	491	PASS
69	198	0.00	100	37.3	25290	PASS
70	69	0.00	2	0.6	148	PASS
127	198	10	80	42.8	29056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67842	PASS
199	198	5	9	7.0	4745	PASS
275	198	10	60	28.1	19038	PASS
365	198	1	100	3.4	2333	PASS
441	198	0.01	100	8.3	5598	PASS
442	198	50	100	54.4	36914	PASS
443	442	15	24	19.7	7280	PASS