
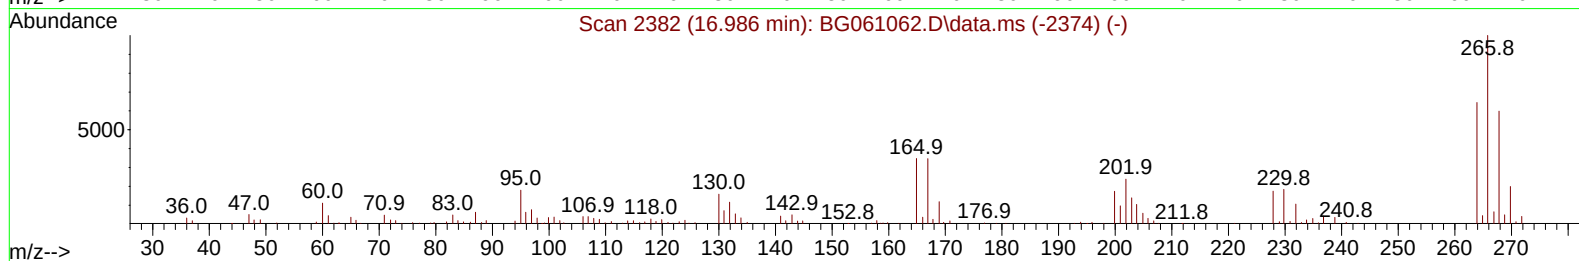
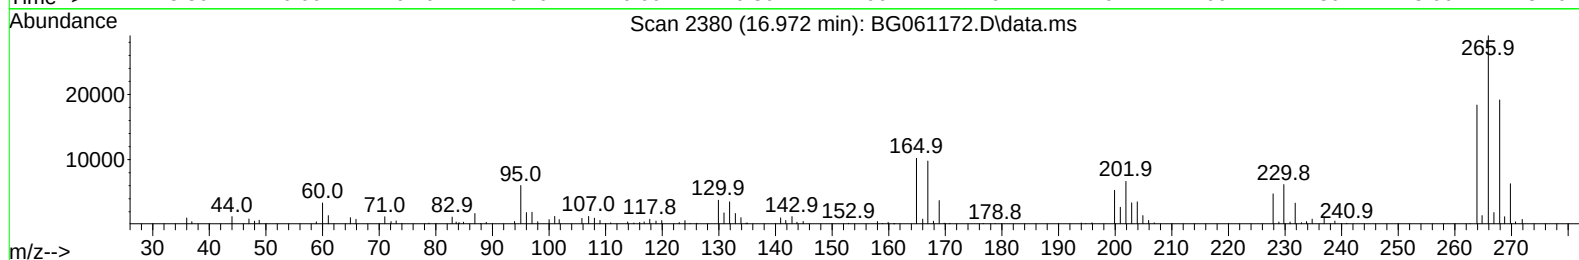


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051324\
Data File : BG061172.D
Acq On : 13 May 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 10:42:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

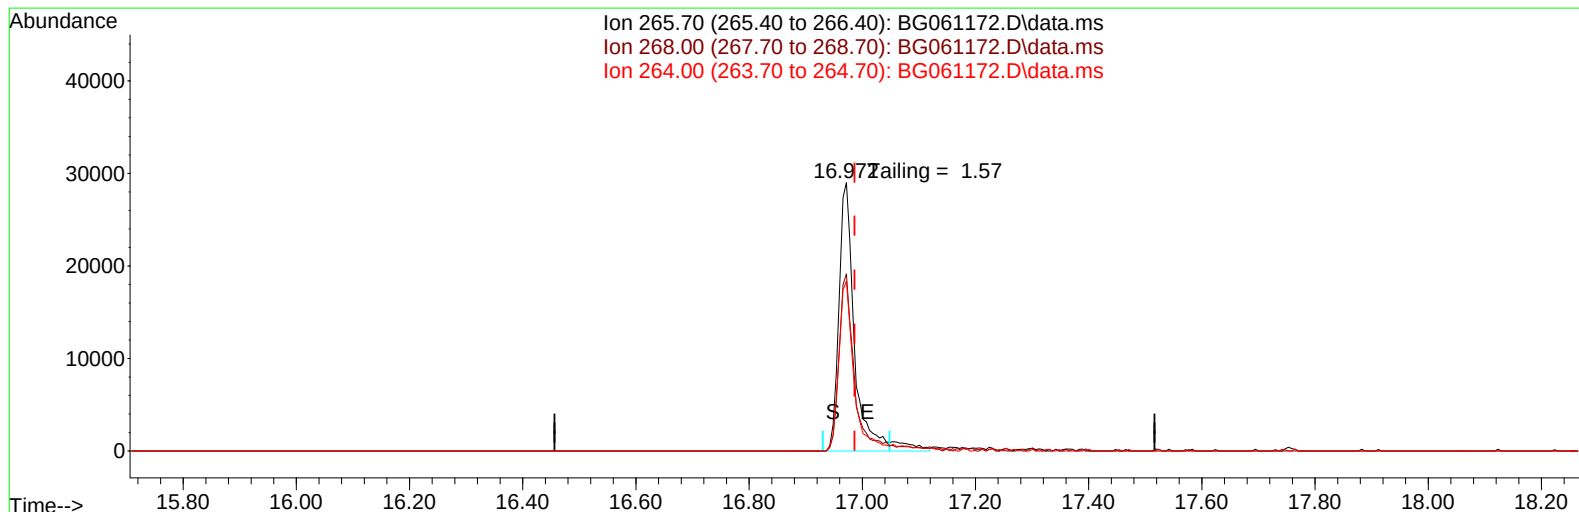

TIC: BG061172.D\data.ms

(70) Pentachlorophenol (C)




16.972min (-0.014) 13489.18 ng

response 53949

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	66.02
264.00	64.40	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051324\
Data File : BG061172.D
Acq On : 13 May 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 10:42:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

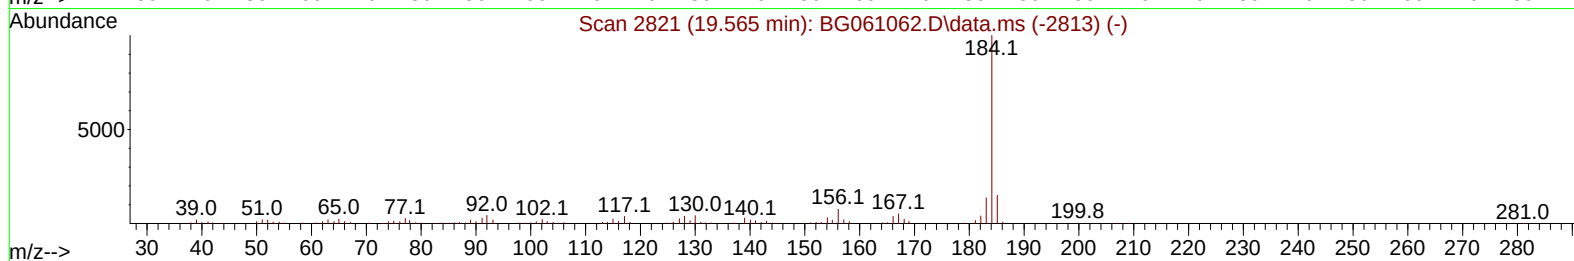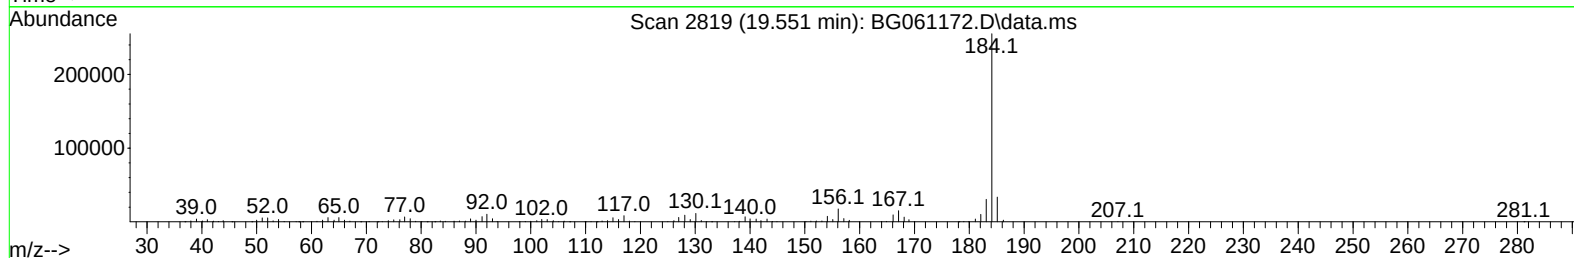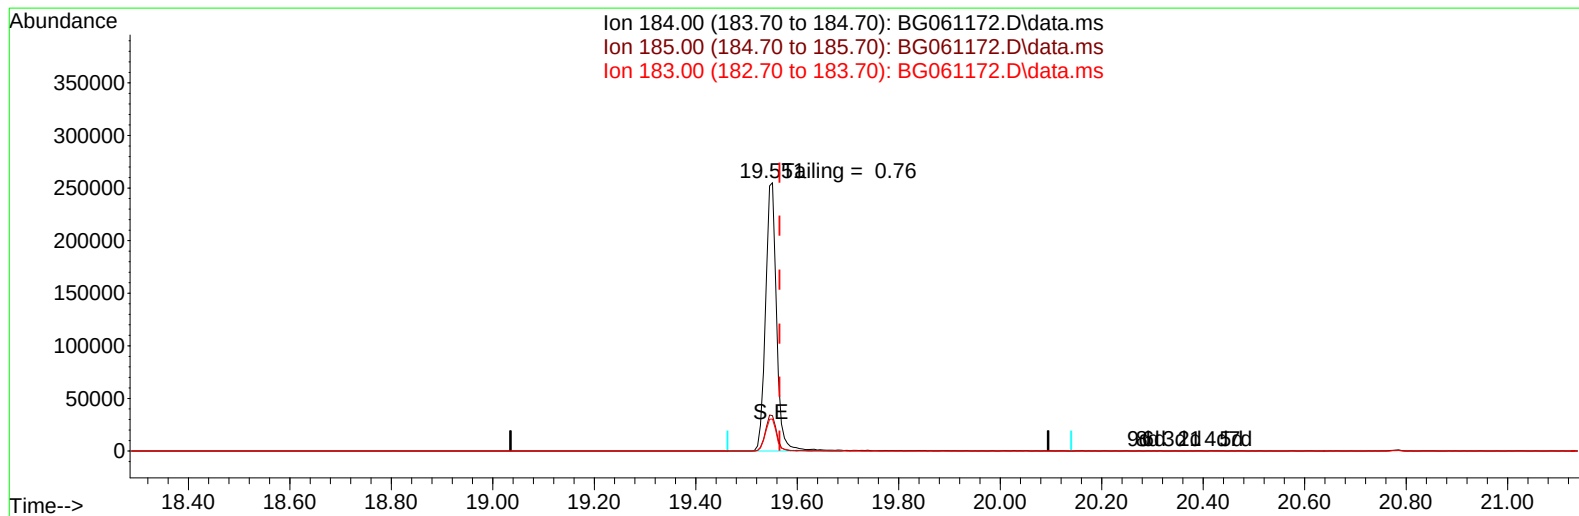

TIC: BG061172.D\data.ms

(77) Benzidine

19.551min (-0.014) 334273.67 ng m

response 384992

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.17
183.00	13.60	11.95
0.00	0.00	0.00