
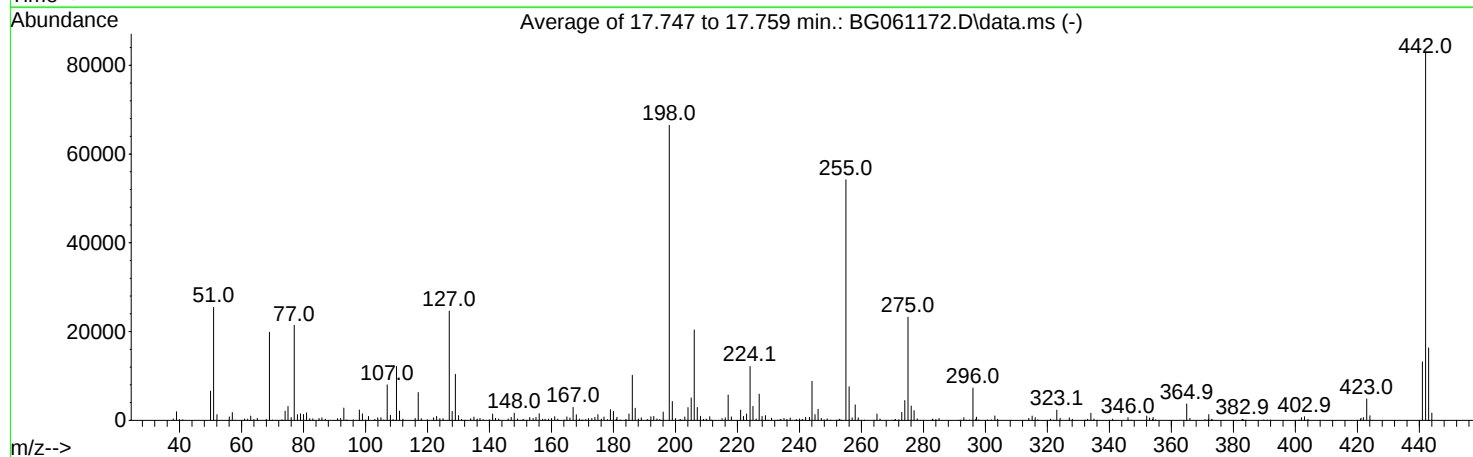


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051324\
Data File : BG061172.D
Acq On : 13 May 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

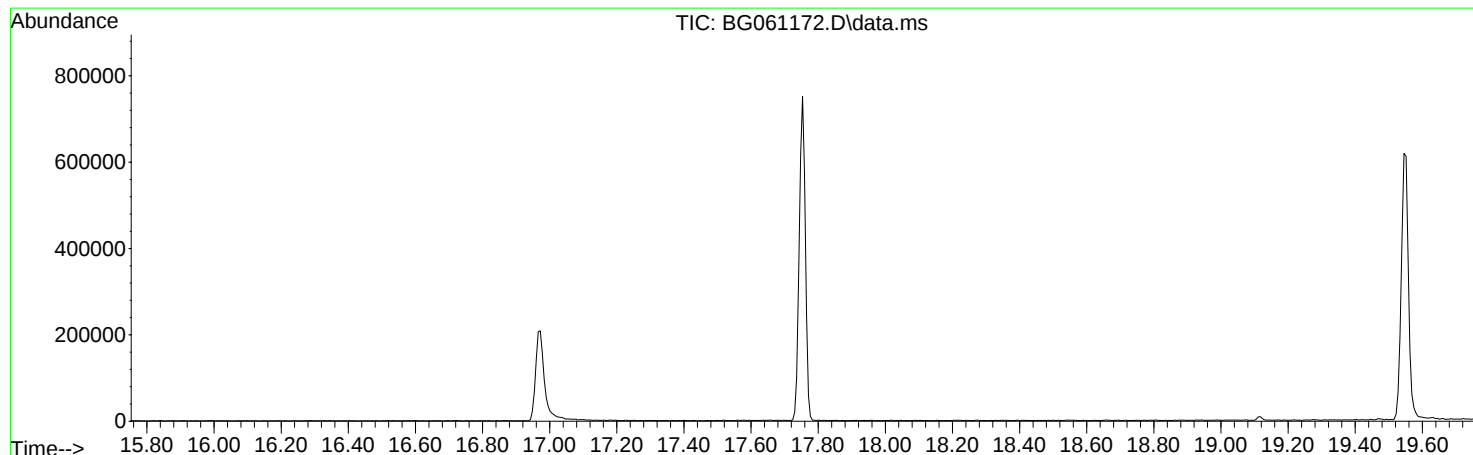

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	25456	PASS
68	69	0.00	2	1.3	268	PASS
69	198	0.00	100	29.9	19856	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	37.0	24627	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66472	PASS
199	198	5	9	6.4	4247	PASS
275	198	10	60	35.0	23253	PASS
365	198	1	100	5.6	3719	PASS
441	198	0.01	100	19.8	13194	PASS
442	442	50	100	100.0	82872	PASS
443	442	15	24	19.7	16332	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2024	BNA_G	<u>BG061172.D</u>
Compound Name	Response	Retention Time
DDT	234060	20.785
DDD	7036	20.338
DDE	715	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7751	241811	3.21

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051324\
Data File : BG061172.D
Acq On : 13 May 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 10:42:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

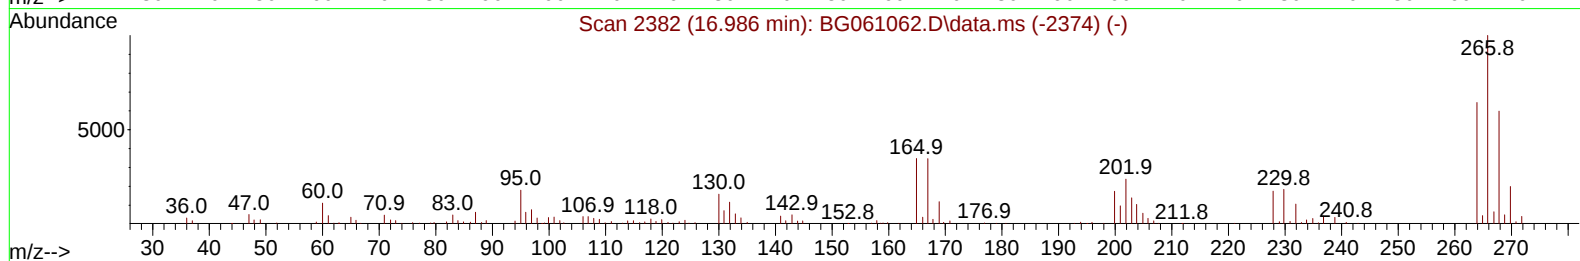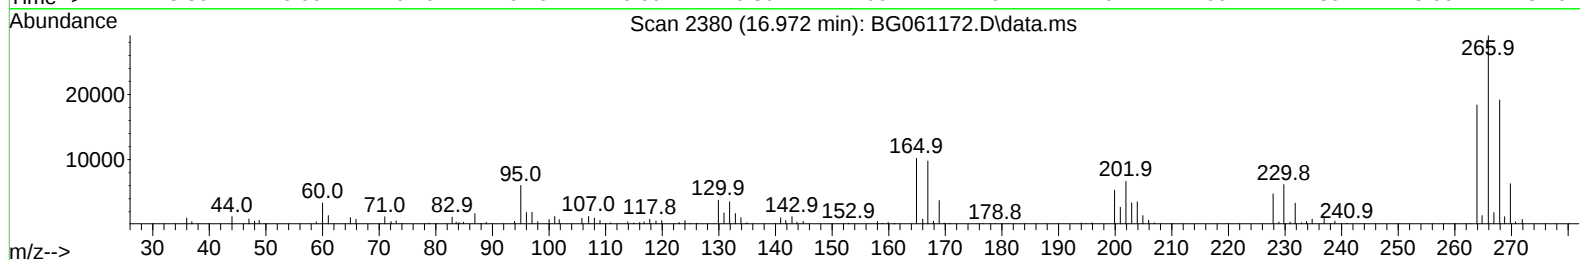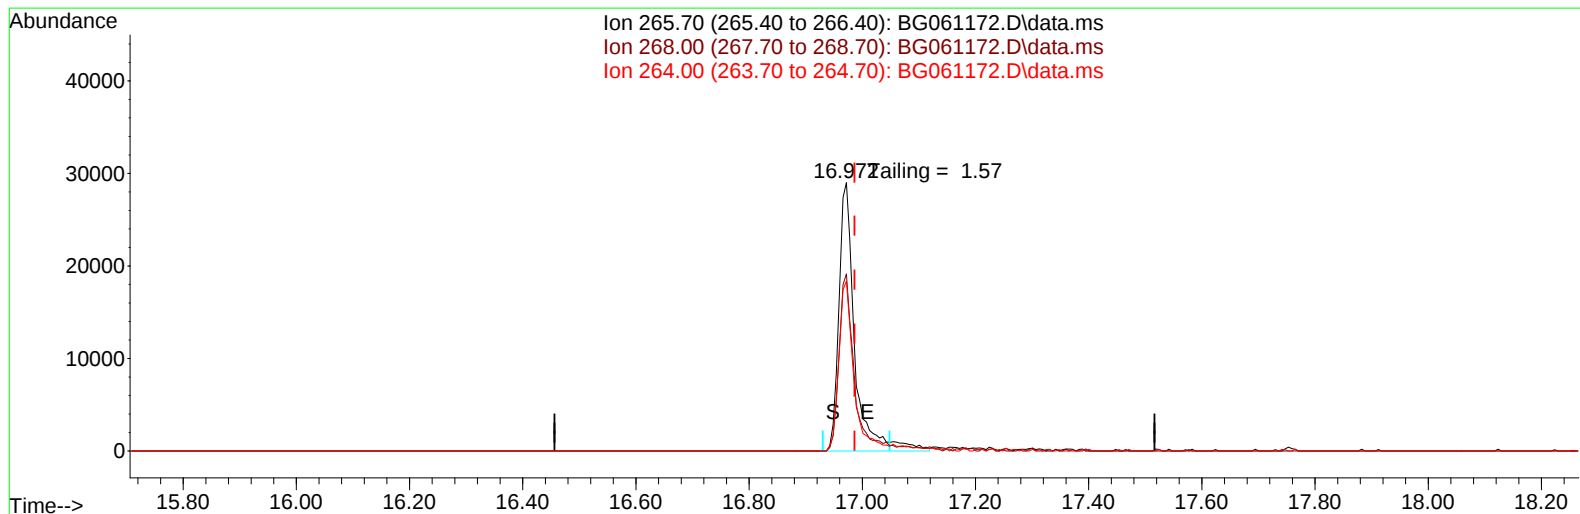

TIC: BG061172.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.014) 13489.18 ng




response 53949

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	66.02
264.00	64.40	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051324\
Data File : BG061172.D
Acq On : 13 May 2024 10:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 13 10:42:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

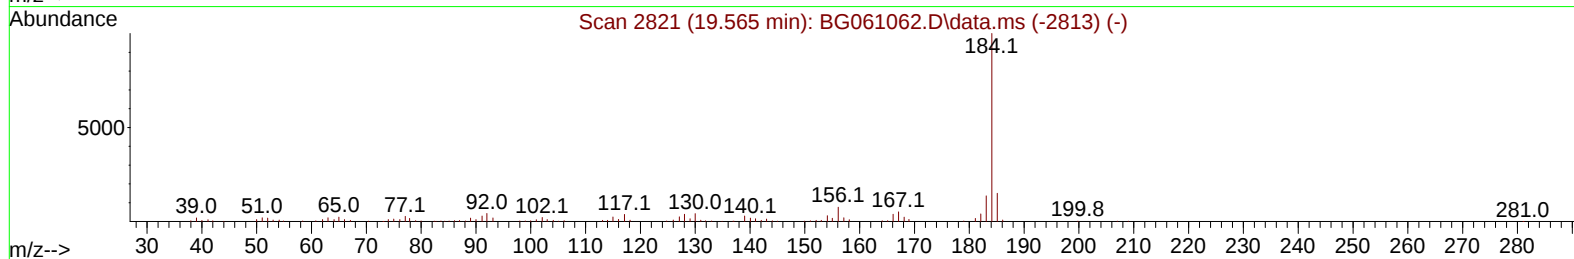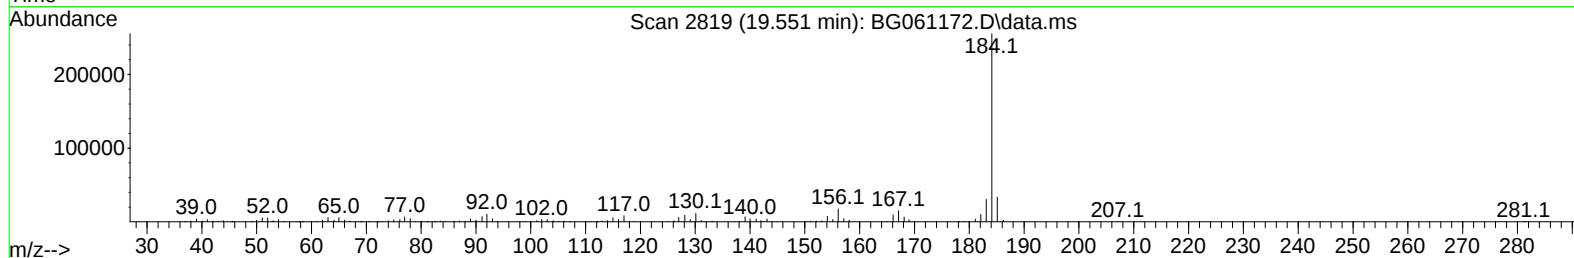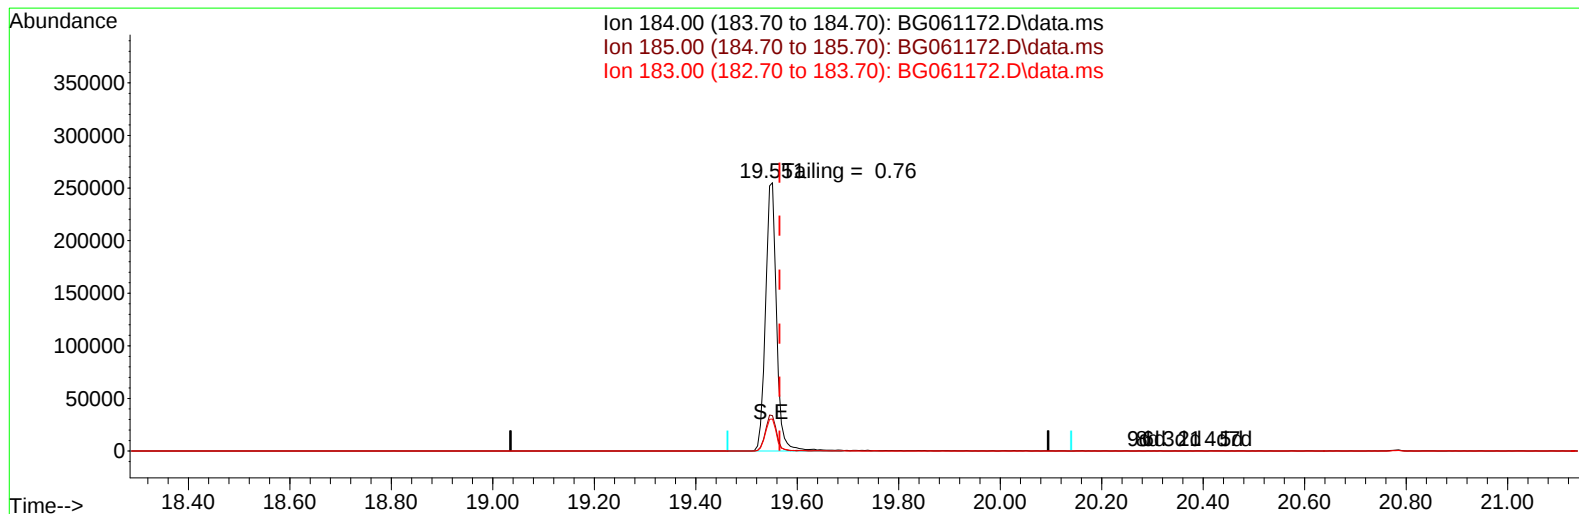

TIC: BG061172.D\data.ms

(77) Benzidine

19.551min (-0.014) 334273.67 ng m

response 384992

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.17
183.00	13.60	11.95
0.00	0.00	0.00