

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051415\
 Data File : BG017146.D
 Acq On : 14 May 2015 18:24
 Operator : TP/IZ
 Sample : G2225-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-141-51215

Quant Time: May 15 05:32:55 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 13 16:12:13 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	47539	20.00	ng	0.00
21) Naphthalene-d8	10.50	136	206510	20.00	ng	0.00
38) Acenaphthene-d10	14.36	164	139013	20.00	ng	0.00
63) Phenanthrene-d10	17.11	188	313338	20.00	ng	0.00
75) Chrysene-d12	21.29	240	311890	20.00	ng	0.00
86) Perylene-d12	23.56	264	305466	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	174543	65.14	ng	0.00
7) Phenol-d6	6.90	99	143543	38.17	ng	0.00
23) Nitrobenzene-d5	8.86	82	396399	89.62	ng	0.00
41) 2,4,6-Tribromophenol	15.86	330	230000	136.87	ng	0.00
44) 2-Fluorobiphenyl	12.98	172	838082	88.46	ng	0.00
78) Terphenyl-d14	19.74	244	1410371	94.23	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.82	163	44482	4.09	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051415\
Data File : BG017146.D
Acq On : 14 May 2015 18:24
Operator : TP/IZ
Sample : G2225-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCW-WW-141-51215

Quant Time: May 15 05:32:55 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

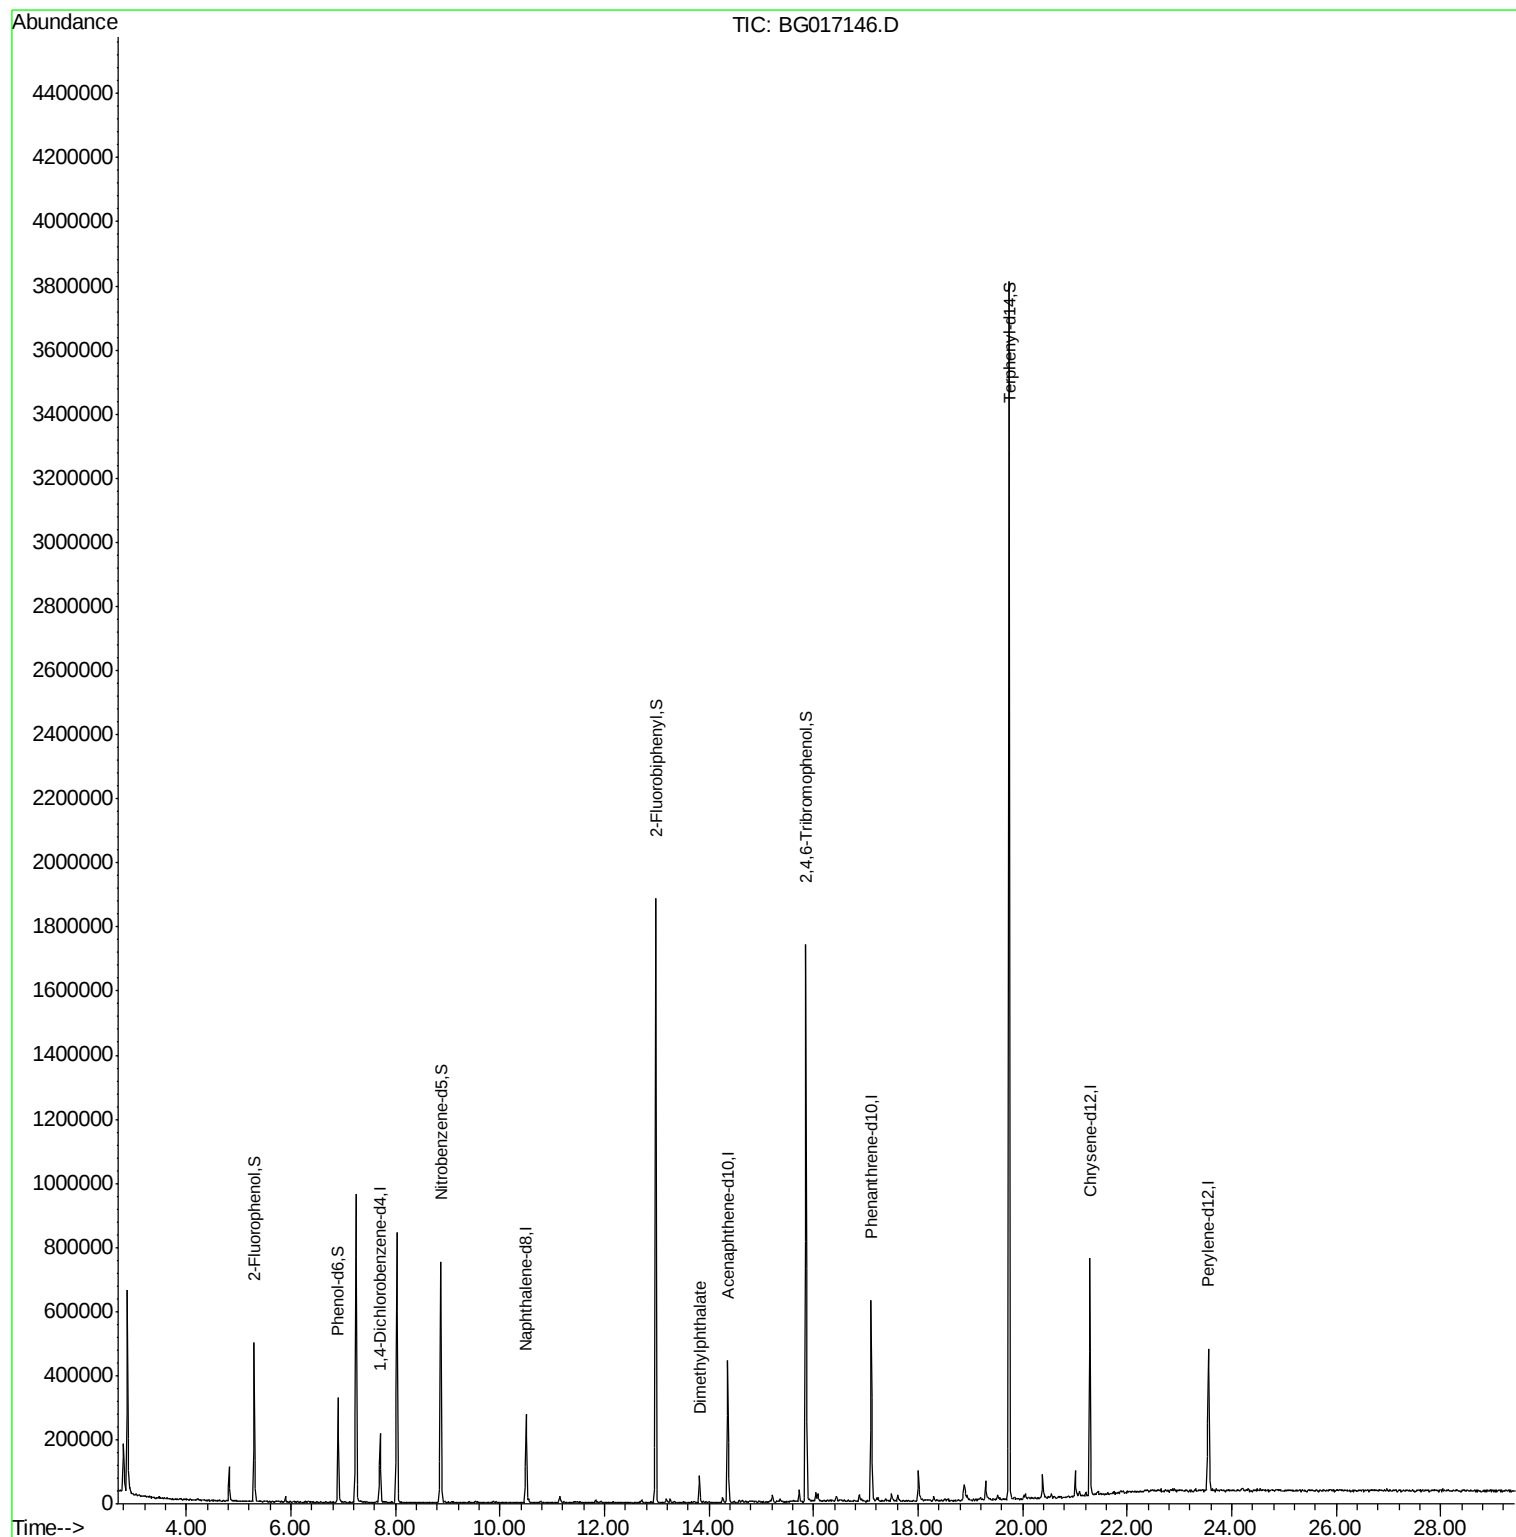



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.71 min Scan# 854

Delta R.T. -0.00 min

Lab File: BG017146.D

Acq: 14 May 2015 18:24

Instrument :

BNA_G

ClientSampleId :

DCW-WW-141-51215


Tgt Ion:152 Resp: 47539

Ion Ratio Lower Upper

152 100

150 145.7 120.8 181.2




115 68.5 49.4 74.2

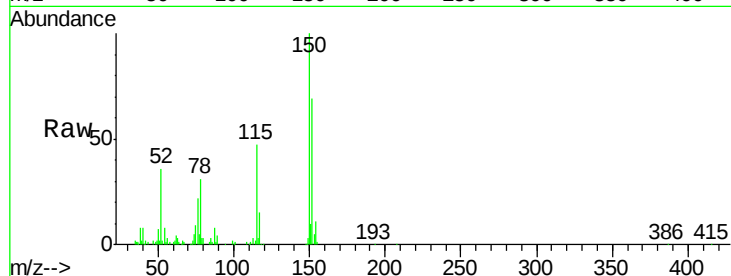

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

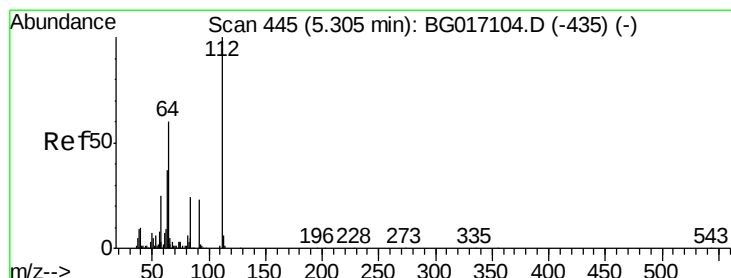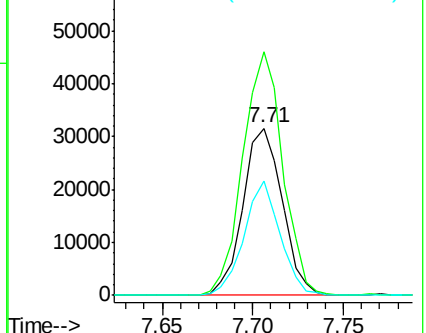

#5

2-Fluorophenol

Concen: 65.14 ng

RT: 5.30 min Scan# 444

Delta R.T. -0.01 min

Lab File: BG017146.D

Acq: 14 May 2015 18:24


Tgt Ion:112 Resp: 174543

Ion Ratio Lower Upper

112 100

64 69.0 48.1 72.1



63 39.4 29.8 44.8

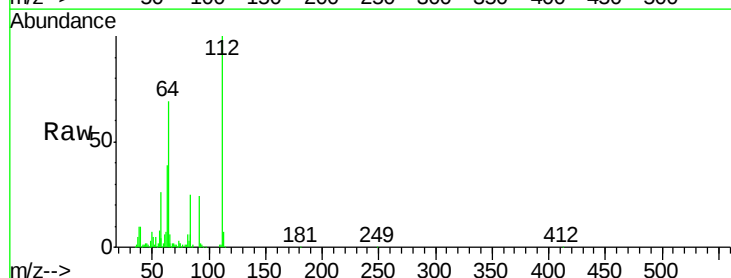


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

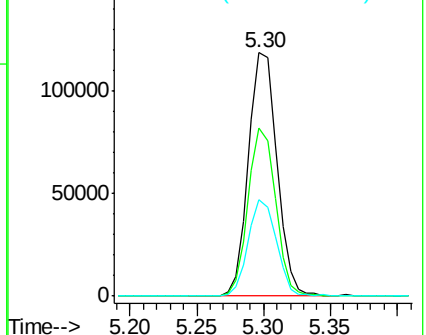

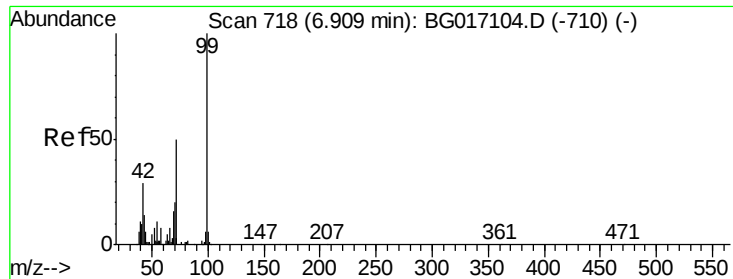

#7

Phenol-d6

Concen: 38.17 ng

RT: 6.90 min Scan# 717

Delta R.T. -0.01 min

Lab File: BG017146.D

Acq: 14 May 2015 18:24

Instrument :

BNA_G

ClientSampleId :

DCW-WW-141-51215


Tgt Ion: 99 Resp: 143543

Ion Ratio Lower Upper




99 100

42 28.2 23.5 35.3

71 45.2 39.8 59.8

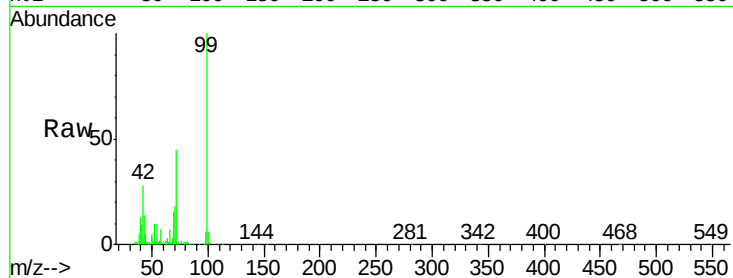

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

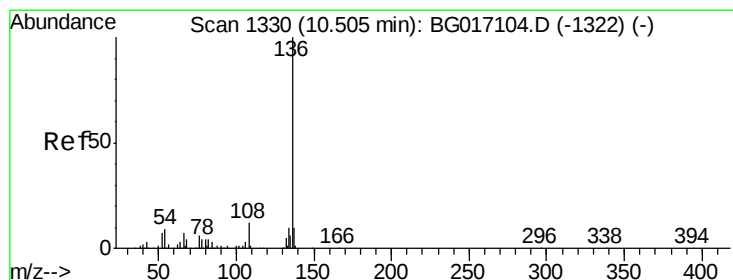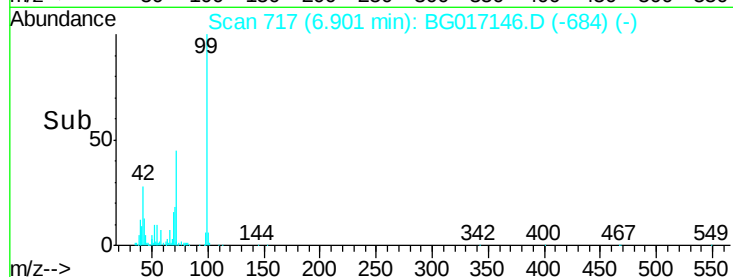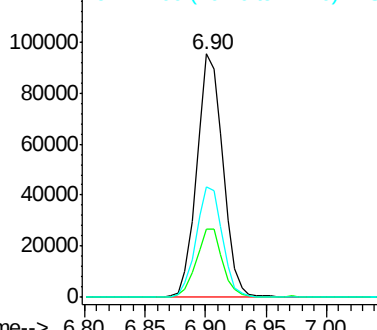

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.50 min Scan# 1329

Delta R.T. -0.01 min

Lab File: BG017146.D

Acq: 14 May 2015 18:24

Tgt Ion: 136 Resp: 206510


Ion Ratio Lower Upper

136 100



137 9.8 8.3 12.5


54 9.5 7.4 11.2

68 6.3 3.6 5.4#

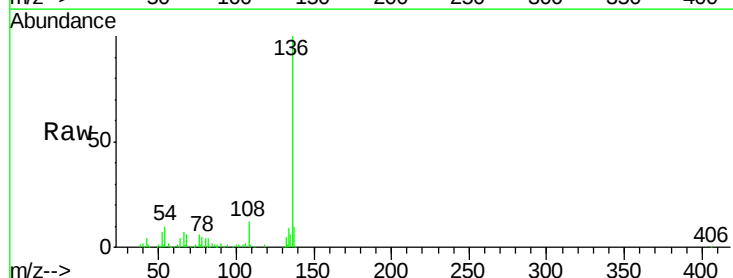

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



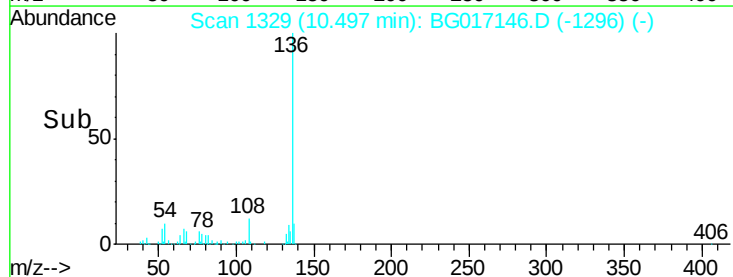
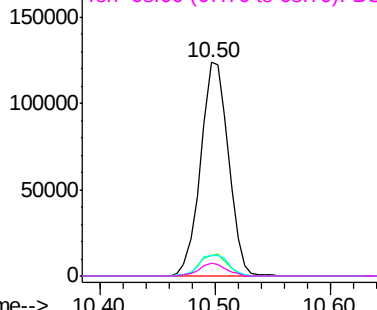


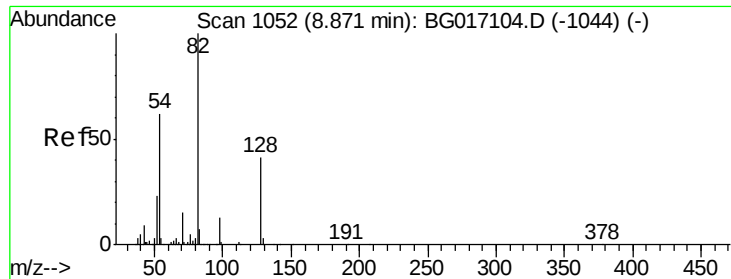

#23
 Nitrobenzene-d5
 Concen: 89.62 ng
 RT: 8.86 min Scan# 1051
 Delta R.T. -0.01 min
 Lab File: BG017146.D
 Acq: 14 May 2015 18:24




Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-141-51215


Tgt Ion	Ratio	Lower	Upper
82	100		
128	38.3	32.6	49.0
54	60.9	49.6	74.4

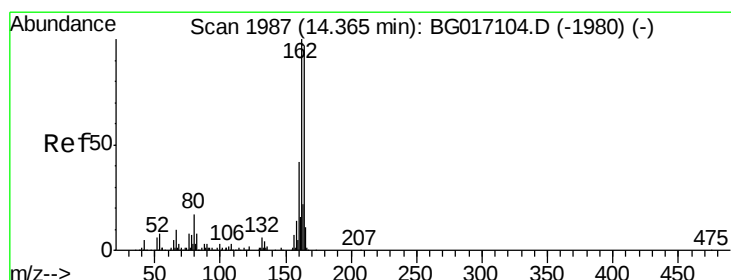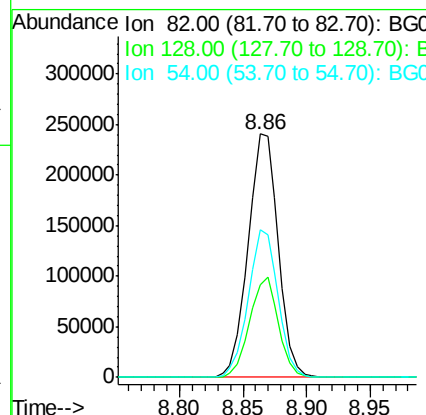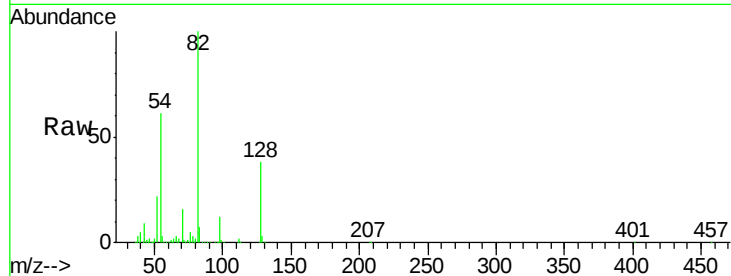

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.36 min Scan# 1987
 Delta R.T. -0.00 min
 Lab File: BG017146.D
 Acq: 14 May 2015 18:24

Tgt Ion	Ratio	Lower	Upper
164	100		
162	91.0	82.1	123.1
160	44.5	34.8	52.2

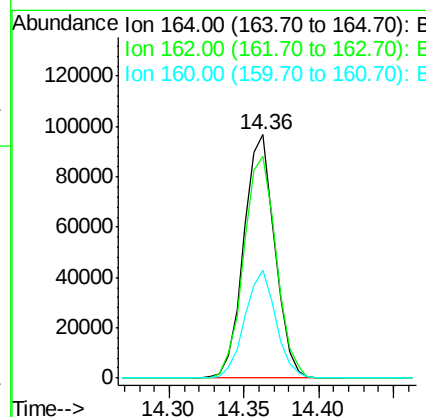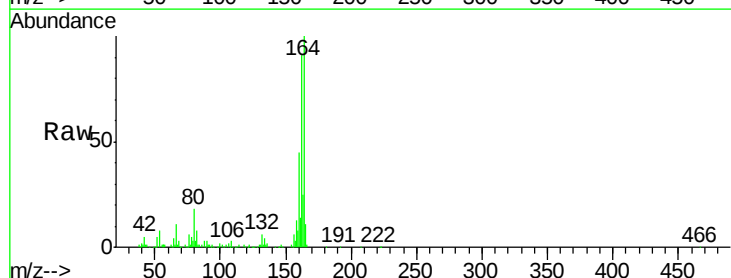


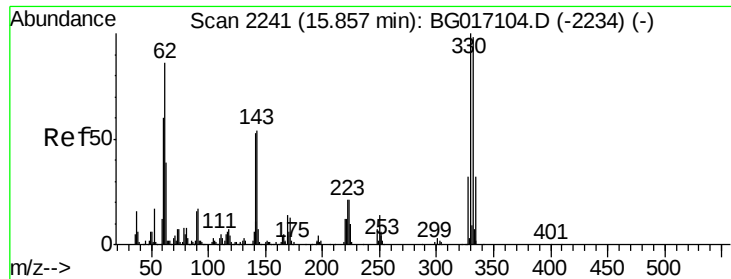




#41
 2,4,6-Tribromophenol
 Concen: 136.87 ng
 RT: 15.86 min Scan# 2241
 Delta R.T. -0.00 min
 Lab File: BG017146.D
 Acq: 14 May 2015 18:24

Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-141-51215

Tgt Ion:330 Resp: 230000
 Ion Ratio Lower Upper
 330 100
 332 97.8 76.9 115.3
 141 51.7 42.2 63.2

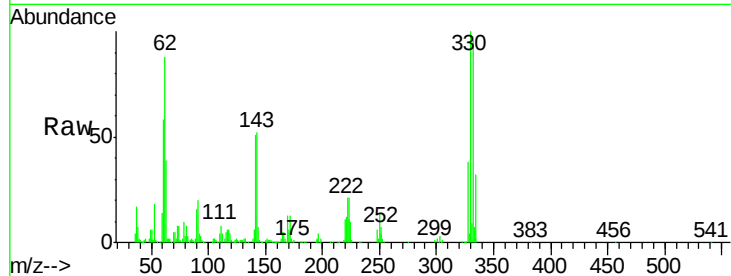


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

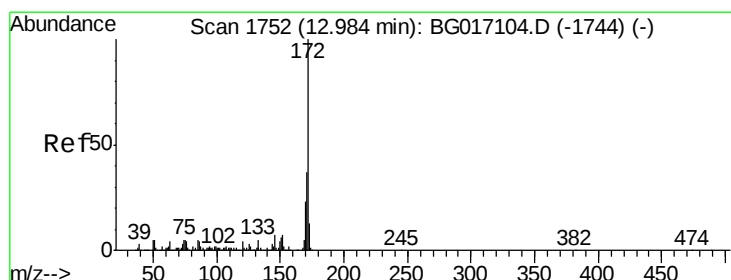
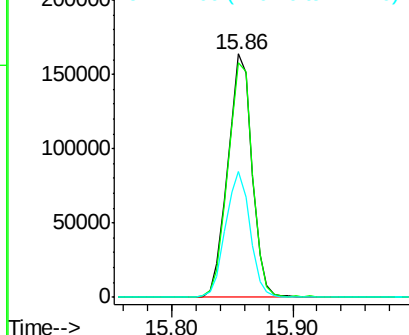



#44
 2-Fluorobiphenyl
 Concen: 88.46 ng
 RT: 12.98 min Scan# 1752
 Delta R.T. -0.00 min
 Lab File: BG017146.D
 Acq: 14 May 2015 18:24

Tgt Ion:172 Resp: 838082
 Ion Ratio Lower Upper
 172 100
 171 38.6 29.7 44.5
 170 24.1 18.4 27.6

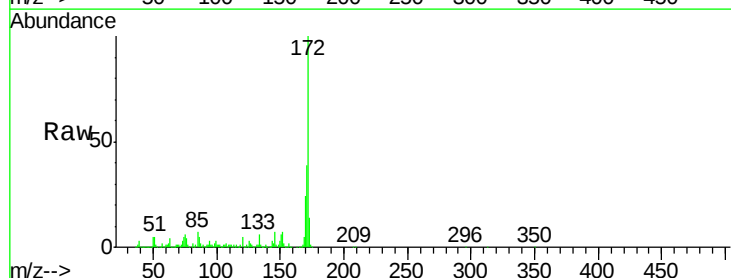

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

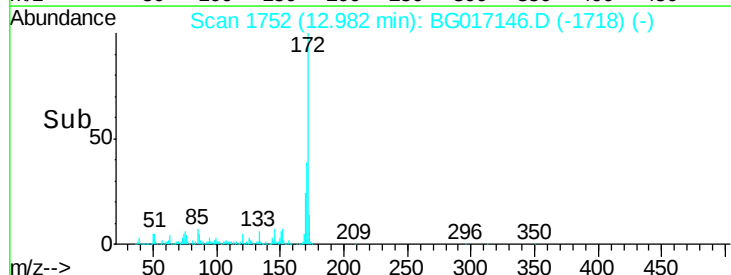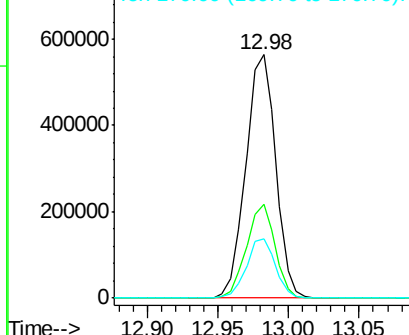



#49

Dimethylphthalate

Concen: 4.09 ng

RT: 13.82 min Scan# 1894

Delta R.T. -0.01 min

Lab File: BG017146.D

Acq: 14 May 2015 18:24

Instrument :

BNA_G

ClientSampleId :

DCW-WW-141-51215


Tgt Ion:163 Resp: 44482

Ion Ratio Lower Upper

163 100

194 7.6 5.6 8.4




164 11.6 8.6 13.0

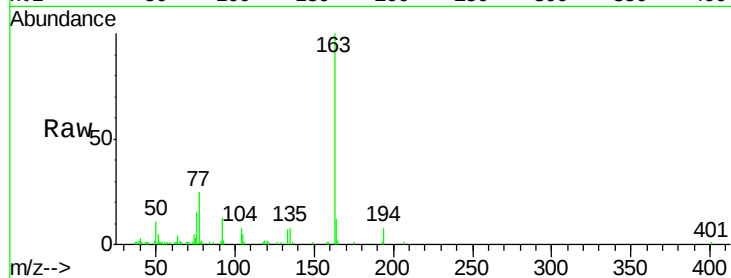

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

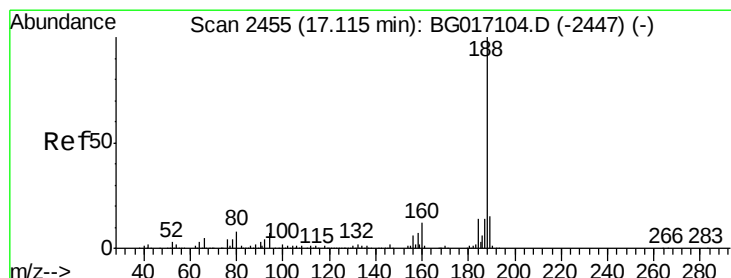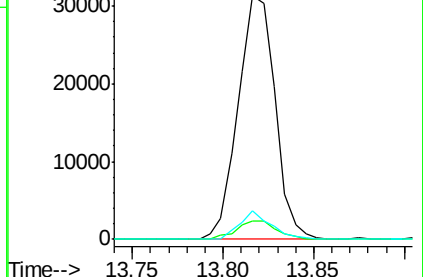

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.11 min Scan# 2454

Delta R.T. -0.01 min

Lab File: BG017146.D

Acq: 14 May 2015 18:24


Tgt Ion:188 Resp: 313338

Ion Ratio Lower Upper

188 100

94 10.1 5.8 8.6#



80 10.0 6.5 9.7#

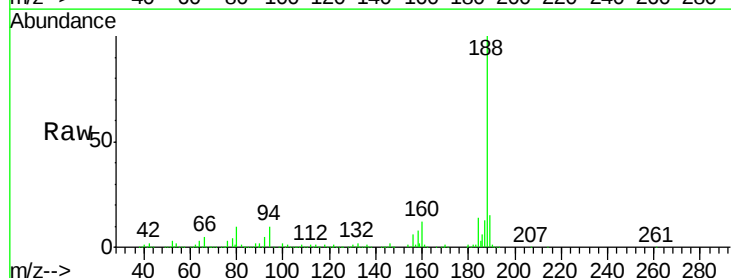


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC




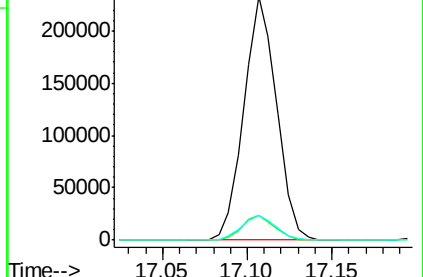


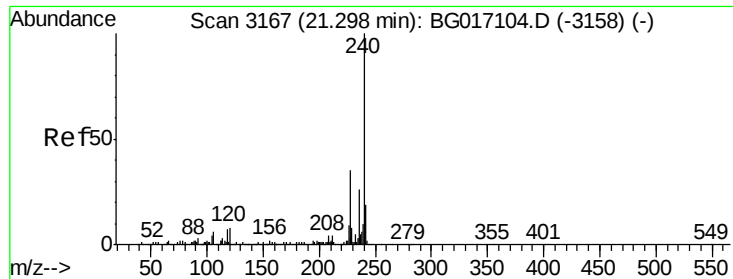

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.29 min Scan# 3166
 Delta R.T. -0.01 min
 Lab File: BG017146.D
 Acq: 14 May 2015 18:24




Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-141-51215


Tgt Ion:240 Resp: 311890
 Ion Ratio Lower Upper
 240 100
 120 10.6 6.0 9.0#
 236 25.0 20.5 30.7

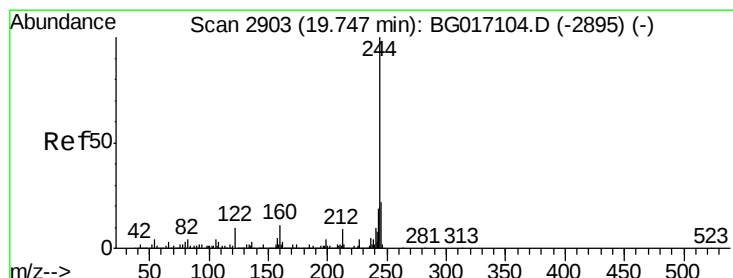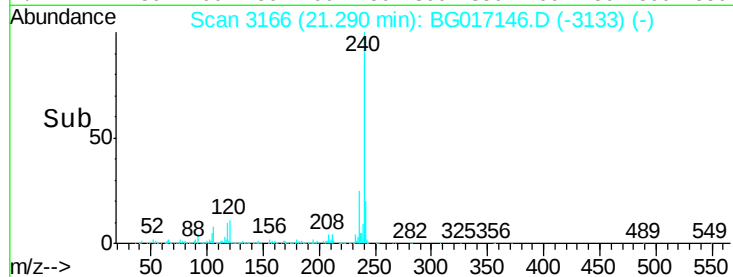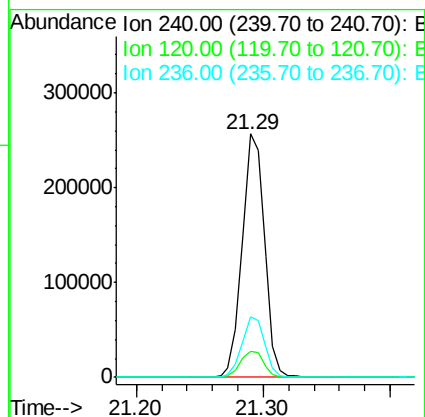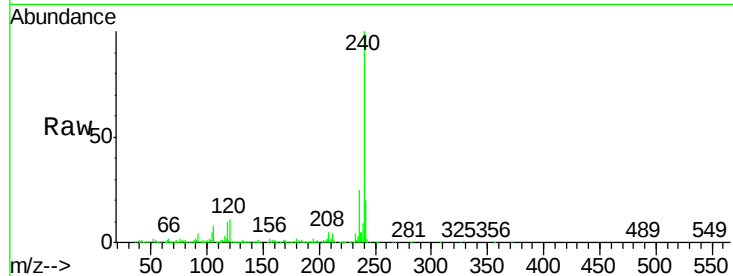

#78
 Terphenyl-d14
 Concen: 94.23 ng
 RT: 19.74 min Scan# 2903
 Delta R.T. -0.00 min
 Lab File: BG017146.D
 Acq: 14 May 2015 18:24

Tgt Ion:244 Resp: 1410371
 Ion Ratio Lower Upper
 244 100
 212 9.0 7.0 10.4
 122 12.7 8.4 12.6#

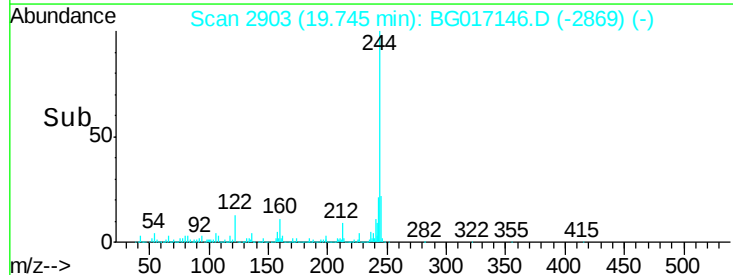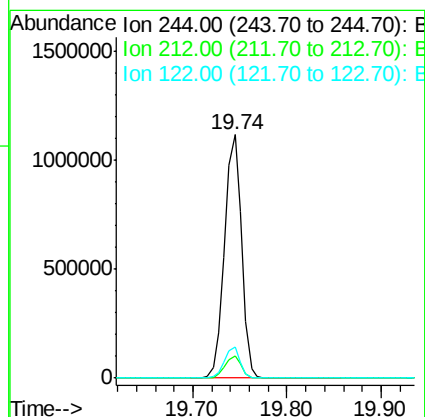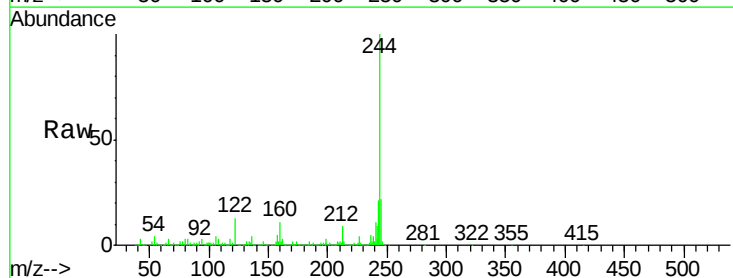



#86

Perylene-d12

Concen: 20.00 ng

RT: 23.56 min Scan# 3552

Delta R.T. -0.01 min

Lab File: BG017146.D


Acq: 14 May 2015 18:24

Instrument :

BNA_G

ClientSampleId :

DCW-WW-141-51215

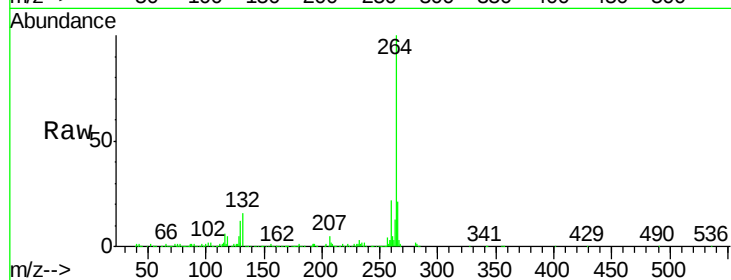


Tgt Ion:264 Resp: 305466

Ion Ratio Lower Upper

264 100

260 22.0 18.0 27.0

265 21.0 17.4 26.0

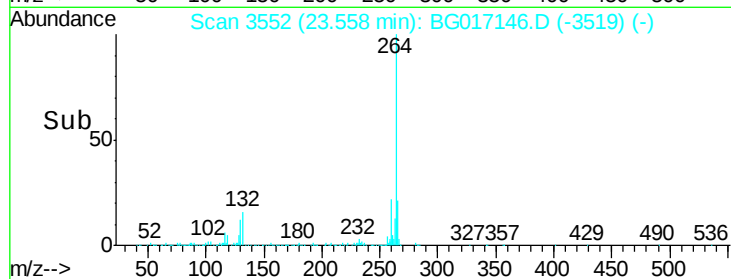

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

