


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051415\
 Data File : BG017154.D
 Acq On : 15 May 2015 00:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

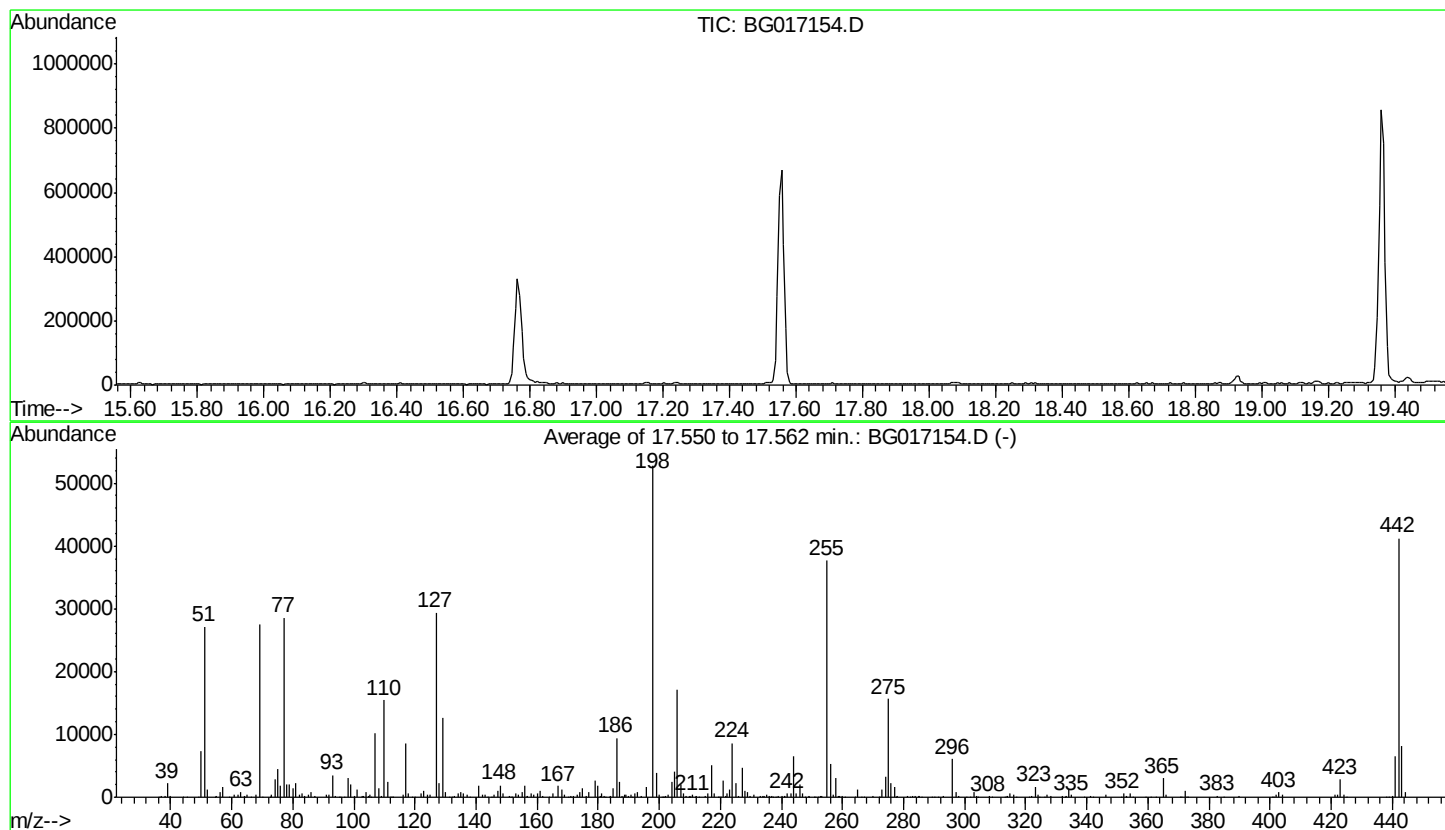

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	27160	PASS
68	69	0.00	2	1.5	421	PASS
69	198	0.00	100	52.0	27453	PASS
70	69	0.00	2	0.2	63	PASS
127	198	10	80	55.7	29378	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52773	PASS
199	198	5	9	7.2	3820	PASS
275	198	10	60	29.7	15674	PASS
365	198	1	100	5.6	2979	PASS
441	442	0.01	24	16.0	6580	PASS
442	198	50	100	78.0	41181	PASS
443	442	15	24	19.6	8055	PASS