
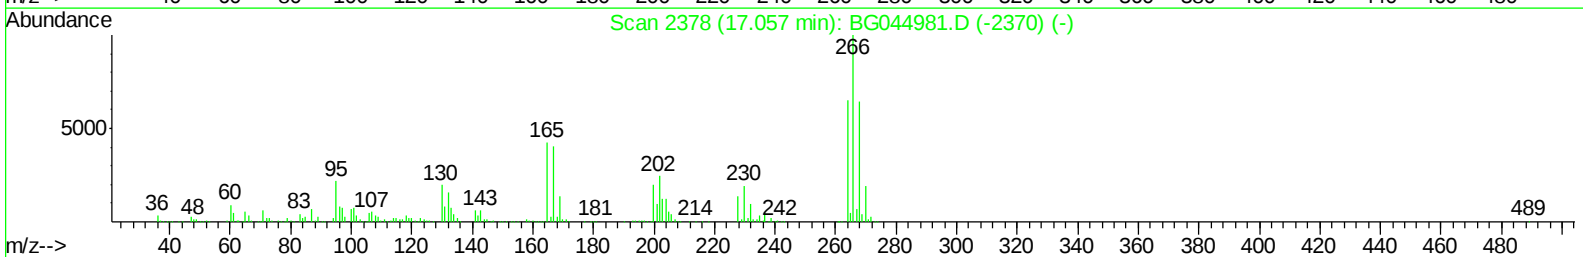
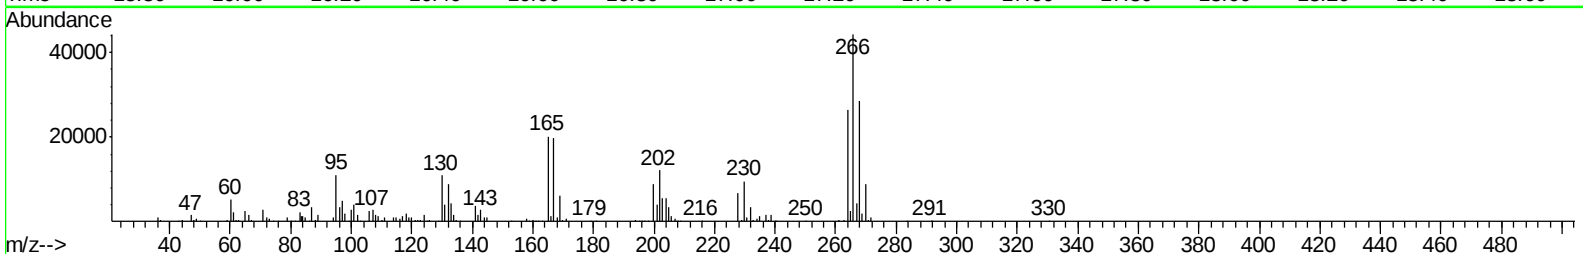


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051420\
Data File : BG045372.D
Acq On : 14 May 2020 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 01:57:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 13:01:16 2020
Response via : Initial Calibration

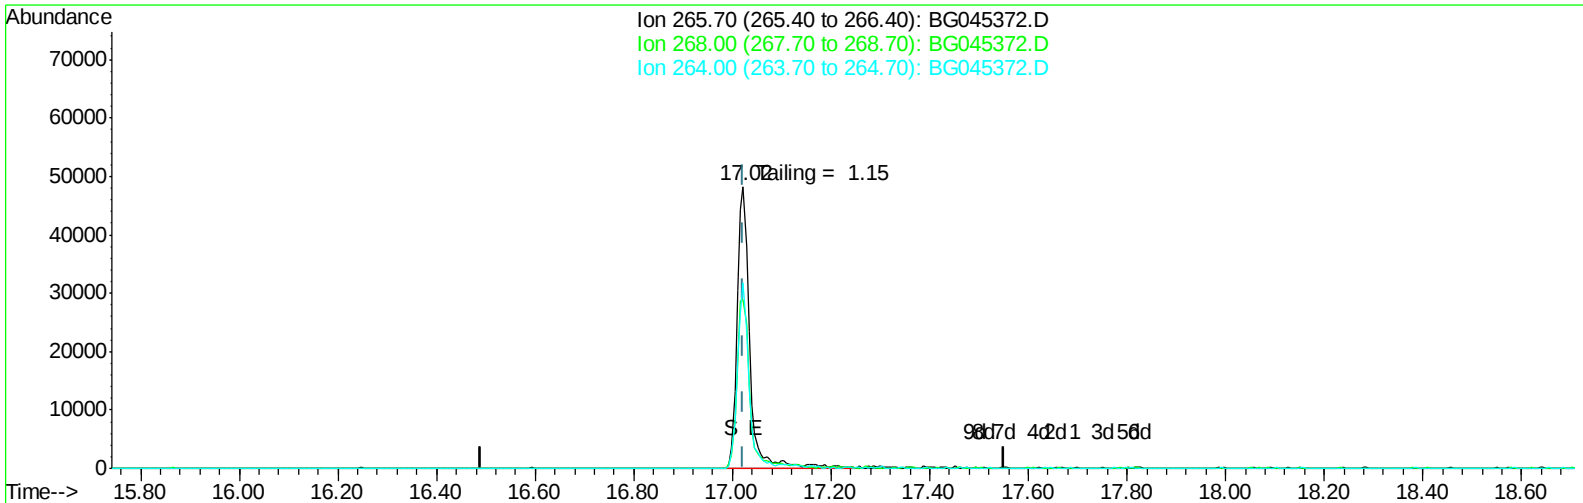

TIC: BG045372.D

(70) Pentachlorophenol (C)




17.698min (+0.676) 163.13ng

response 79

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	0.00#
264.00	65.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051420\
 Data File : BG045372.D
 Acq On : 14 May 2020 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 01:57:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 14 13:01:16 2020
 Response via : Initial Calibration

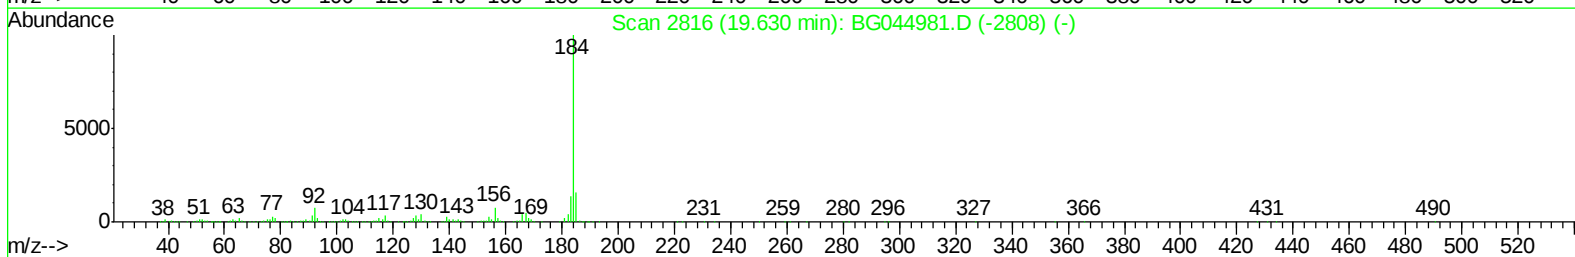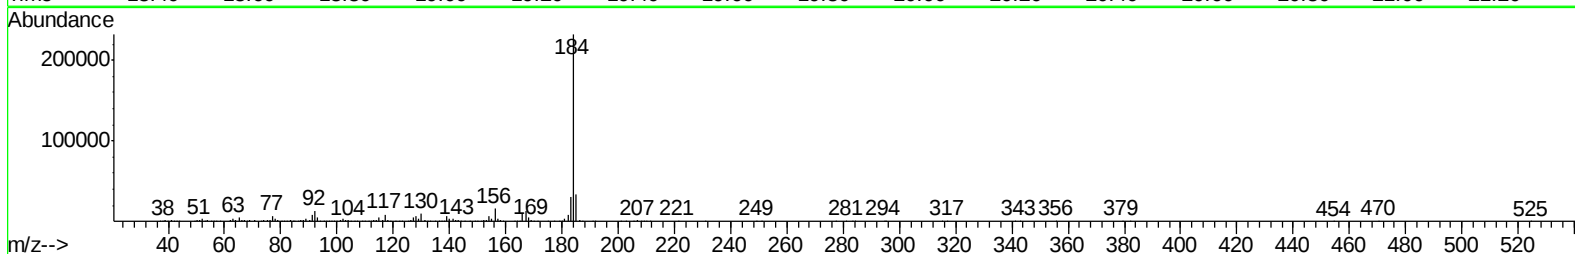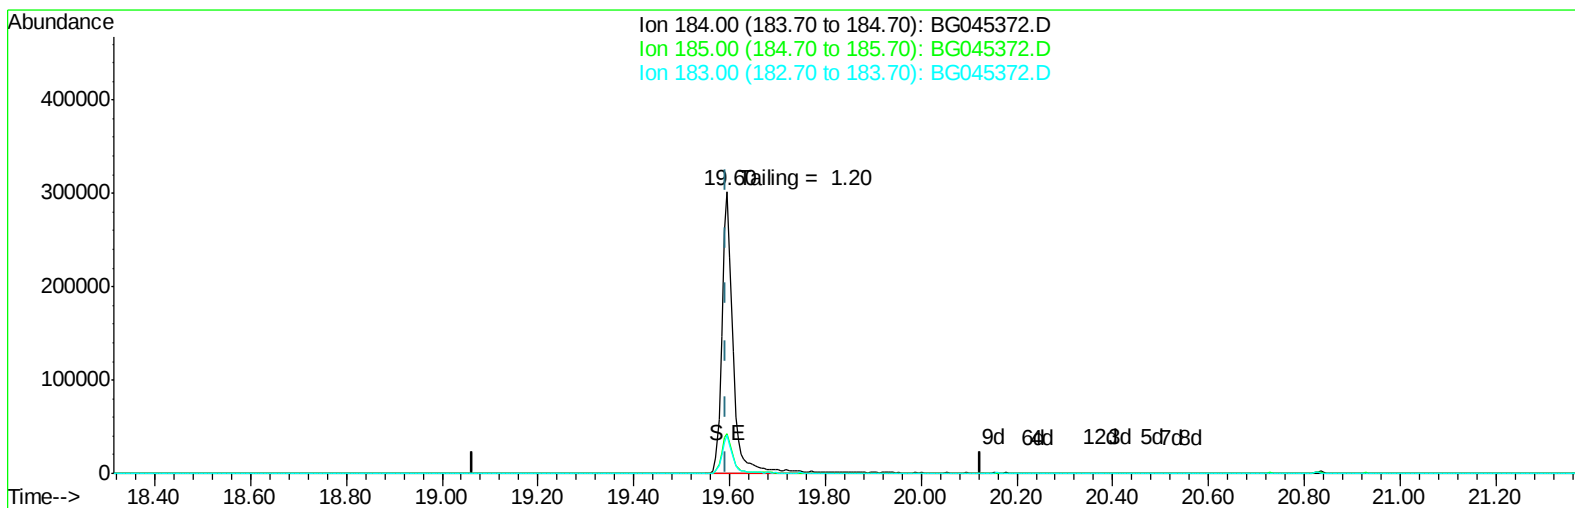

TIC: BG045372.D

(77) Benzidine

20.353min (+0.758) 272.34ng

response 421

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	30.78#
183.00	14.10	34.85#
0.00	0.00	0.00