


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051420\
 Data File : BG045372.D
 Acq On : 14 May 2020 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 14 13:01:16 2020

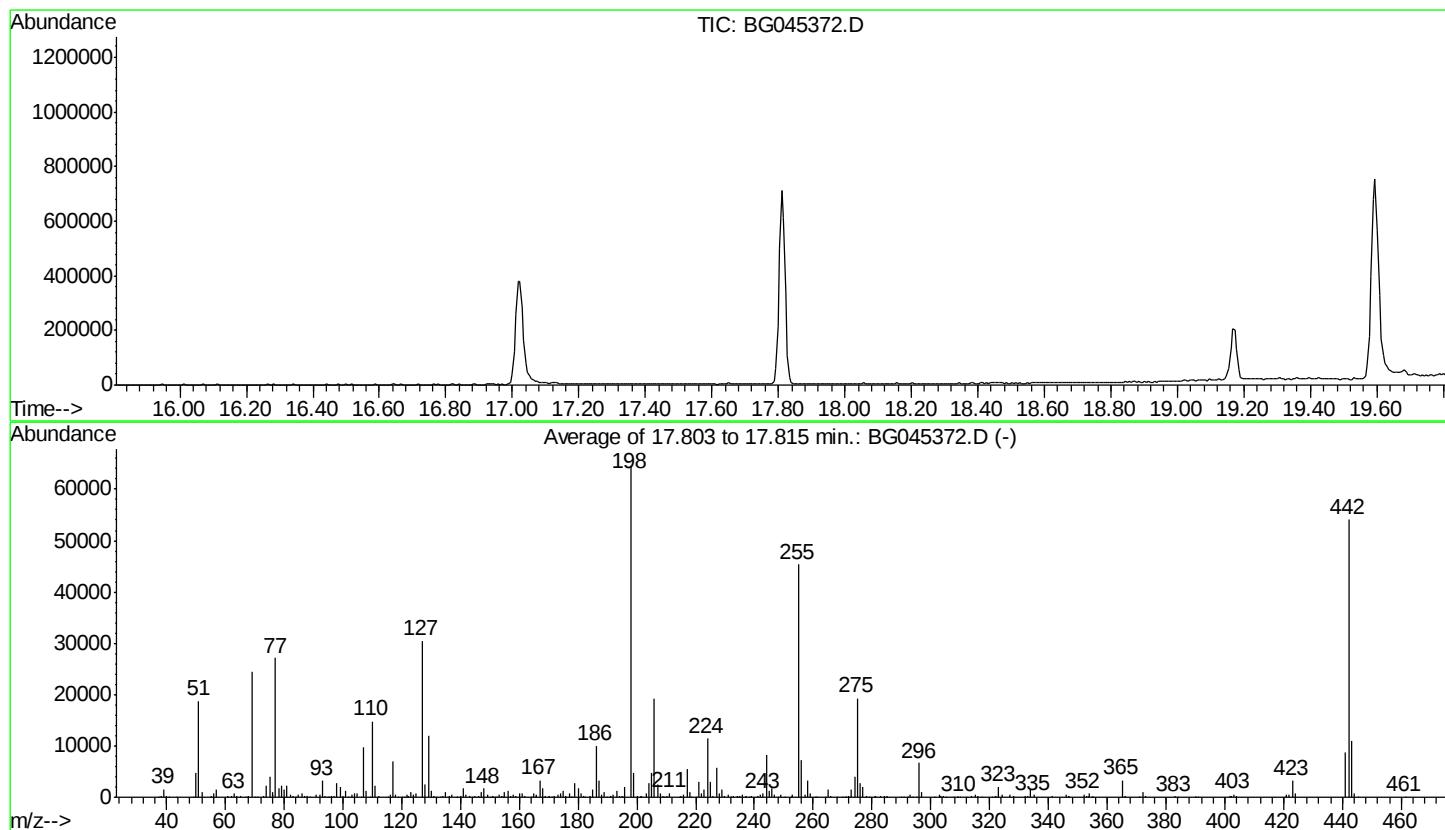

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	18749	PASS
68	69	0.00	2	0.6	137	PASS
69	198	0.00	100	37.7	24352	PASS
70	69	0.00	2	0.5	121	PASS
127	198	10	80	47.2	30512	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64605	PASS
199	198	5	9	7.3	4741	PASS
275	198	10	60	29.8	19234	PASS
365	198	1	100	5.1	3283	PASS
441	198	0.01	100	13.6	8805	PASS
442	198	50	100	83.7	54096	PASS
443	442	15	24	20.3	11004	PASS