


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051424\
Data File : BG061182.D
Acq On : 14 May 2024 9:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

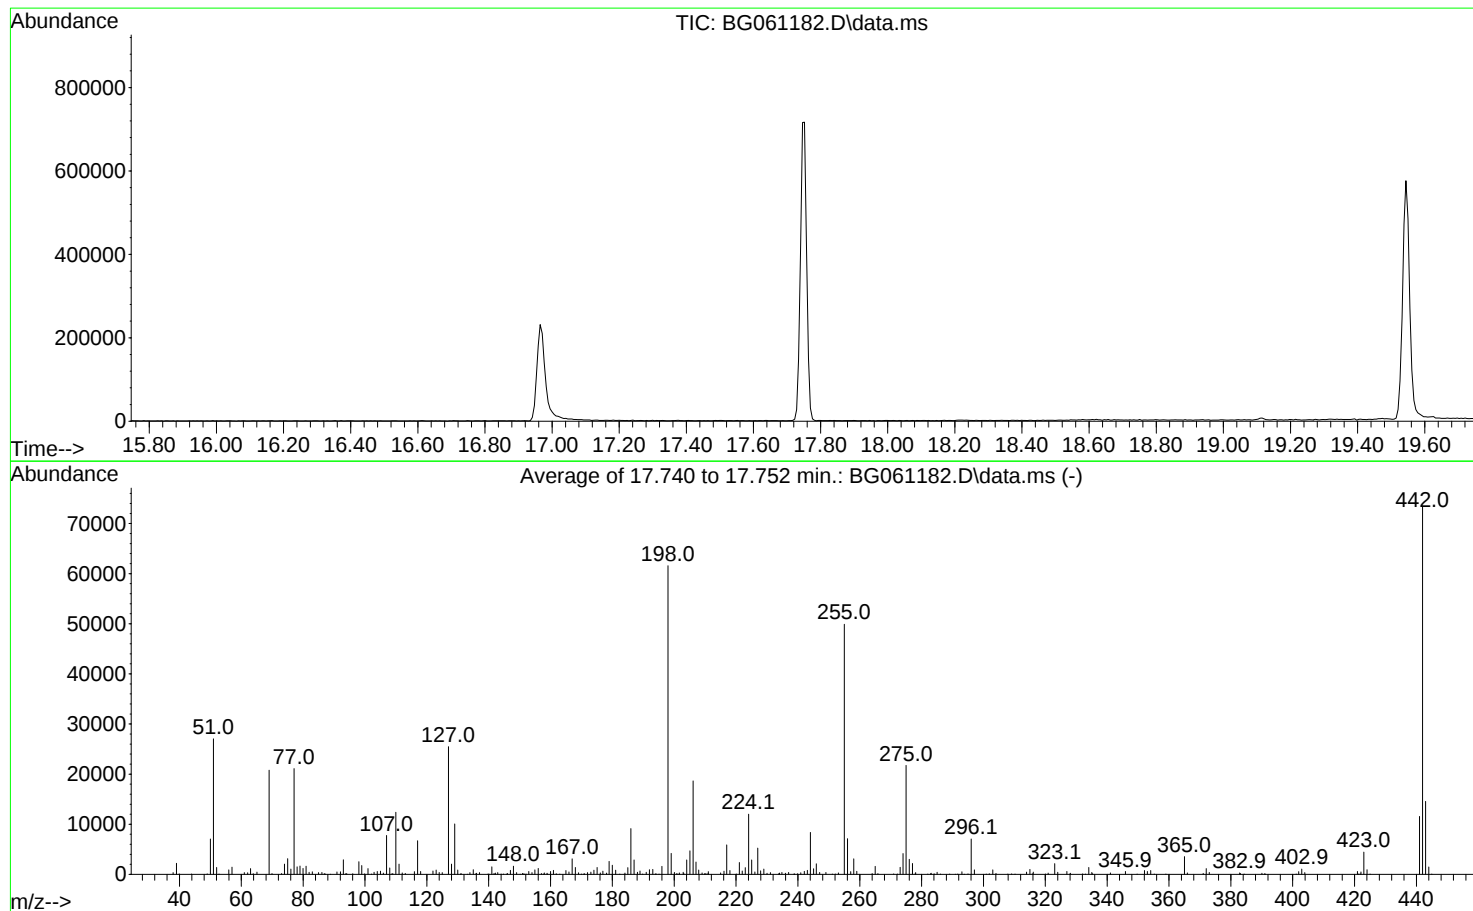




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	27059	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	20797	PASS
70	69	0.00	2	0.7	148	PASS
127	198	10	80	41.4	25475	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61595	PASS
199	198	5	9	6.8	4176	PASS
275	198	10	60	35.3	21743	PASS
365	198	1	100	5.8	3557	PASS
441	198	0.01	100	18.8	11567	PASS
442	442	50	100	100.0	73400	PASS
443	442	15	24	19.8	14562	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051424\
Data File : BG061182.D
Acq On : 14 May 2024 9:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 14 11:43:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

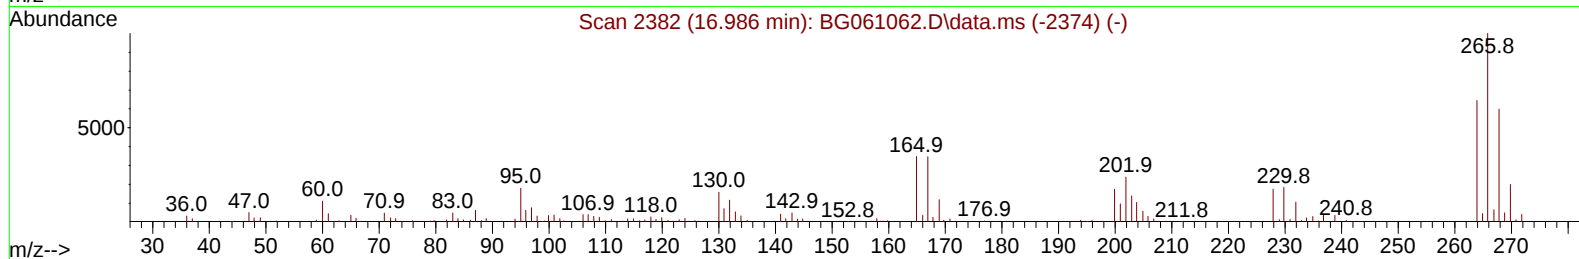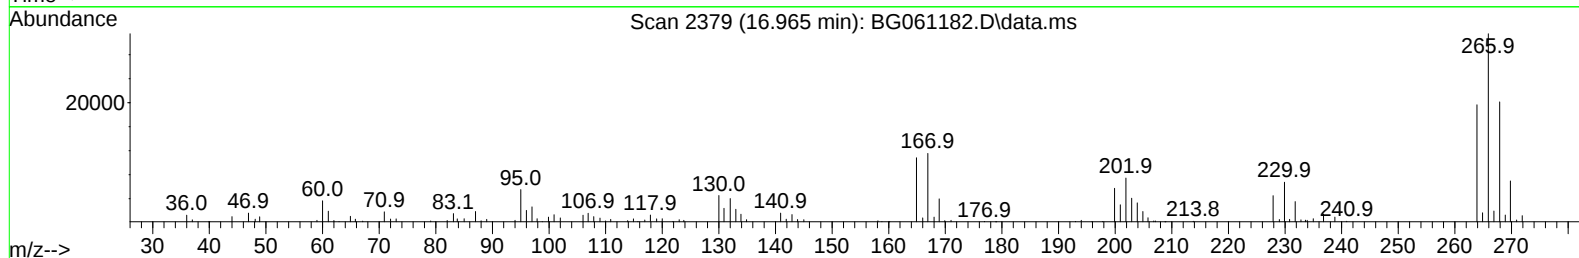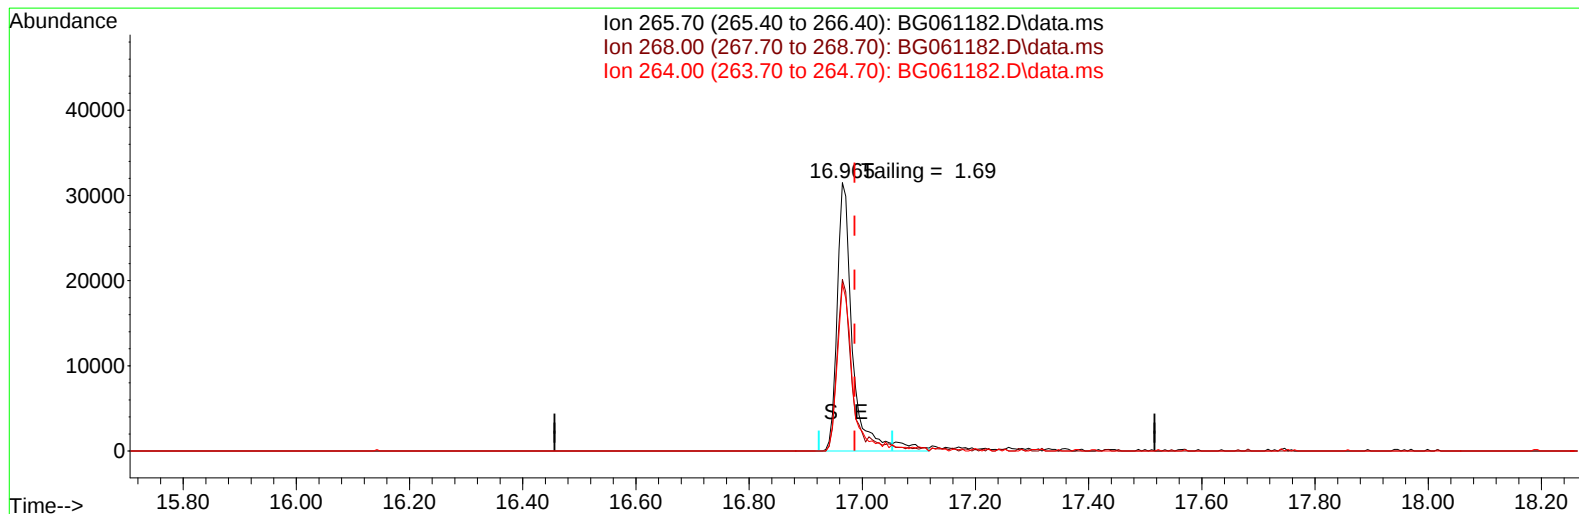

TIC: BG061182.D\data.ms

(70) Pentachlorophenol (C)

16.965min (-0.021) 14808.23 ng




response 57357

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	63.89
264.00	64.40	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051424\
Data File : BG061182.D
Acq On : 14 May 2024 9:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 14 11:43:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

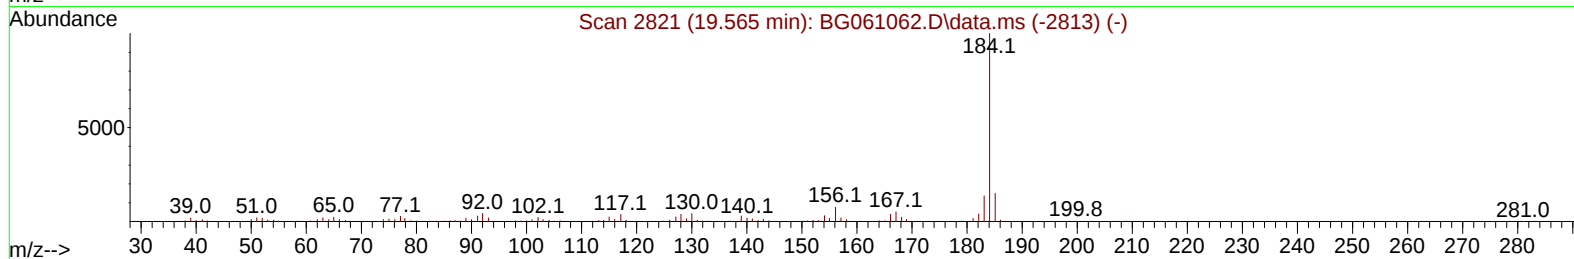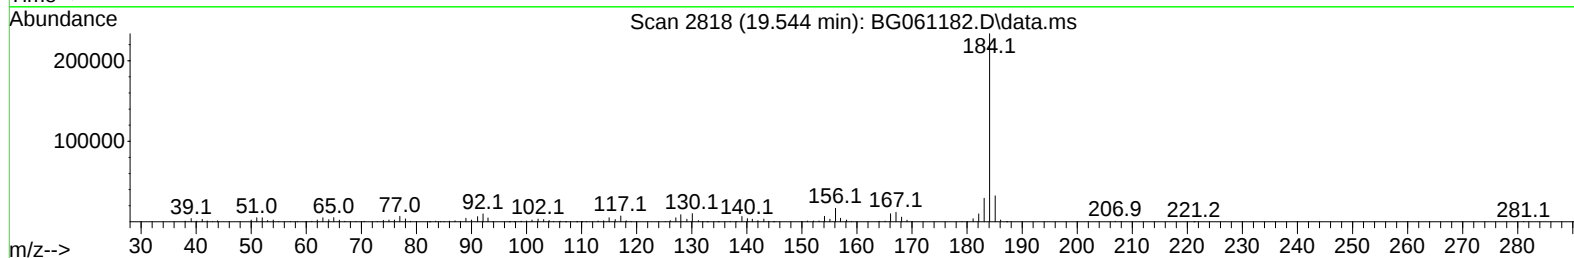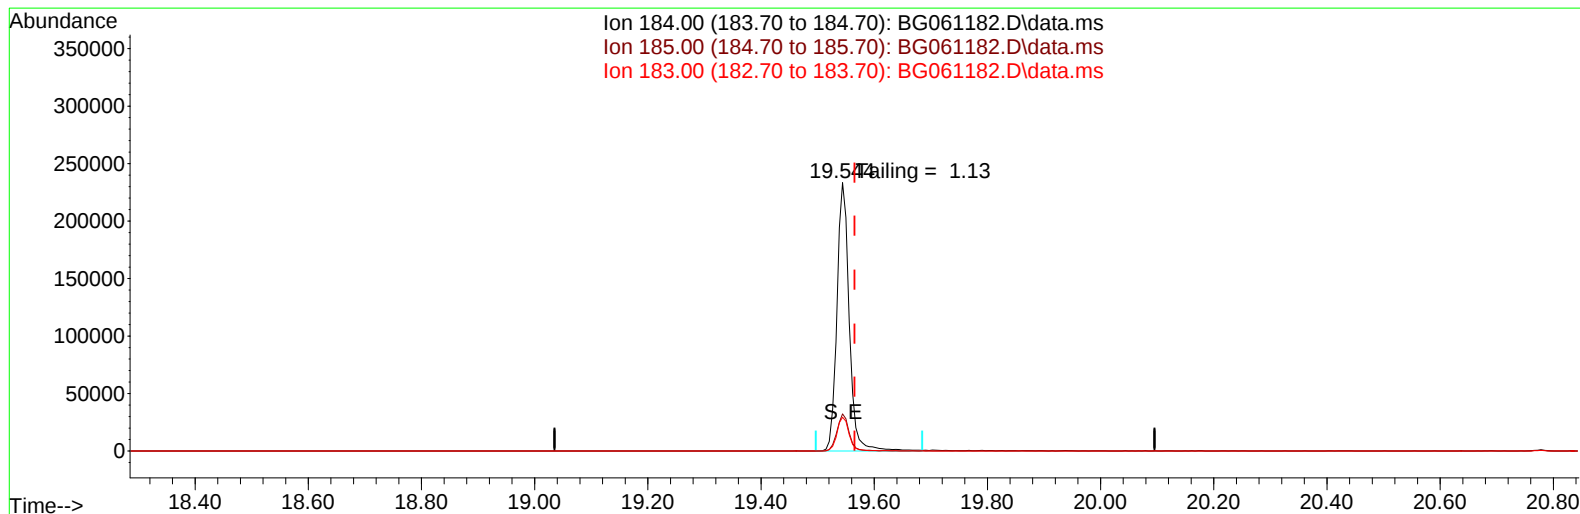

TIC: BG061182.D\data.ms

(77) Benzidine

19.544min (-0.021) 0.00 ng

response 353643

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.87
183.00	13.60	12.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/14/2024	BNA_G	<u>BG061182.D</u>
Compound Name	Response	Retention Time
DDT	239751	20.778
DDD	7370	20.343
DDE	609	19.844
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7979	247730	3.22

Instrument :
BNA_G
ClientSampleId :
DFTPP