

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051515\
 Data File : BG017185.D
 Acq On : 15 May 2015 20:42
 Operator : TP/IZ
 Sample : G2234-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW11

Quant Time: May 16 00:21:52 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 16 00:01:34 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	44018	20.00	ng	0.00
21) Naphthalene-d8	10.50	136	181932	20.00	ng	0.00
38) Acenaphthene-d10	14.36	164	116225	20.00	ng	0.00
63) Phenanthrene-d10	17.11	188	282457	20.00	ng	0.00
75) Chrysene-d12	21.29	240	304985	20.00	ng	0.00
86) Perylene-d12	23.56	264	297364	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	146853	59.19	ng	0.00
7) Phenol-d6	6.91	99	120407	34.58	ng	0.00
23) Nitrobenzene-d5	8.86	82	321208	82.43	ng	0.00
41) 2,4,6-Tribromophenol	15.86	330	191124	136.03	ng	0.00
44) 2-Fluorobiphenyl	12.98	172	666623	84.16	ng	0.00
78) Terphenyl-d14	19.74	244	1109891	75.84	ng	0.00
Target Compounds						
9) Benzaldehyde	6.91	77	161	Below Cal	Qvalue #	6

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051515\
Data File : BG017185.D
Acq On : 15 May 2015 20:42
Operator : TP/IZ
Sample : G2234-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW11

Quant Time: May 16 00:21:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 16 00:01:34 2015
Response via : Initial Calibration

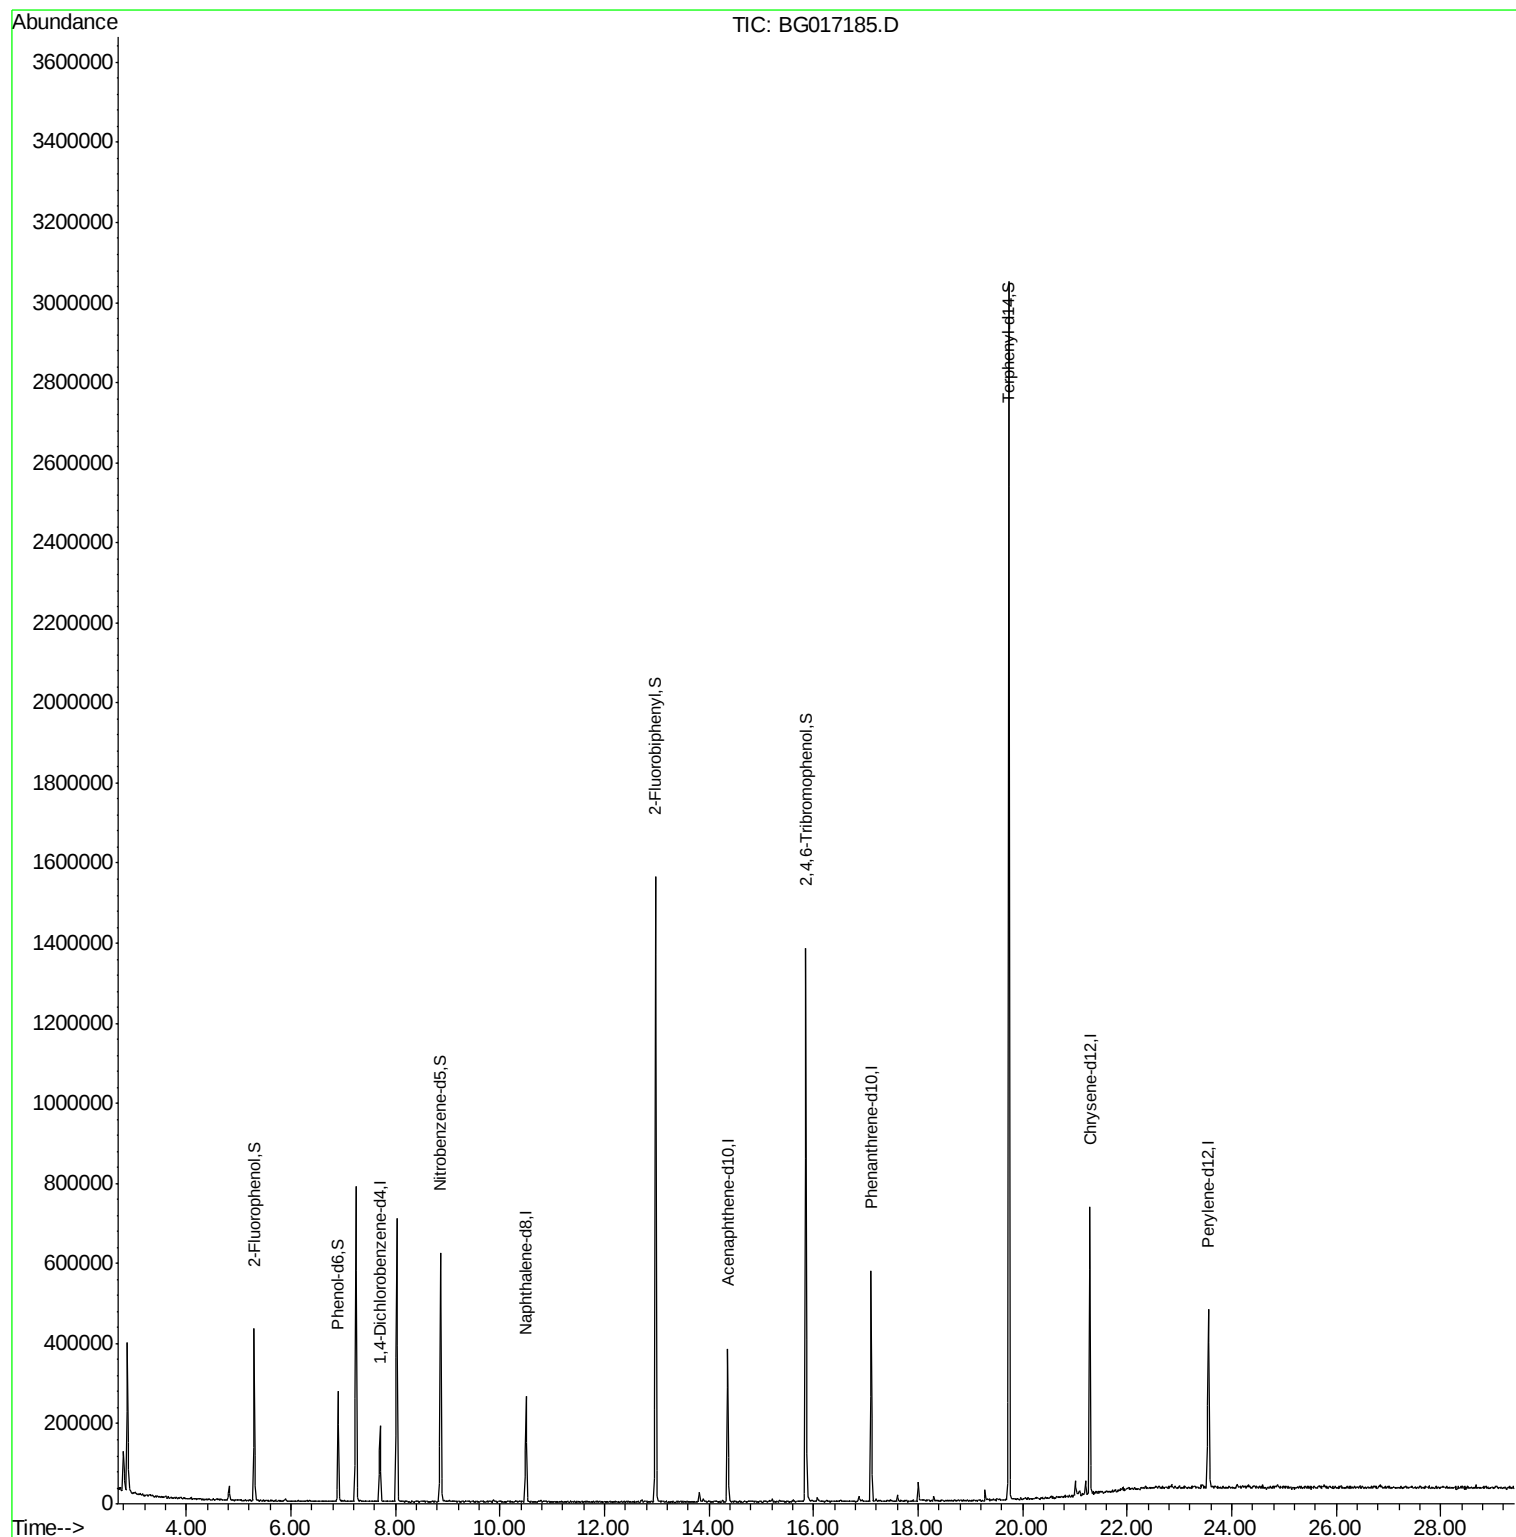




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.70 min Scan# 853
Delta R.T. -0.00 min
Lab File: BG017185.D
Acq: 15 May 2015 20:42

Instrument :
BNA_G
ClientSampleId :
MW11

Tgt Ion	Ratio	Lower	Upper
152	100		
150	141.6	120.8	181.2
115	66.8	49.4	74.2

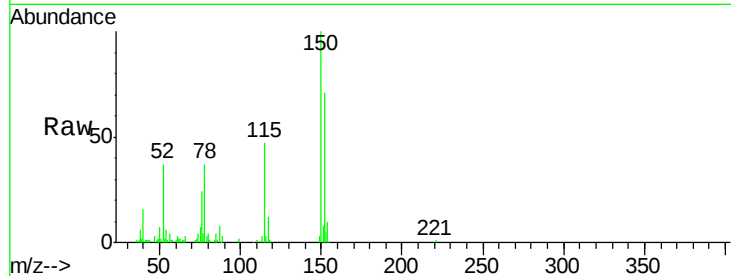


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

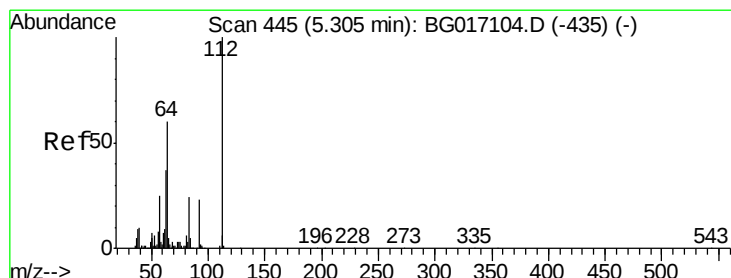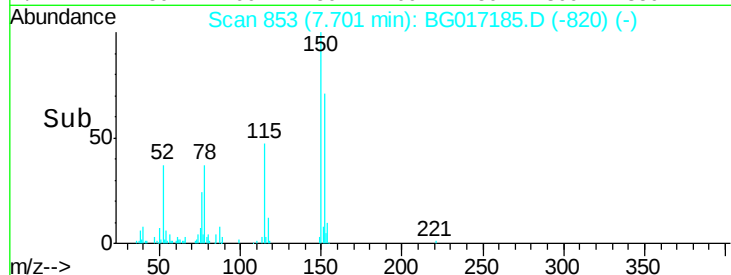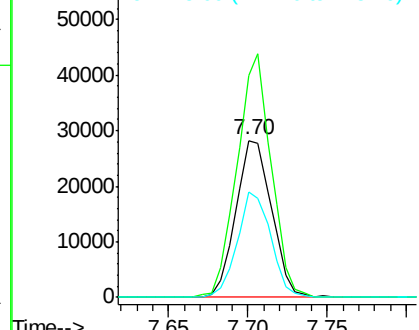



#5


2-Fluorophenol
Concen: 59.19 ng
RT: 5.30 min Scan# 444
Delta R.T. 0.00 min
Lab File: BG017185.D
Acq: 15 May 2015 20:42

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.3	48.1	72.1
63	40.8	29.8	44.8

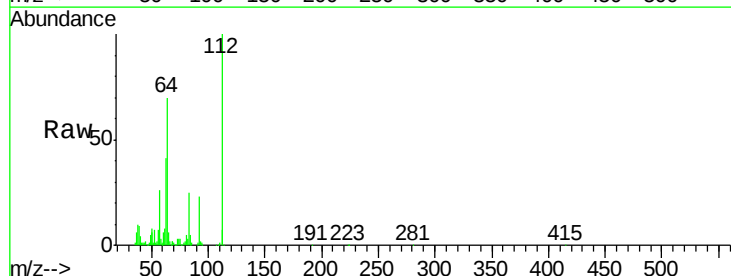

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

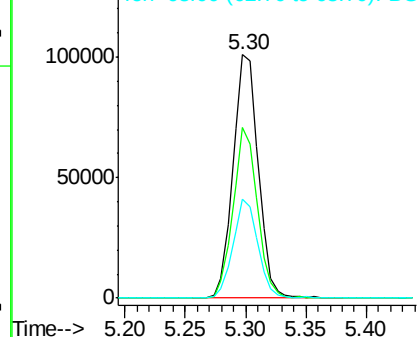

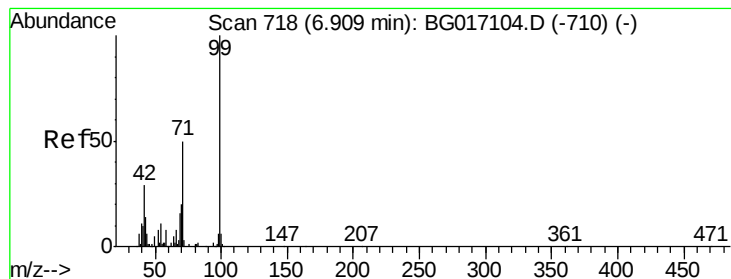

#7

Phenol-d6

Concen: 34.58 ng

RT: 6.91 min Scan# 718

Delta R.T. 0.00 min

Lab File: BG017185.D

Acq: 15 May 2015 20:42

Instrument :

BNA_G

ClientSampleId :

MW11


Tgt Ion: 99 Resp: 120407

Ion Ratio Lower Upper




99 100

42 29.0 23.5 35.3

71 50.4 39.8 59.8

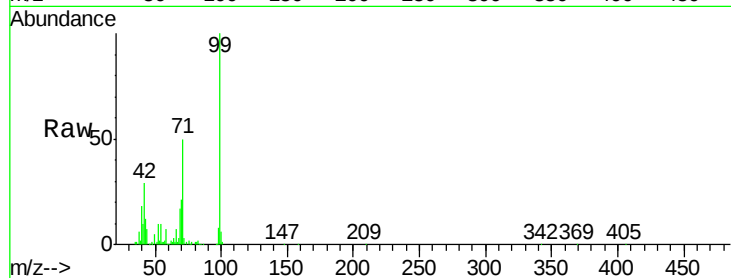

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

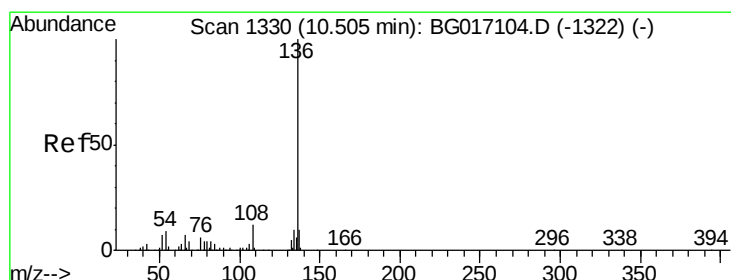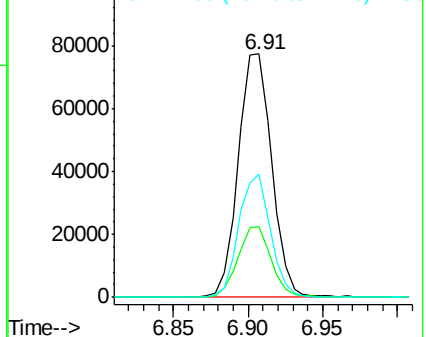

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.50 min Scan# 1329

Delta R.T. -0.00 min

Lab File: BG017185.D

Acq: 15 May 2015 20:42

Tgt Ion: 136 Resp: 181932


Ion Ratio Lower Upper

136 100



137 11.6 8.3 12.5


54 10.1 7.4 11.2

68 6.3 3.6 5.4#

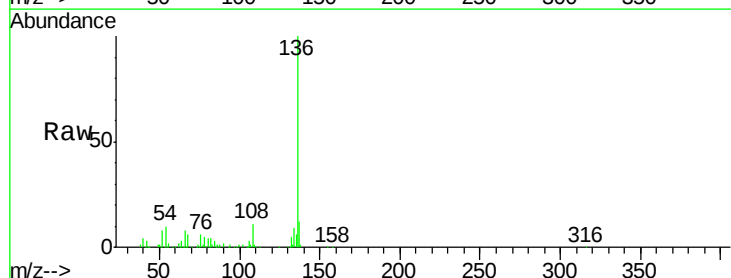

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



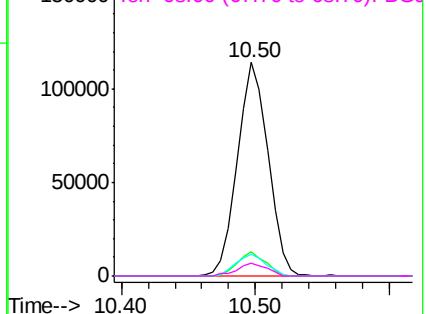




#23
 Nitrobenzene-d5
 Concen: 82.43 ng
 RT: 8.86 min Scan# 1051
 Delta R.T. -0.00 min
 Lab File: BG017185.D
 Acq: 15 May 2015 20:42




Instrument :
 BNA_G
 ClientSampleId :
 MW11

Tgt Ion: 82 Resp: 321208
 Ion Ratio Lower Upper
 82 100
 128 38.9 32.6 49.0
 54 60.4 49.6 74.4

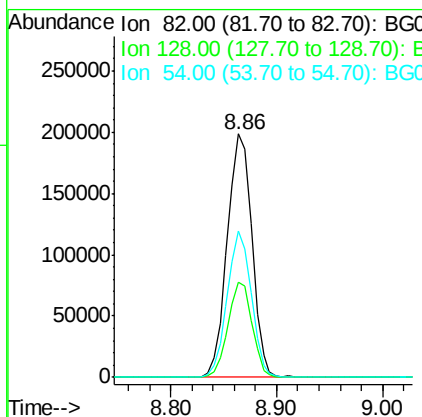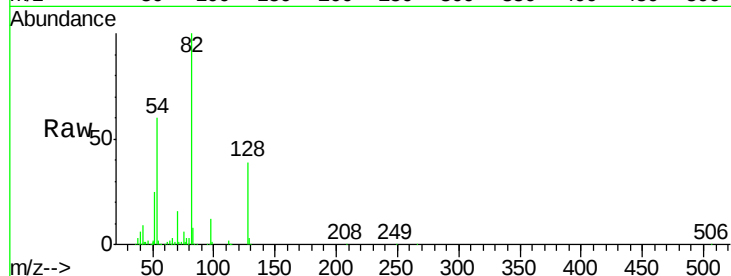

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.36 min Scan# 1986
 Delta R.T. -0.00 min
 Lab File: BG017185.D
 Acq: 15 May 2015 20:42

Tgt Ion: 164 Resp: 116225
 Ion Ratio Lower Upper
 164 100
 162 102.8 82.1 123.1
 160 46.0 34.8 52.2

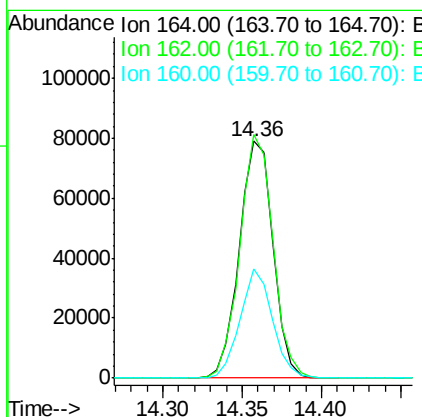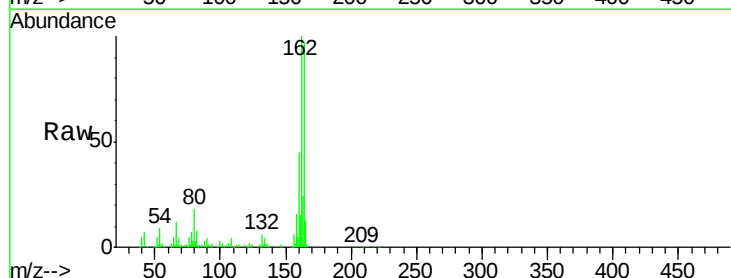






#41
 2,4,6-Tribromophenol
 Concen: 136.03 ng
 RT: 15.86 min Scan# 2241
 Delta R.T. 0.00 min
 Lab File: BG017185.D
 Acq: 15 May 2015 20:42

Instrument :
 BNA_G
 ClientSampleId :
 MW11

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	76.9	115.3
141	52.1	42.2	63.2

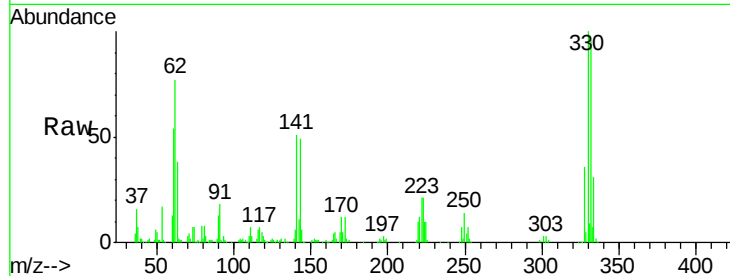


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

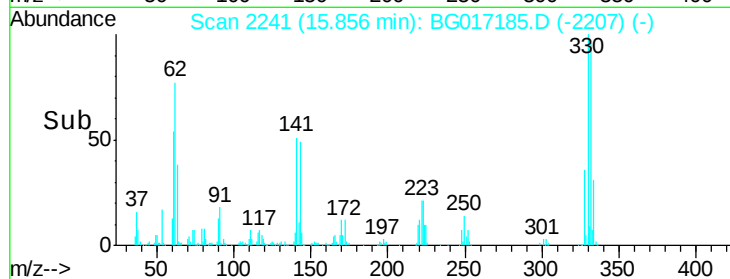
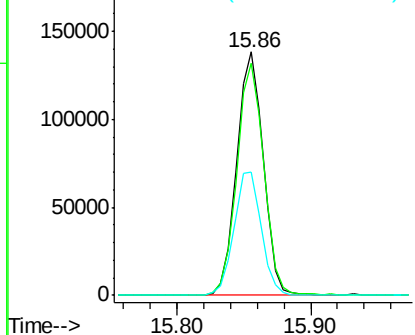



#44
 2-Fluorobiphenyl
 Concen: 84.16 ng
 RT: 12.98 min Scan# 1751
 Delta R.T. -0.00 min
 Lab File: BG017185.D
 Acq: 15 May 2015 20:42

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.7	44.5
170	23.5	18.4	27.6

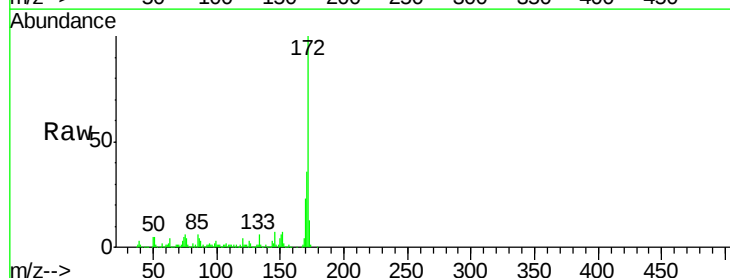

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

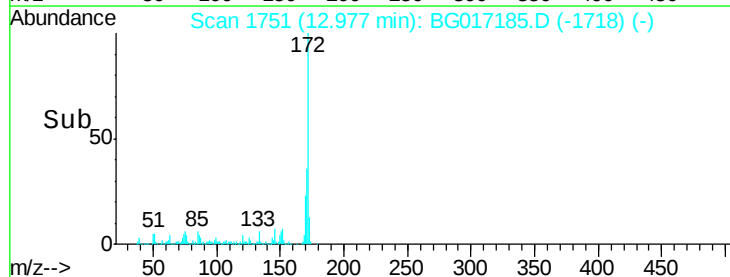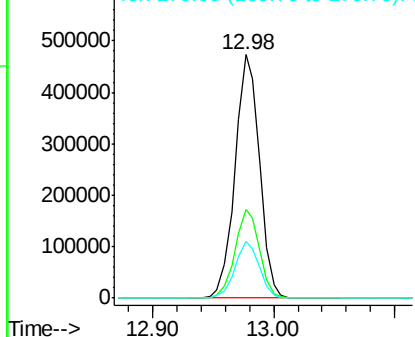

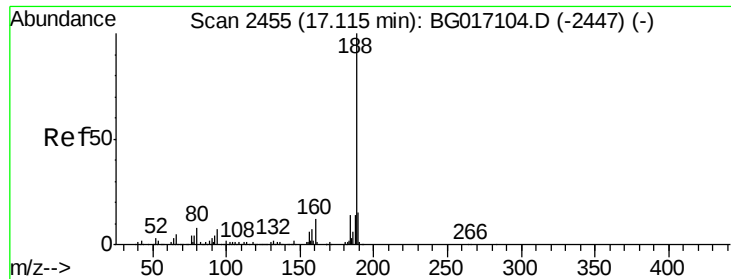

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.11 min Scan# 2454

Delta R.T. -0.00 min

Lab File: BG017185.D

Acq: 15 May 2015 20:42

Instrument :

BNA_G

ClientSampled :

MW11


Tgt Ion:188 Resp: 282457

Ion Ratio Lower Upper

188 100

94 10.1 5.8 8.6#




80 10.3 6.5 9.7#

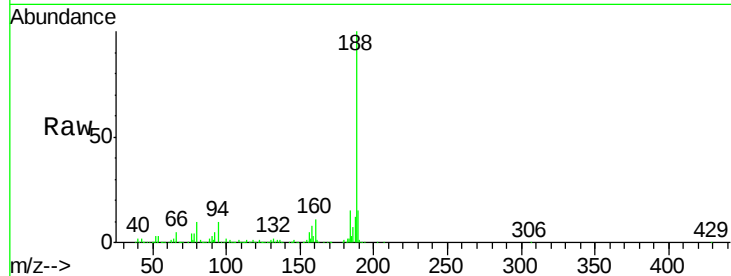

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

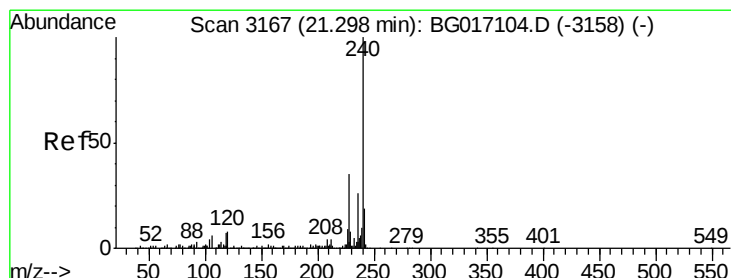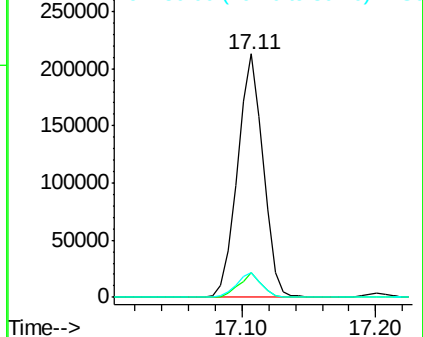

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.29 min Scan# 3166

Delta R.T. -0.00 min

Lab File: BG017185.D

Acq: 15 May 2015 20:42


Tgt Ion:240 Resp: 304985

Ion Ratio Lower Upper

240 100

120 10.0 6.0 9.0#



236 25.8 20.5 30.7

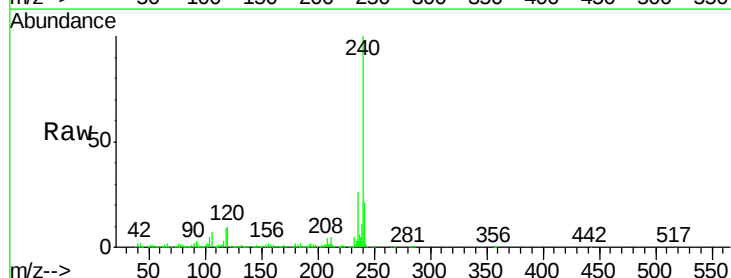


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

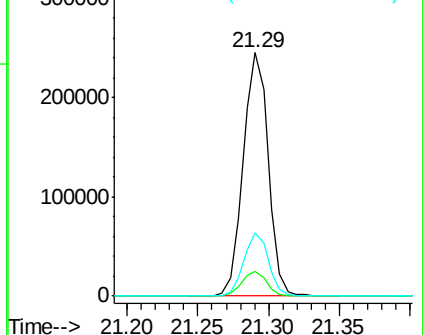



#78

Terphenyl-d14

Concen: 75.84 ng

RT: 19.74 min Scan# 2902

Delta R.T. -0.00 min

Lab File: BG017185.D

Acq: 15 May 2015 20:42

Instrument :

BNA_G

ClientSampleId :

MW11


Tgt Ion:244 Resp: 1109891

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.4




122 12.2 8.4 12.6

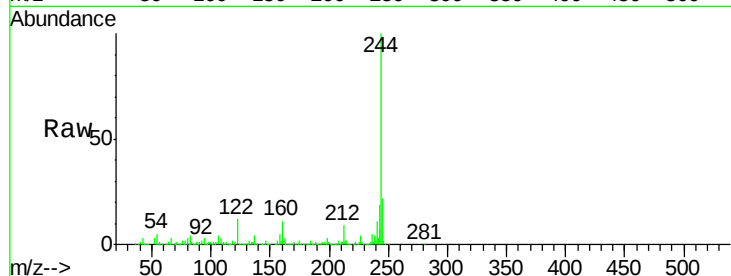

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

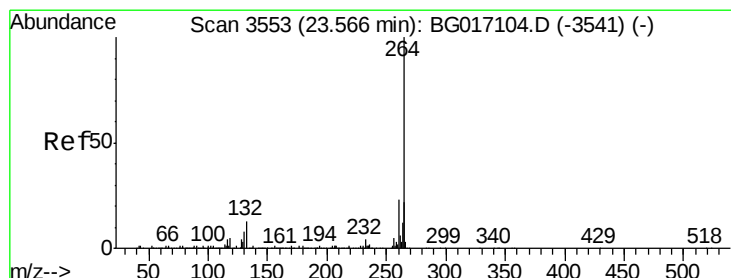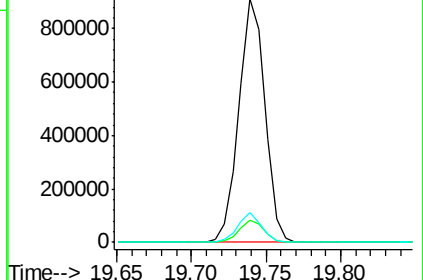

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.56 min Scan# 3552

Delta R.T. 0.00 min

Lab File: BG017185.D

Acq: 15 May 2015 20:42


Tgt Ion:264 Resp: 297364

Ion Ratio Lower Upper

264 100

260 24.9 18.0 27.0

265 21.4 17.4 26.0

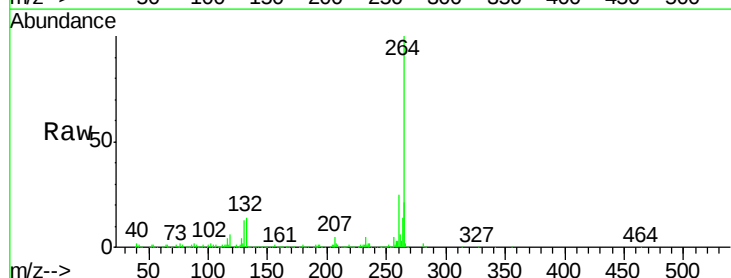

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

