


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051515\
 Data File : BG017171.D
 Acq On : 15 May 2015 11:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

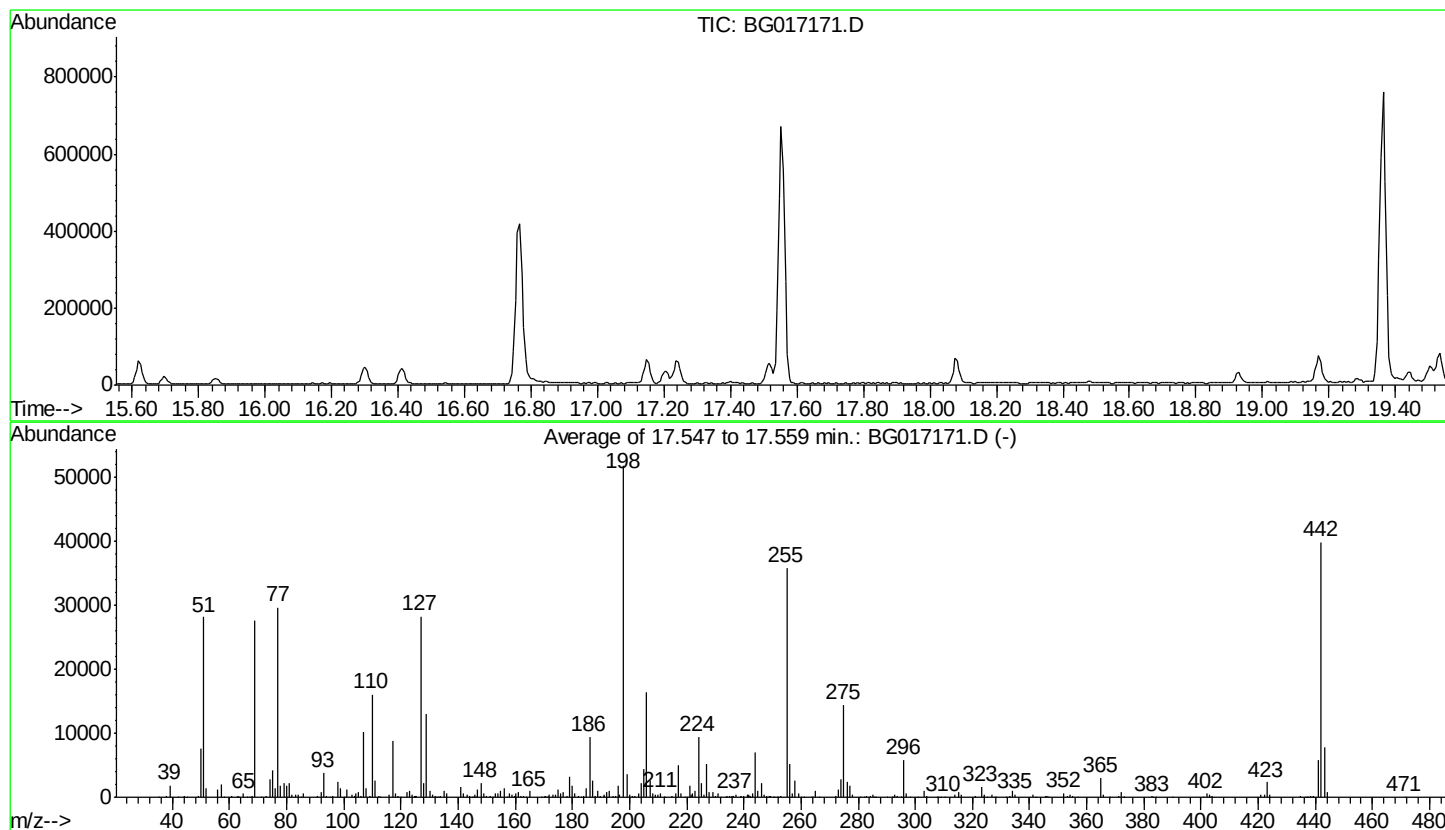

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	28209	PASS
68	69	0.00	2	1.1	299	PASS
69	198	0.00	100	53.4	27722	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.6	28333	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51872	PASS
199	198	5	9	7.0	3619	PASS
275	198	10	60	28.0	14509	PASS
365	198	1	100	5.9	3078	PASS
441	442	0.01	24	14.5	5787	PASS
442	198	50	100	77.0	39933	PASS
443	442	15	24	19.8	7899	PASS