
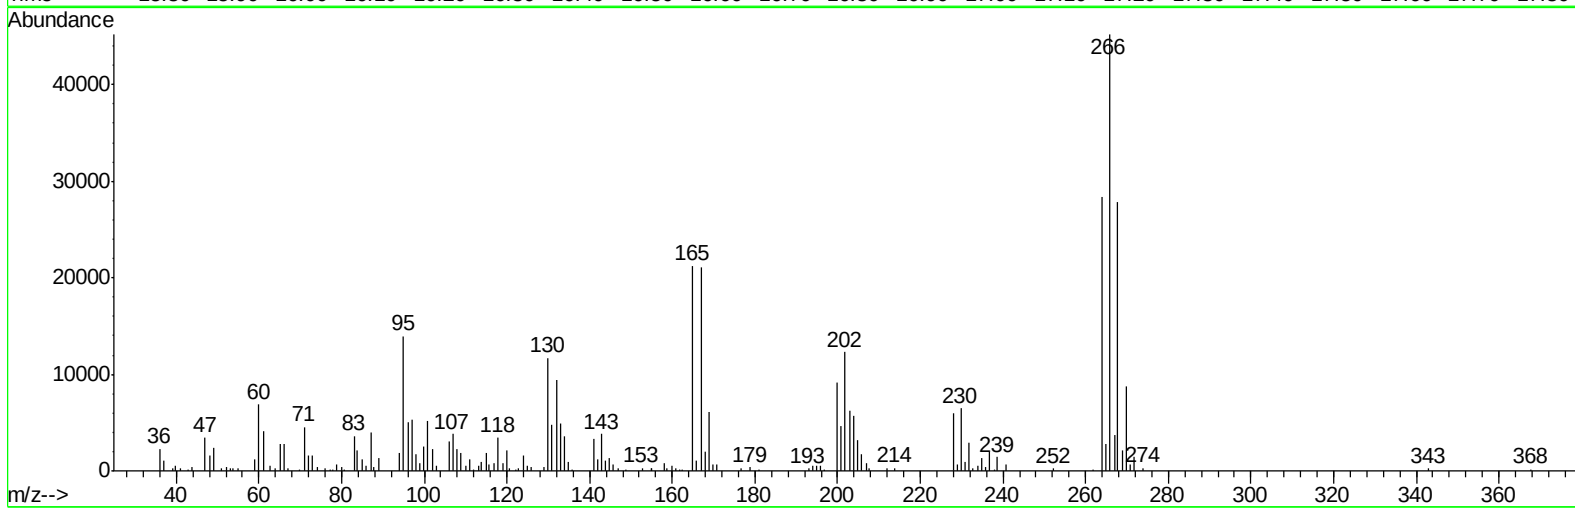


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051515\
Data File : BG017171.D
Acq On : 15 May 2015 11:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 03:36:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

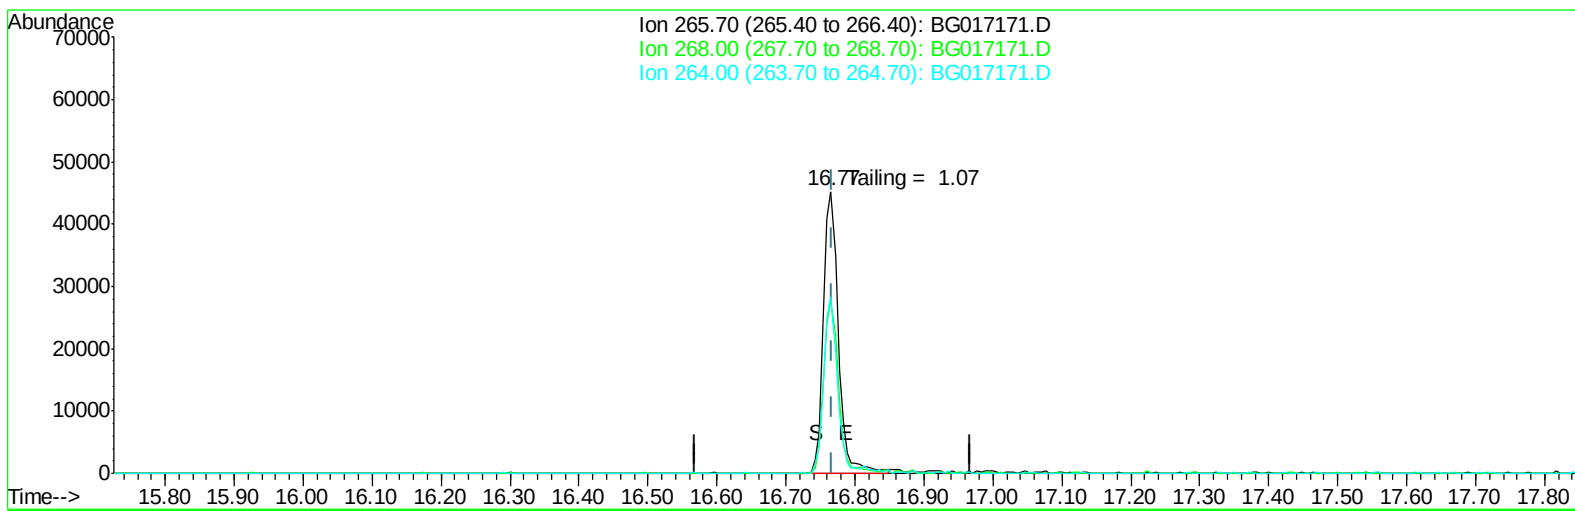

TIC: BG017171.D

(69) Pentachlorophenol (C)



16.766min (-0.003) 538.86ng

response 67781

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	61.53
264.00	61.70	62.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG051515\
Data File : BG017171.D
Acq On : 15 May 2015 11:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 03:36:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

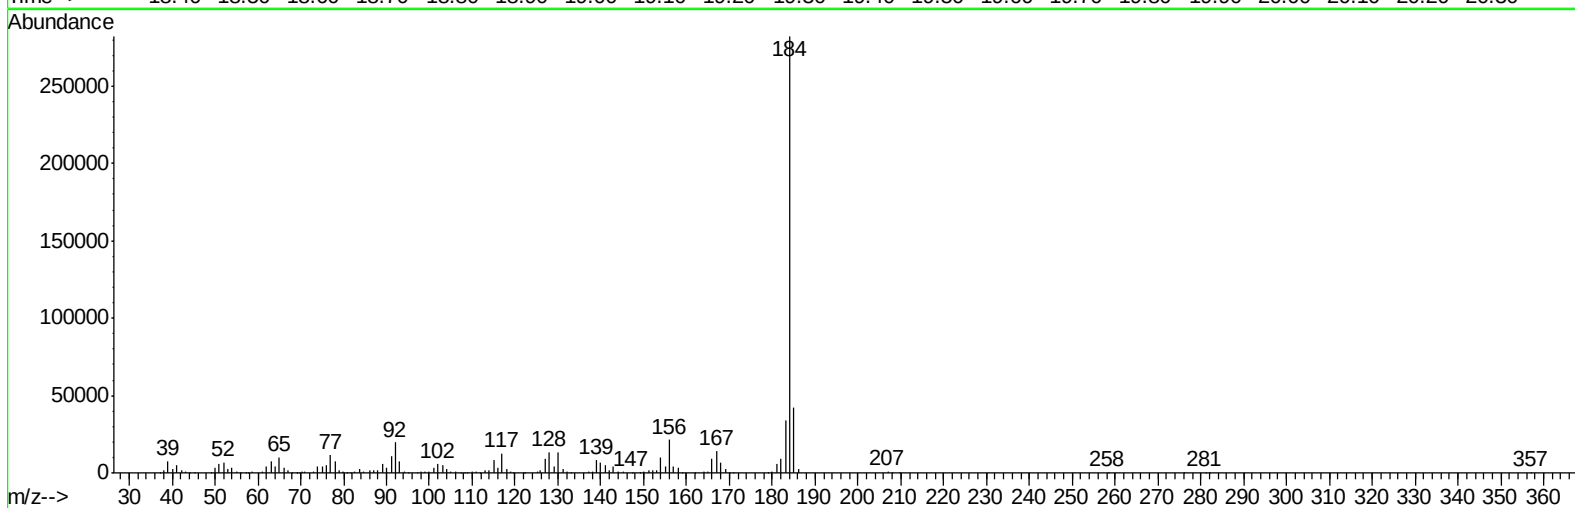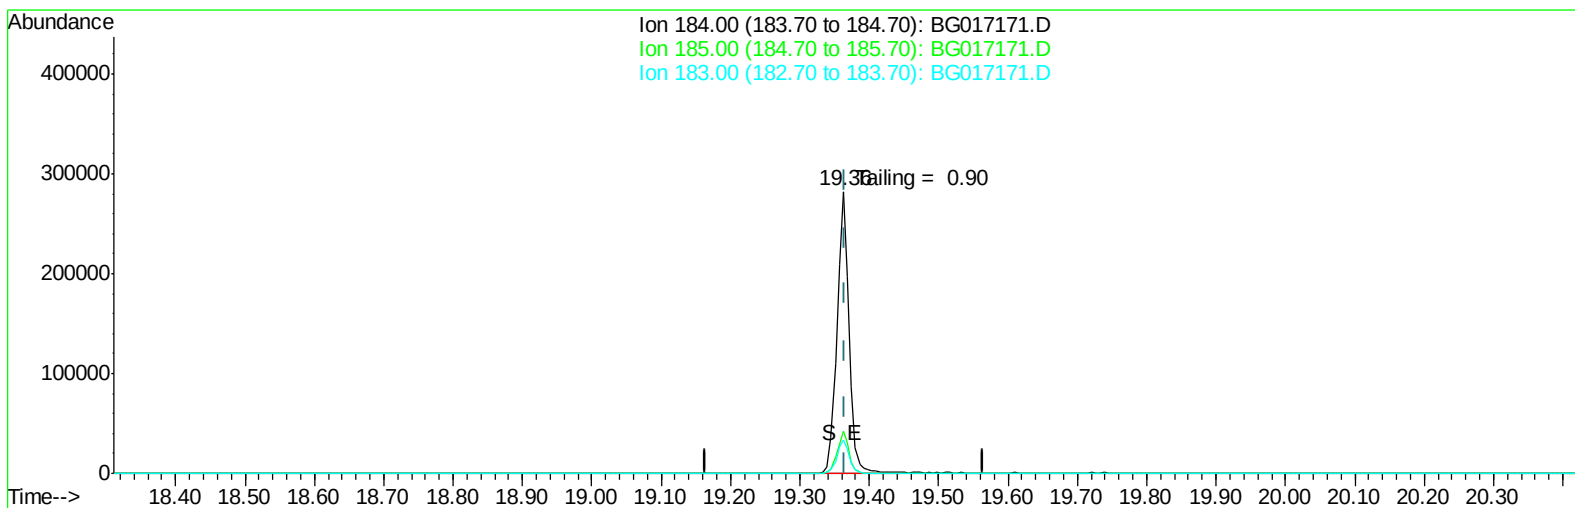

TIC: BG017171.D

(76) Benzidine

19.363min (-0.003) 139167.59ng

response 345328

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.91
183.00	14.30	12.03
0.00	0.00	0.00