
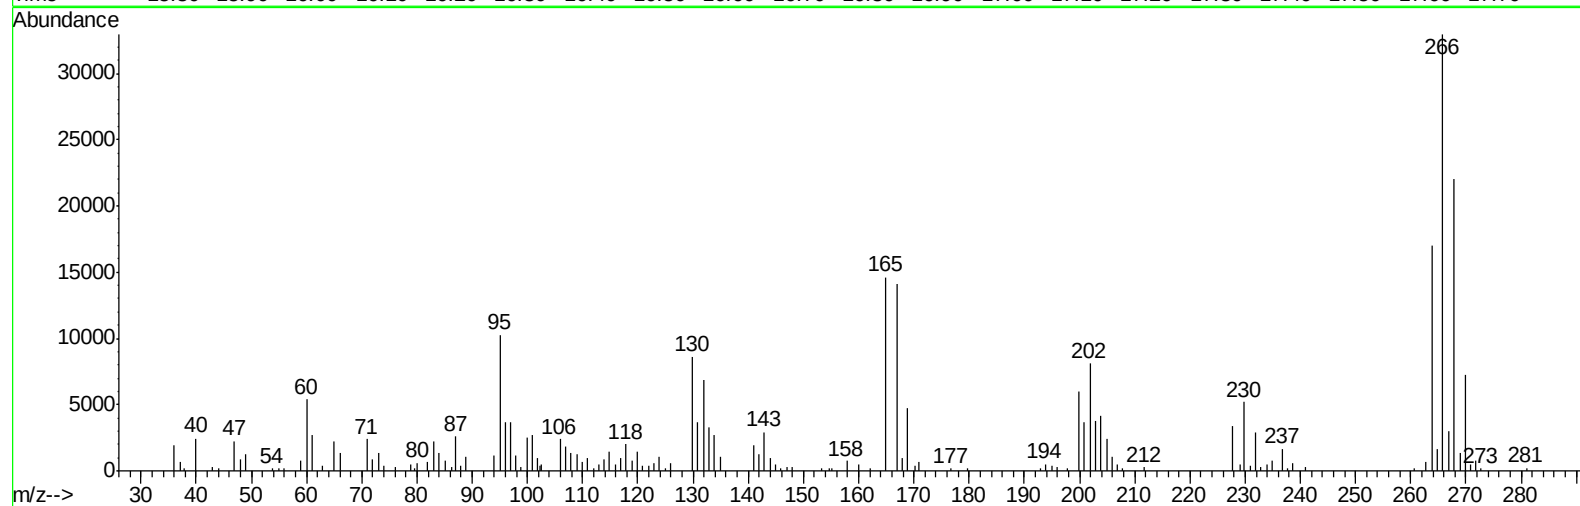


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051515\
Data File : BG017188.D
Acq On : 15 May 2015 23:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 09:23:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

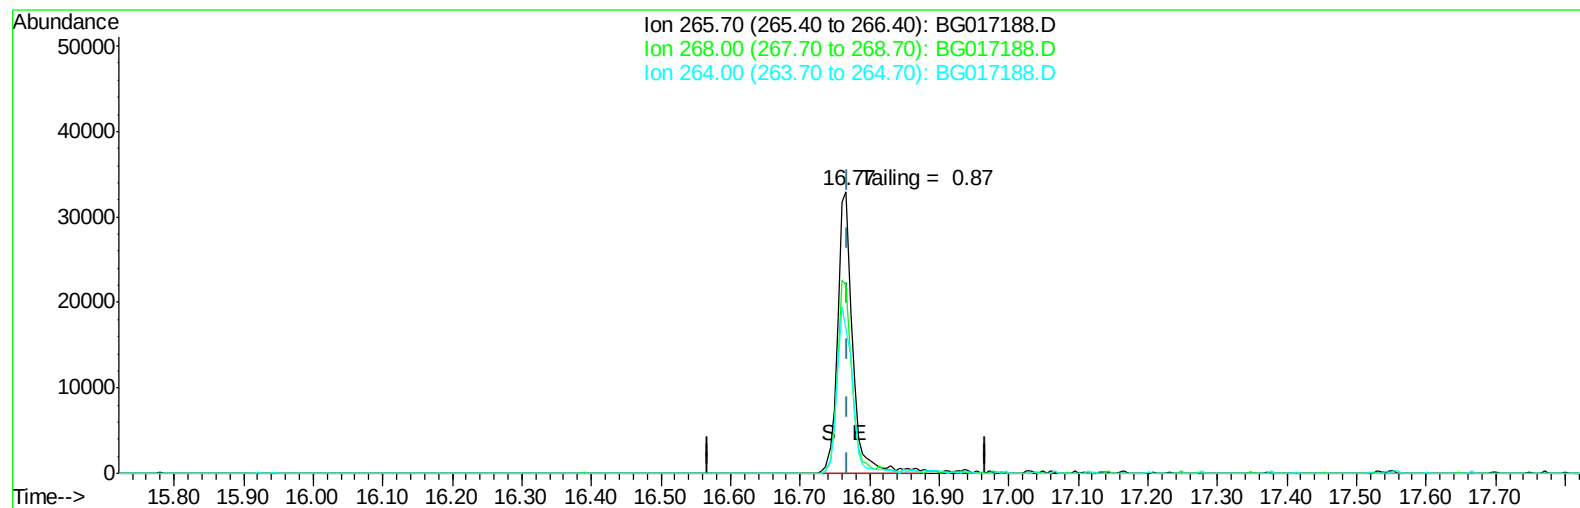

TIC: BG017188.D

(69) Pentachlorophenol (C)



16.766min (-0.002) 29678.24ng

response 47975

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	66.78
264.00	61.70	51.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG051515\
Data File : BG017188.D
Acq On : 15 May 2015 23:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 09:23:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

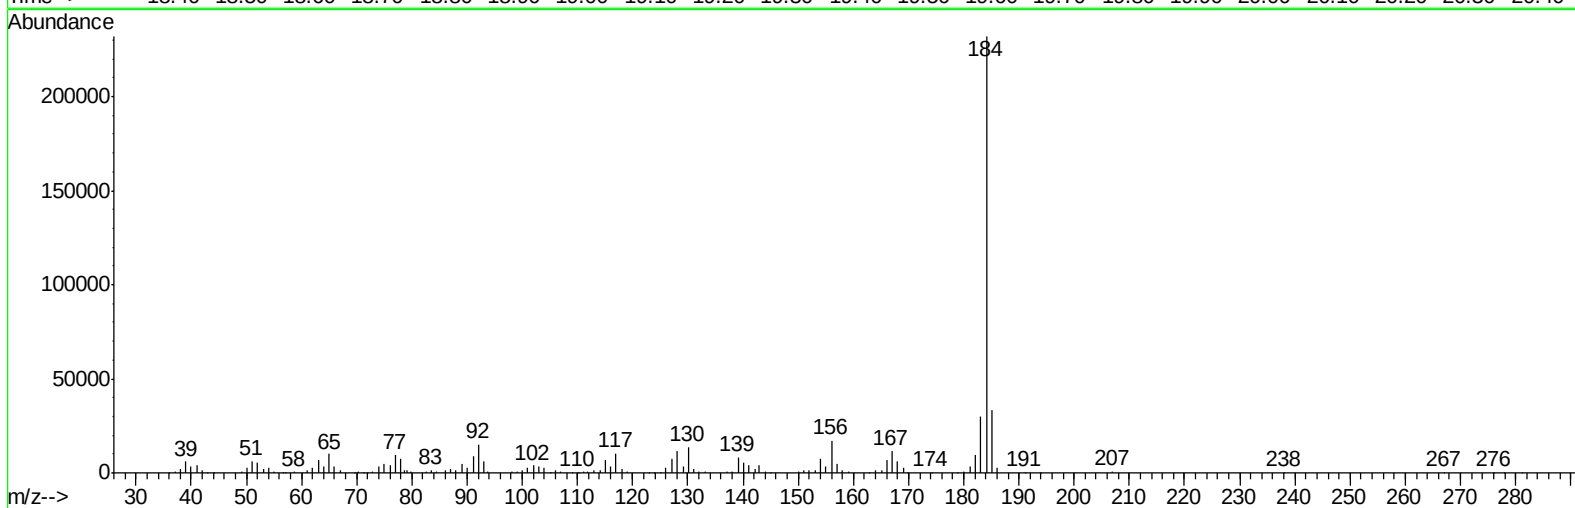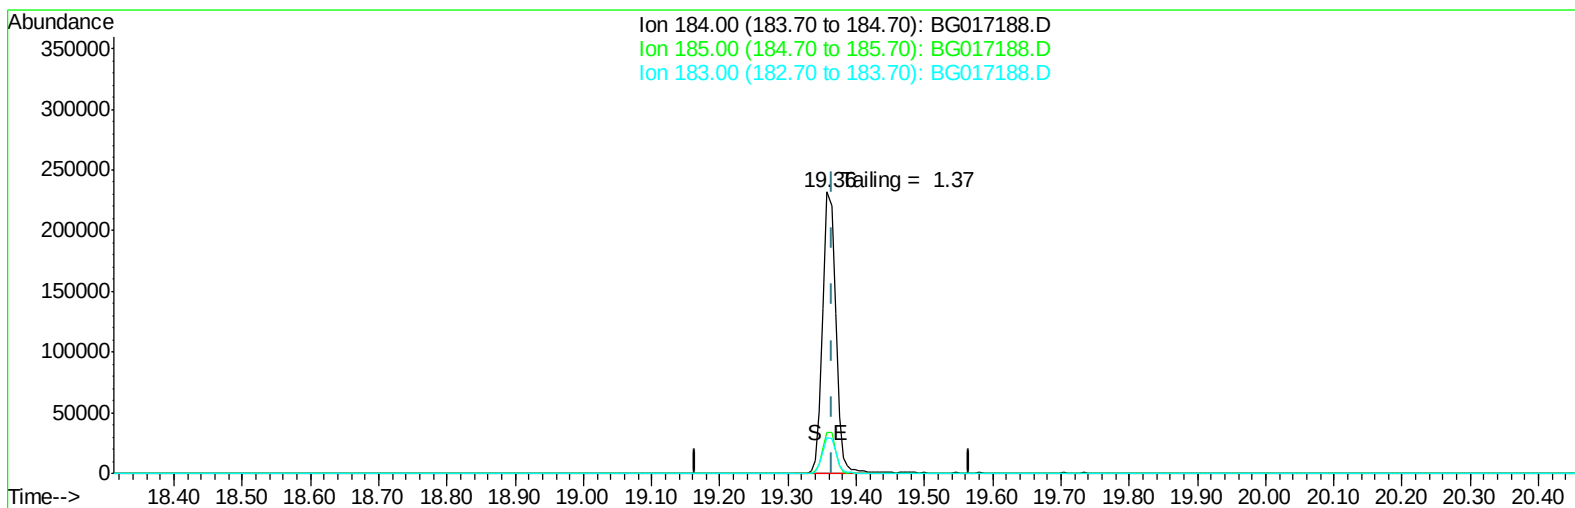

TIC: BG017188.D

(76) Benzidine

19.357min (-0.008) 26356.20ng

response 307207

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.46
183.00	14.30	12.96
0.00	0.00	0.00