
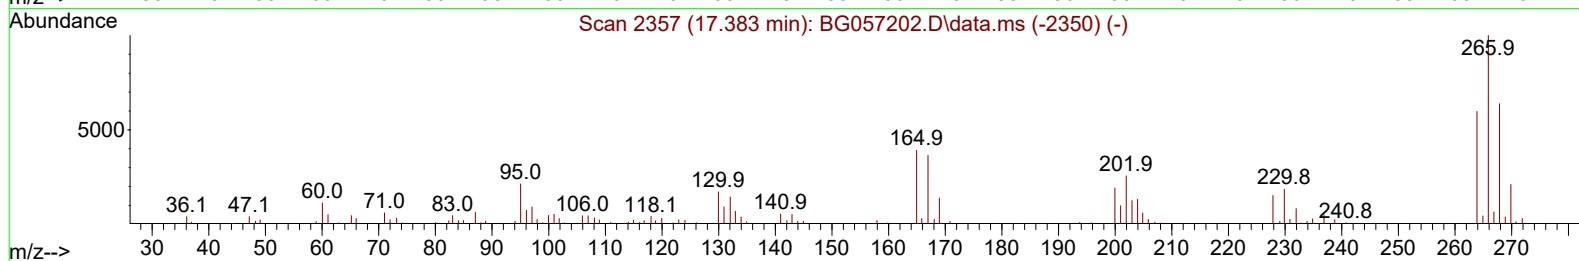
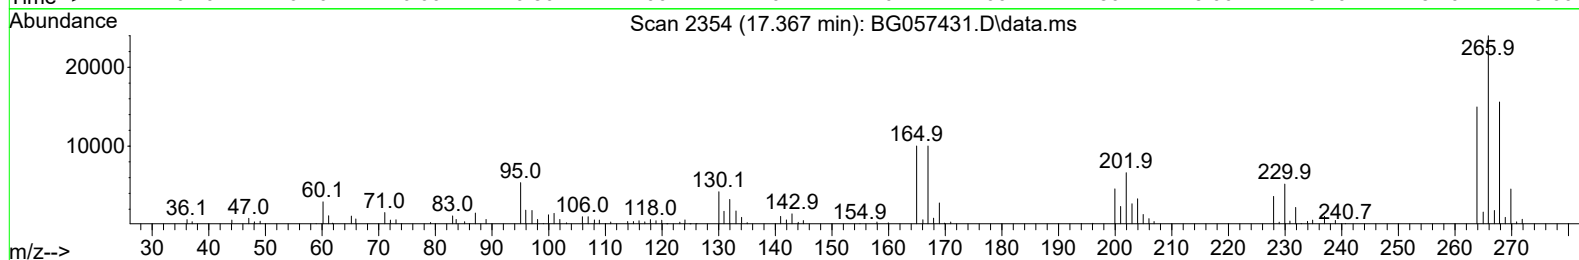


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051523\
Data File : BG057431.D
Acq On : 15 May 2023 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 07:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

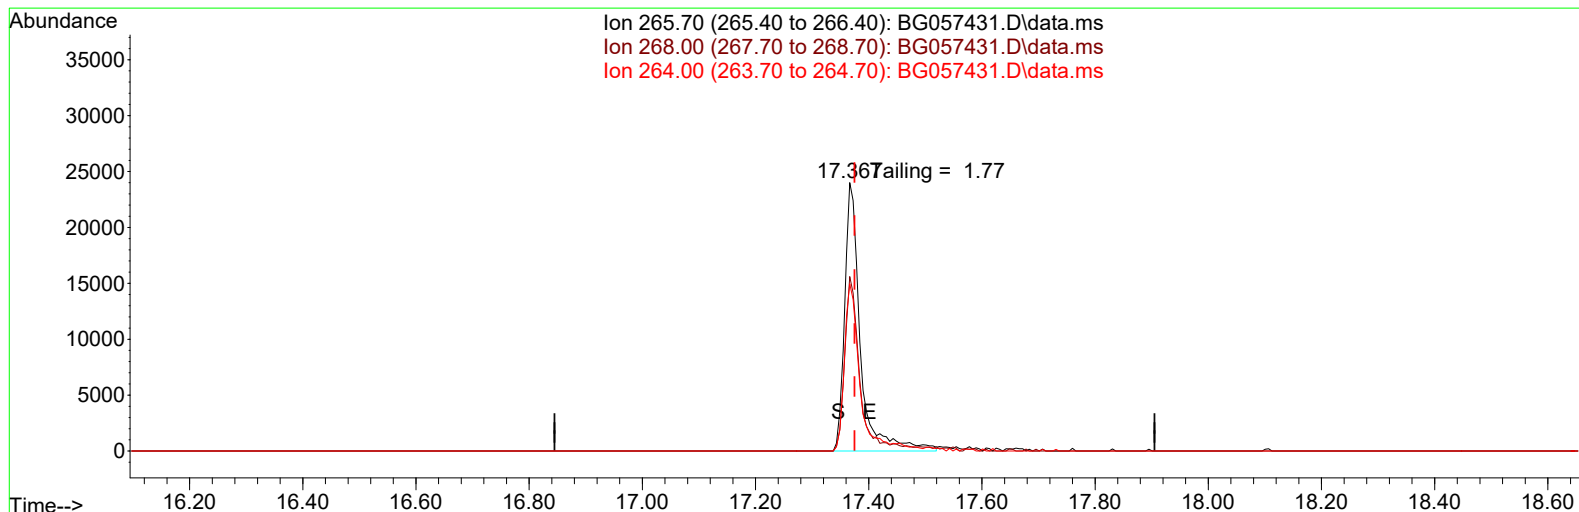

TIC: BG057431.D\data.ms

(70) Pentachlorophenol (C)




17.367min (-0.008) 36905.47 ng

response 45669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.00
264.00	59.70	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051523\
Data File : BG057431.D
Acq On : 15 May 2023 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 07:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

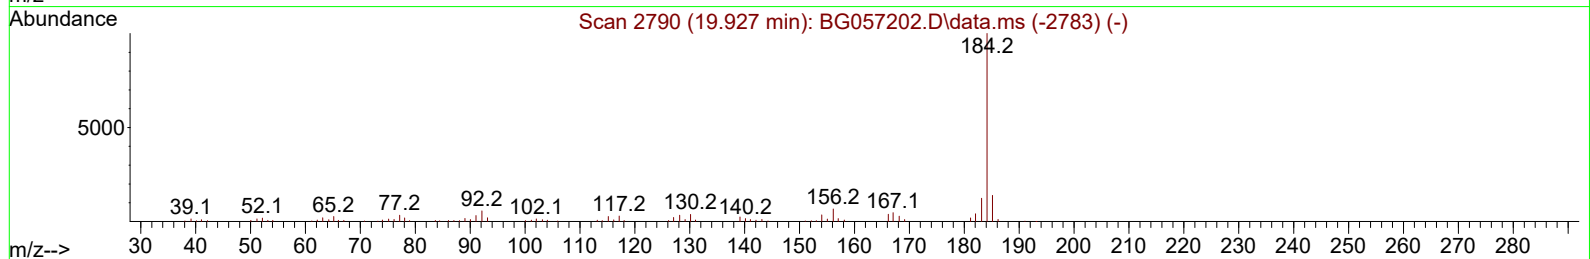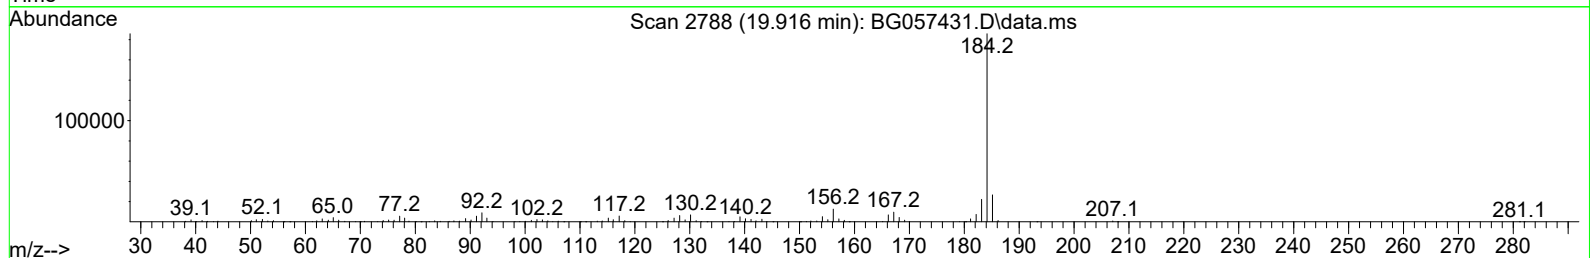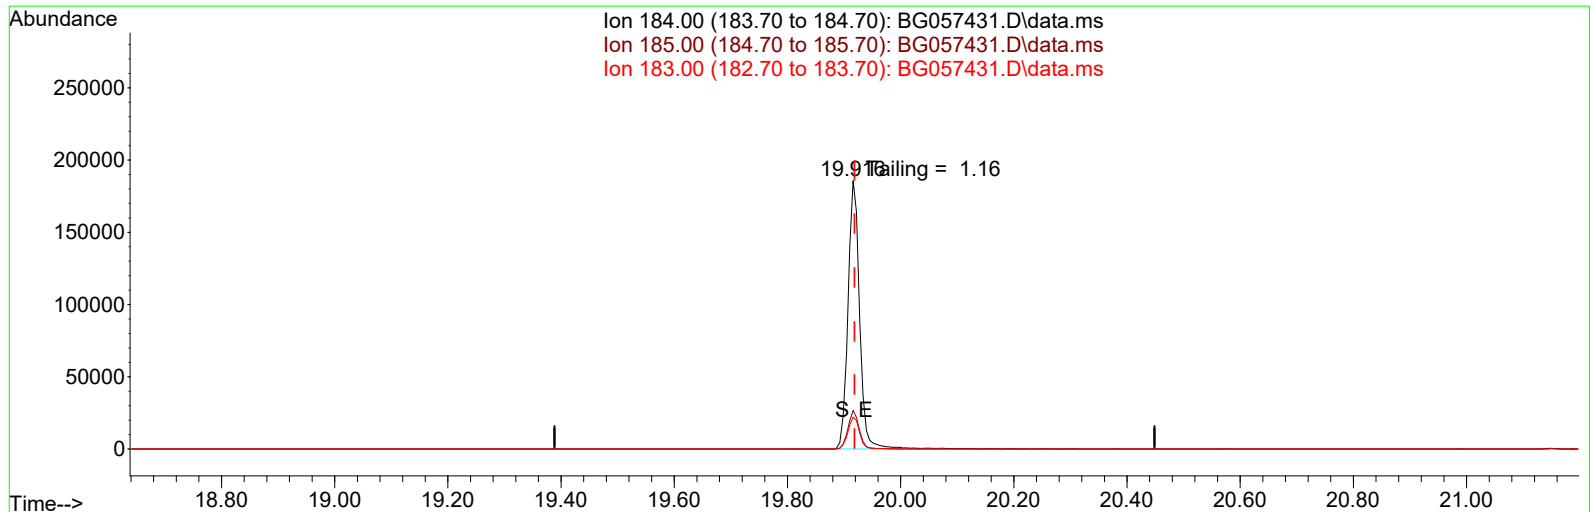

TIC: BG057431.D\data.ms

(77) Benzidine

19.916min (-0.002) 0.00 ng

response 264411

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.41
183.00	12.40	11.96
0.00	0.00	0.00