


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051523\
Data File : BG057431.D
Acq On : 15 May 2023 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 12 22:04:03 2023

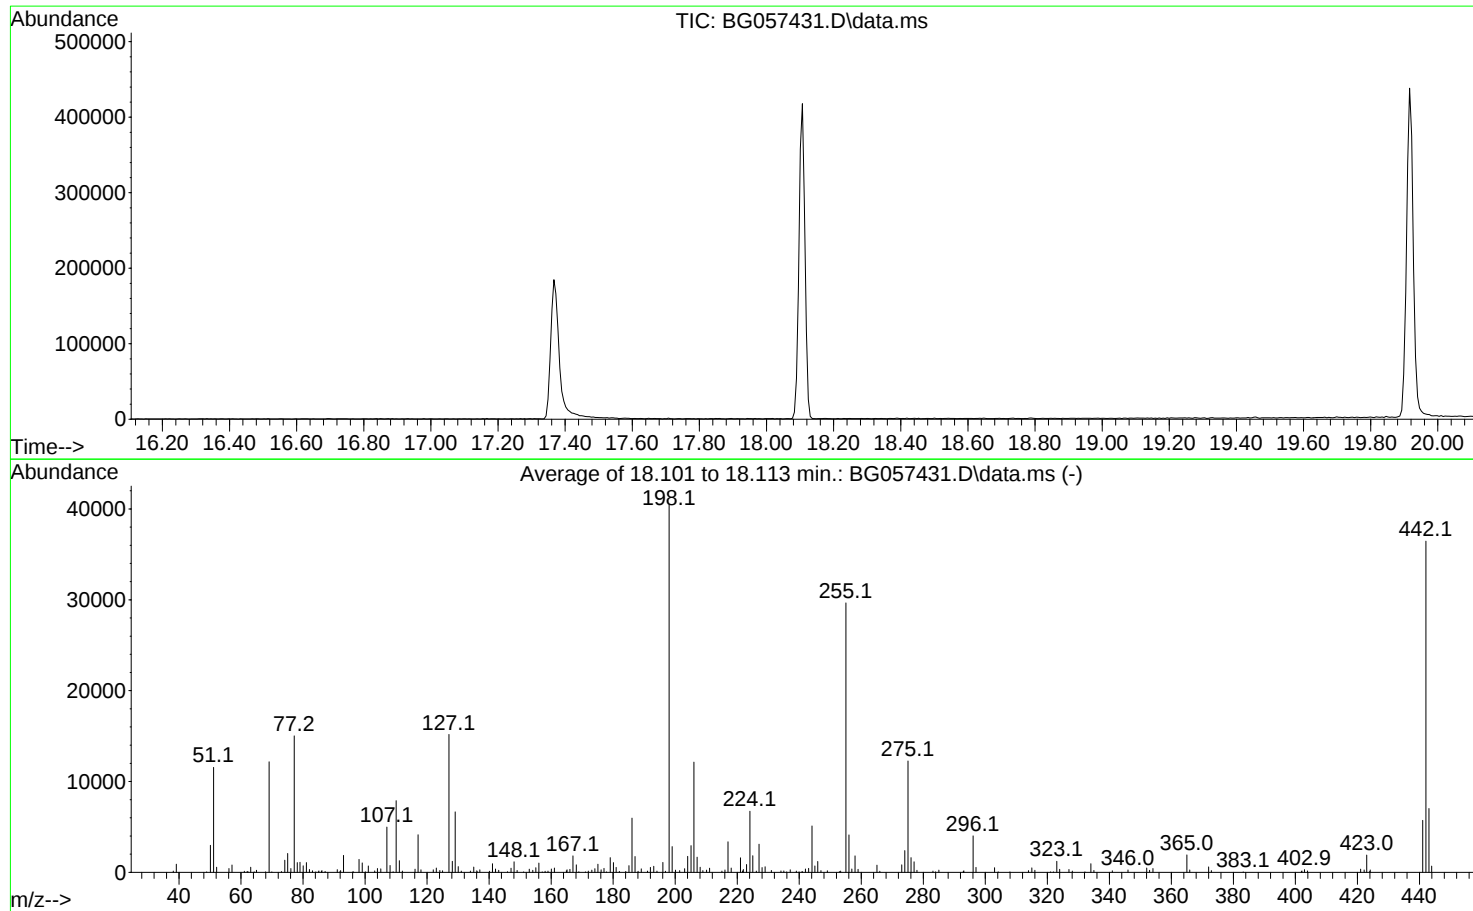




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	11560	PASS
68	69	0.00	2	0.5	61	PASS
69	198	0.00	100	30.0	12163	PASS
70	69	0.00	2	0.4	51	PASS
127	198	10	80	37.5	15174	PASS
197	198	0.00	2	0.3	127	PASS
198	198	100	100	100.0	40488	PASS
199	198	5	9	7.0	2833	PASS
275	198	10	60	30.3	12261	PASS
365	198	1	100	4.7	1917	PASS
441	198	0.01	100	14.1	5727	PASS
442	442	50	100	100.0	36459	PASS
443	442	15	24	19.3	7035	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051523\
Data File : BG057431.D
Acq On : 15 May 2023 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 07:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

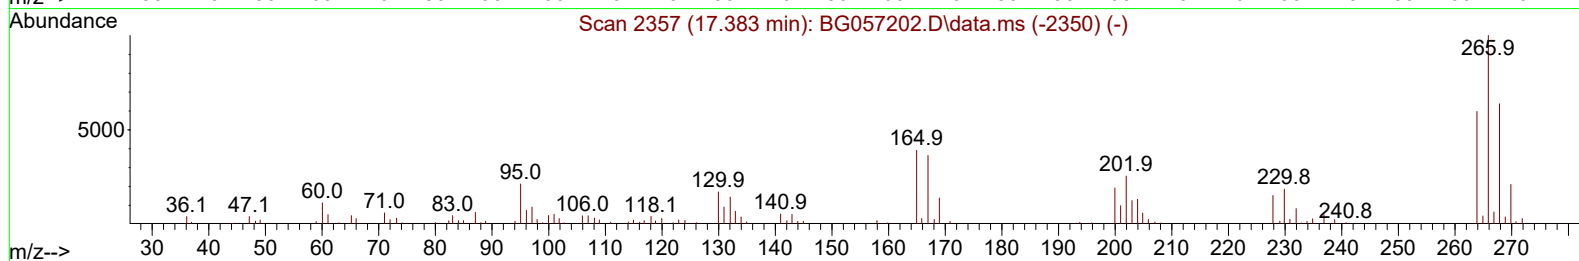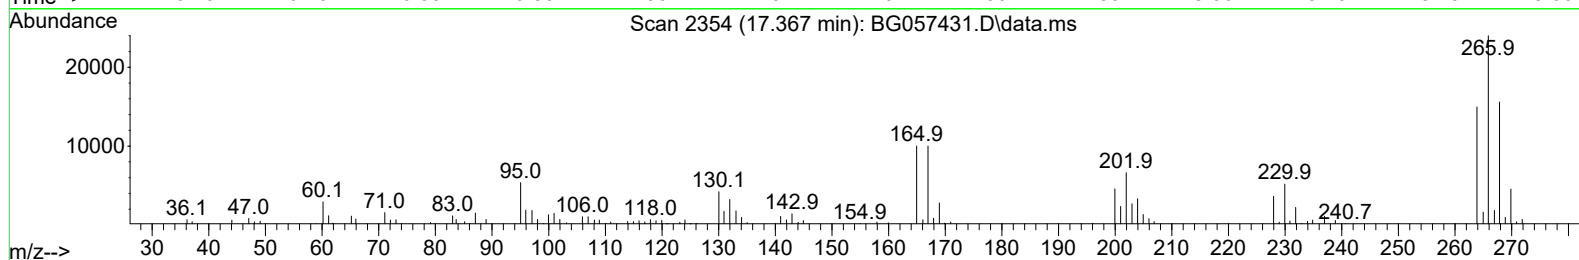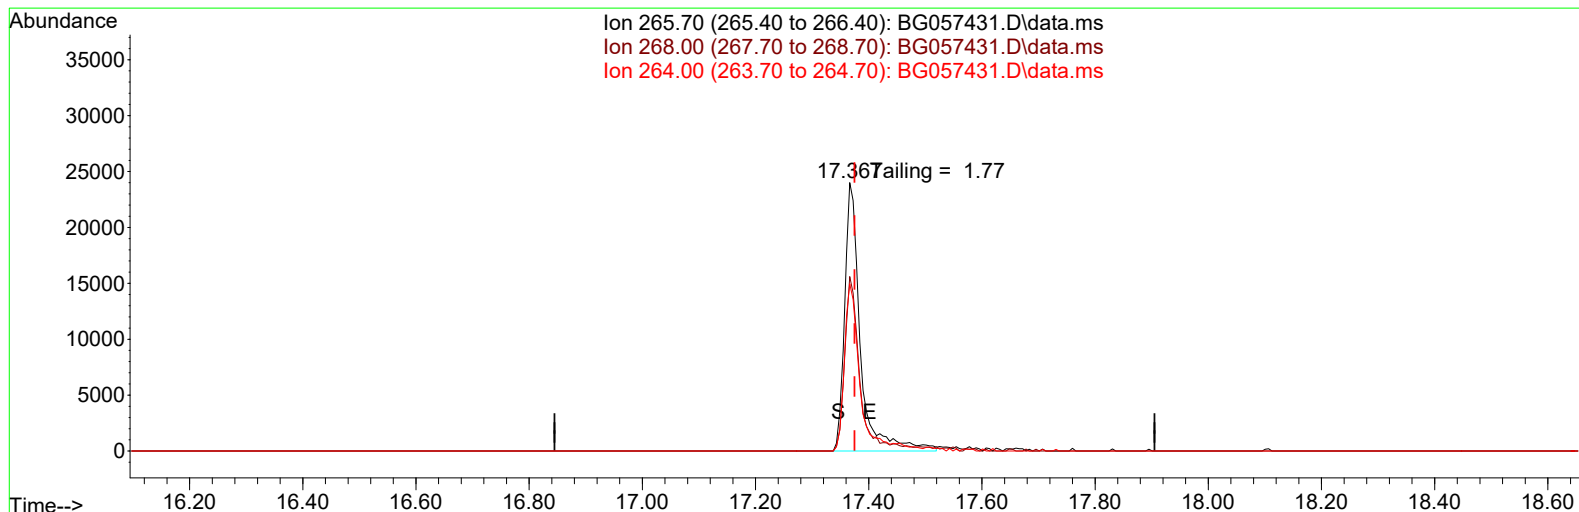

TIC: BG057431.D\data.ms

(70) Pentachlorophenol (C)

17.367min (-0.008) 36905.47 ng




response 45669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.00
264.00	59.70	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051523\
Data File : BG057431.D
Acq On : 15 May 2023 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 07:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

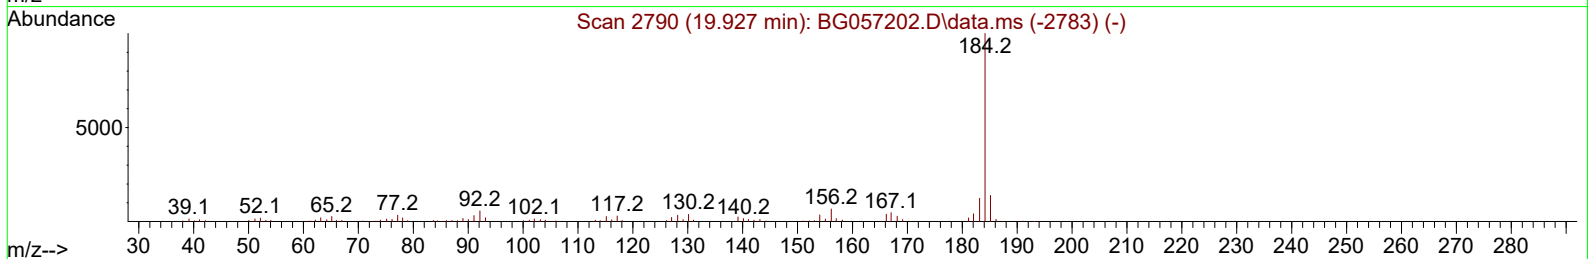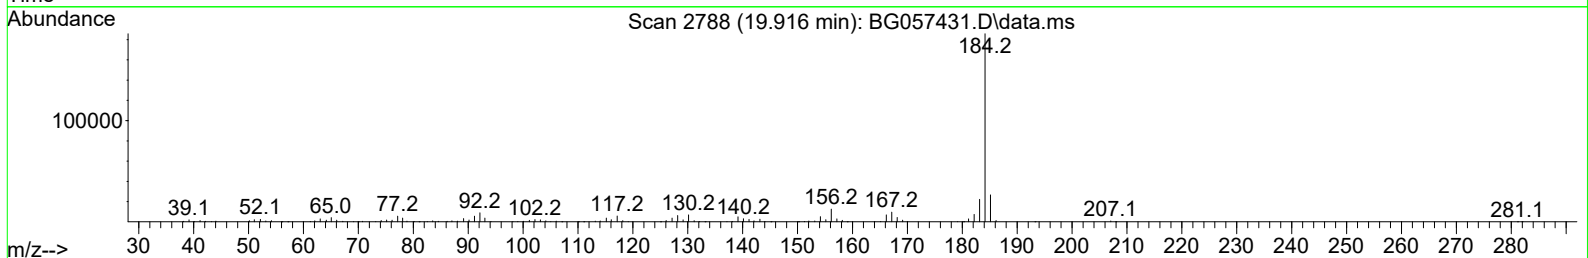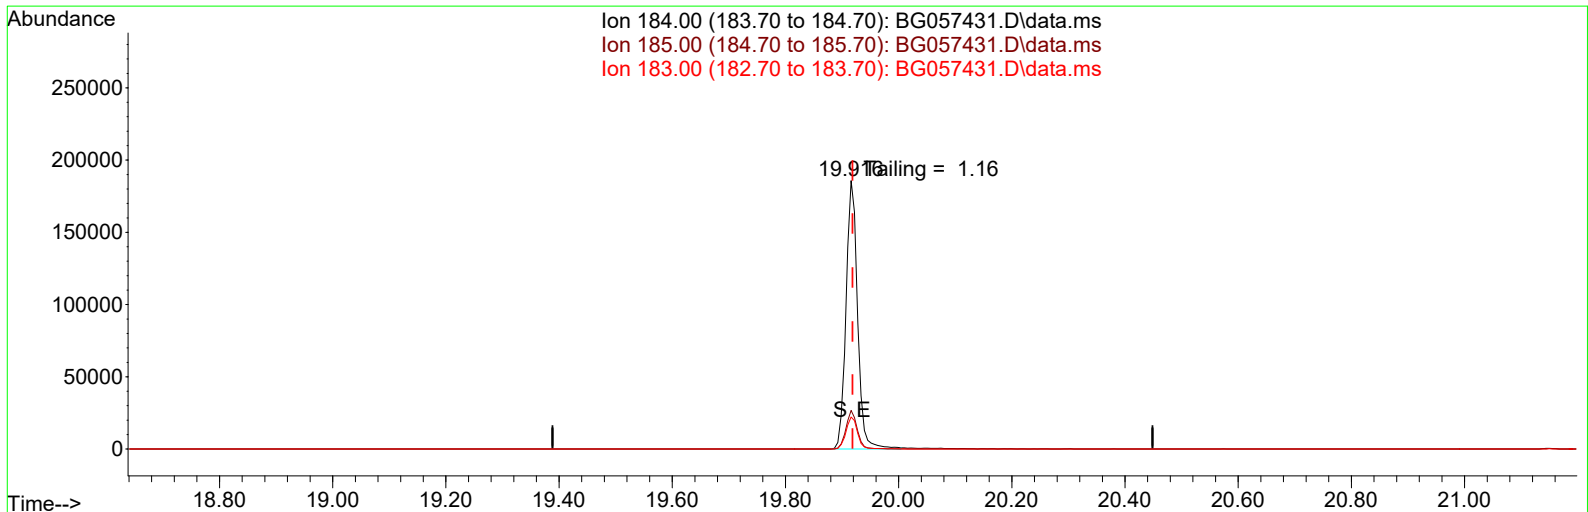

TIC: BG057431.D\data.ms

(77) Benzidine

19.916min (-0.002) 0.00 ng

response 264411

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.41
183.00	12.40	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/15/2023	BNA_G	<u>BG057431.D</u>
Compound Name	Response	Retention Time
DDT	136405	21.15
DDD	2545	20.744
DDE	135	20.192
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2680	139085	1.93

Instrument :
BNA_G
ClientSampleId :
DFTPP