

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051616\
 Data File : BG021914.D
 Acq On : 16 May 2016 20:05
 Operator : UM/SJ
 Sample : H3095-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9XE2

Quant Time: May 17 01:37:26 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 01:35:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	70481	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	335920	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.79	164	192999	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.54	188	394071	20.00	ng/ul	0.00
76) Chrysene-d12	21.83	240	378634	20.00	ng/ul	0.01
84) Perylene-d12	25.18	264	383256	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	4791	3.28	ng/uL	0.00
5) Phenol-d5	7.32	99	105215	20.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	53213	20.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	99639	24.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	74616	16.99	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	51889	23.50	ng/ul	0.01
22) 2-Nitrophenol-d4	10.06	143	58079	41.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	101928	25.84	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	57875	13.62	ng/ul	0.00
44) Dimethylphthalate-d6	14.19	166	324774	23.96	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	453213	23.55	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	16555	7.12	ng/ul	0.02
58) Fluorene-d10	15.78	176	307494	21.54	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	26978	24.71	ng/ul	0.01
71) Anthracene-d10	17.64	188	431289	22.48	ng/ul	0.00
77) Pyrene-d10	19.91	212	444584	25.08	ng/ul	0.00
88) Benzo(a)pyrene-d12	24.94	264	424554	23.31	ng/ul	0.02

Target Compounds


					Ovalue	
4) Benzaldehyde	7.30	77	916	1.61	ng/ul#	37
28) Naphthalene	11.04	128	20952	1.24	ng/ul	99
34) 2-Methylnaphthalene	12.64	142	16527	1.33	ng/ul	96
35) 1-Methylnaphthalene	12.85	142	13539	1.10	ng/ul#	98
45) Dimethylphthalate	14.24	163	132916	9.63	ng/ul	98
70) Phenanthrene	17.58	178	143980	6.68	ng/ul	96
72) Anthracene	17.67	178	26340	1.20	ng/ul	96
74) Di-n-butylphthalate	18.48	149	103256	5.99	ng/ul#	95
75) Fluoranthene	19.58	202	302969	12.38	ng/ul	96
78) Pyrene	19.95	202	266759	12.18	ng/ul	97
79) Butylbenzylphthalate	20.82	149	1236629	255.37	ng/ul#	81
81) Benzo(a)anthracene	21.80	228	157963	7.50	ng/ul	96
82) Bis(2-ethylhexyl)phthalate	21.69	149	205457	25.99	ng/ul	97
83) Chrysene	21.87	228	166457	7.99	ng/ul	94
86) Benzo(b)fluoranthene	24.11	252	258746	11.79	ng/ul#	94
87) Benzo(k)fluoranthene	24.11	252	258746	11.02	ng/ul#	94
89) Benzo(a)pyrene	25.01	252	164593	7.54	ng/ul#	94
90) Indeno(1,2,3-cd)pyrene	29.01	276	96130	3.71	ng/ul#	90
92) Benzo(g,h,i)perylene	30.19	276	41661	1.95	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051616\
Data File : BG021914.D
Acq On : 16 May 2016 20:05
Operator : UM/SJ
Sample : H3095-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9XE2

Quant Time: May 17 01:37:26 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 01:35:08 2016
Response via : Initial Calibration

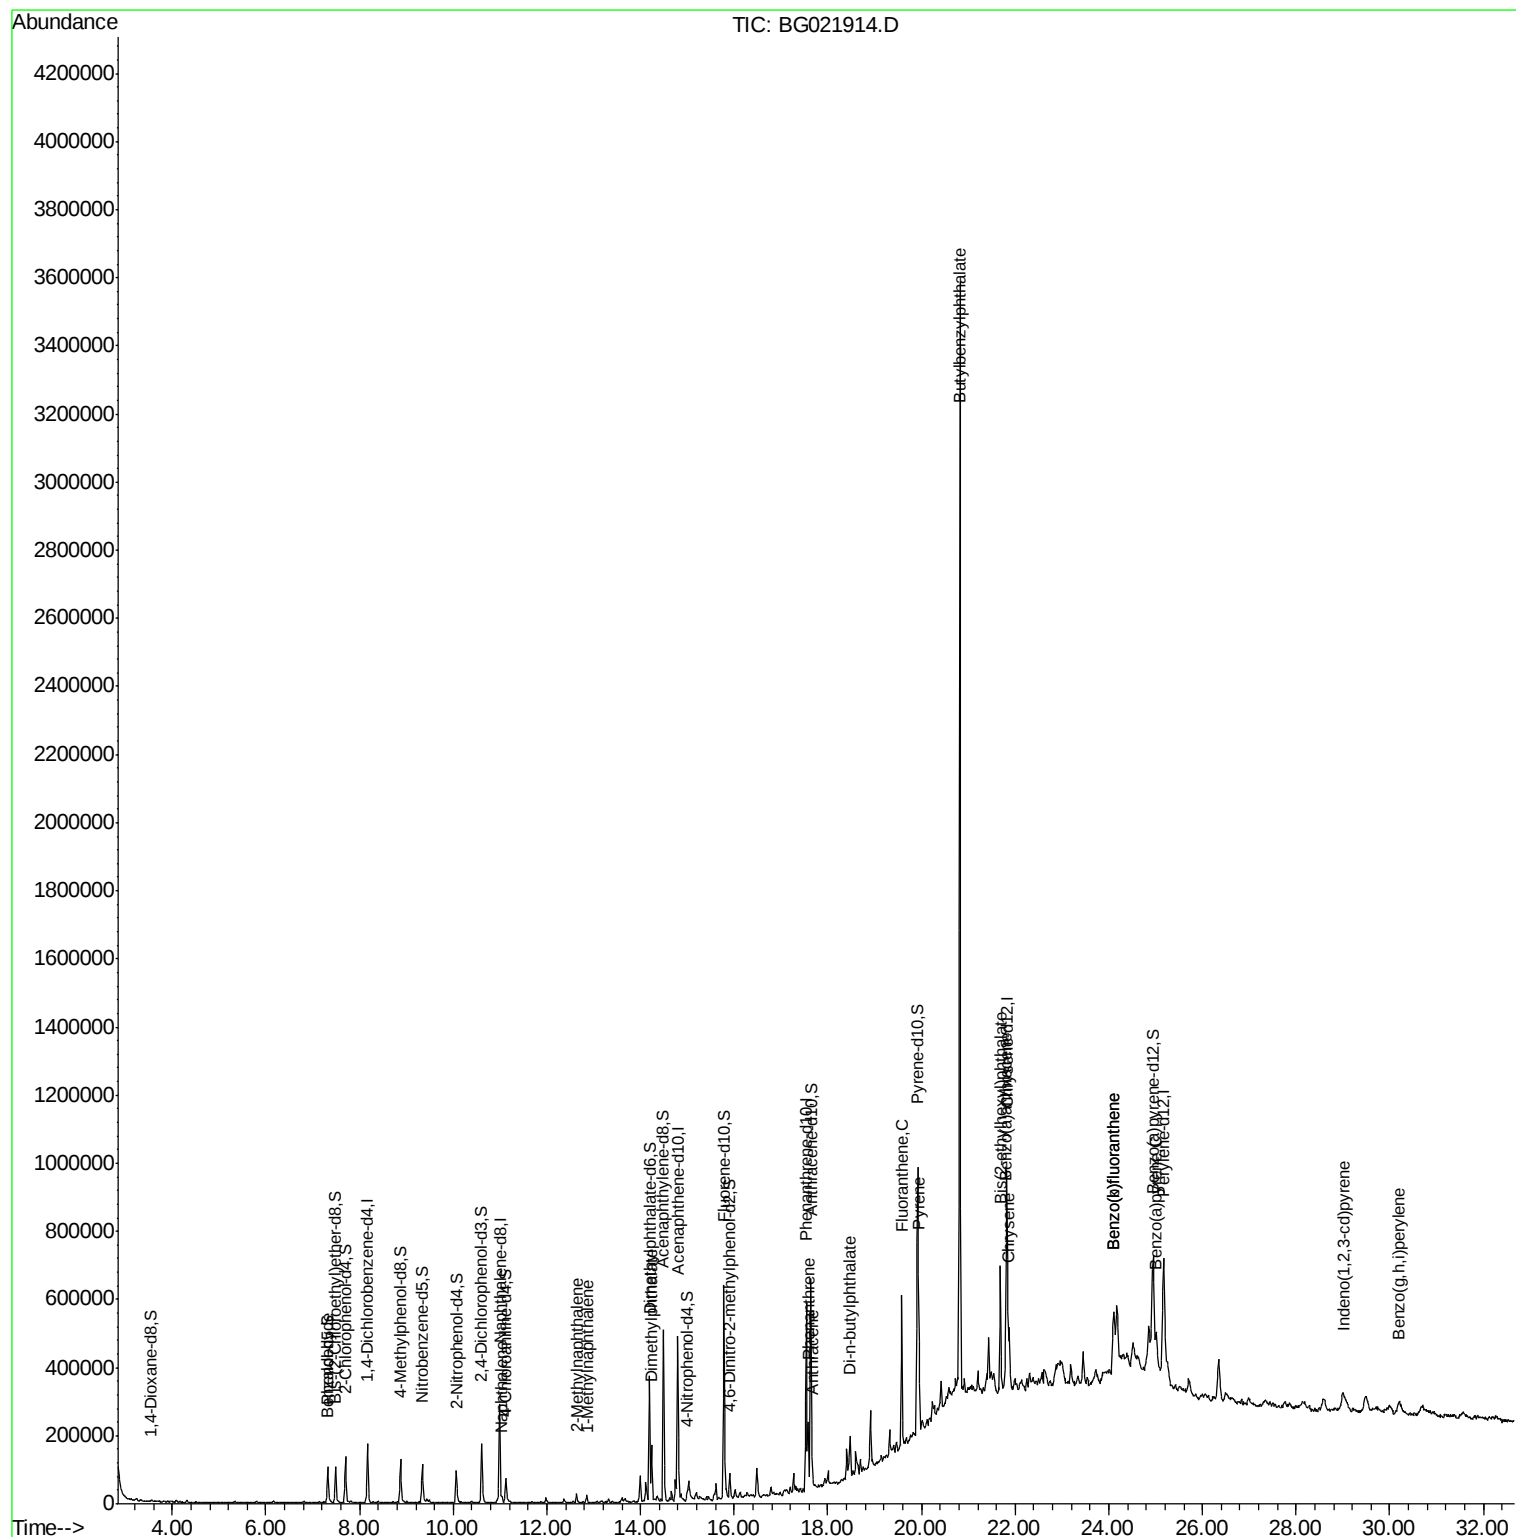

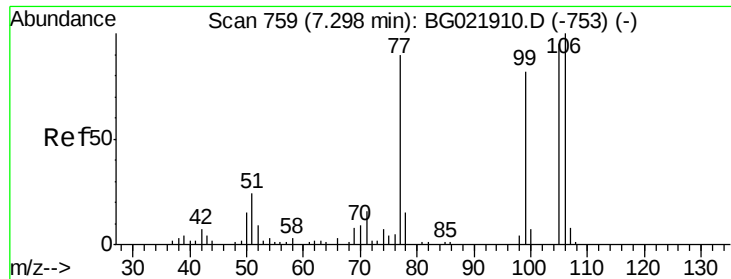

#4

Benzaldehyde

Concen: 1.61 ng/ul

RT: 7.30 min Scan# 760

Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Instrument :

BNA_G

ClientSampleId :

D9XE2





Tot Ion: 77 Resp: 916

Ion Ratio Lower Upper

77 100

105 190.8 68.5 102.7#

106 89.2 65.0 97.4

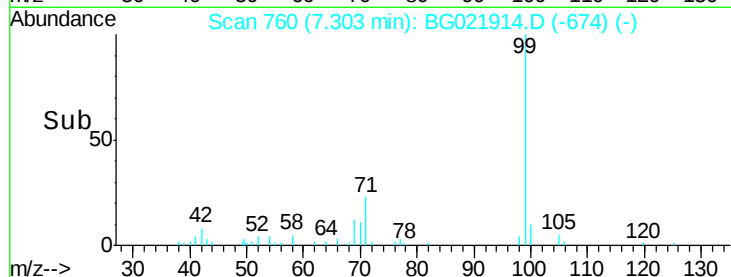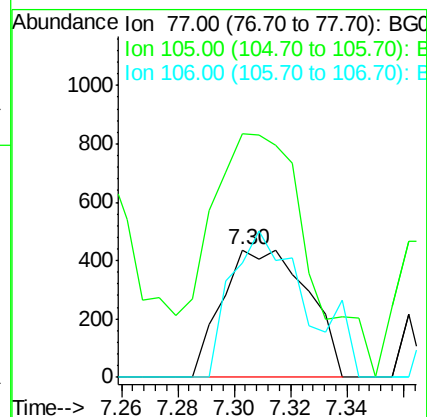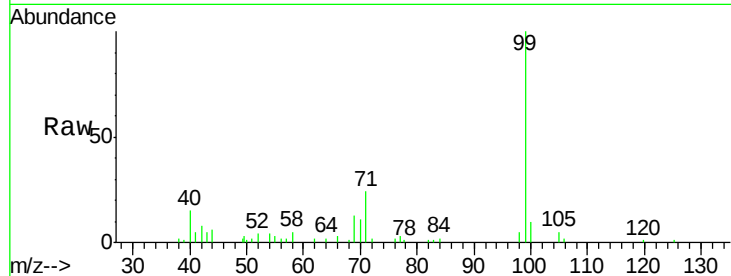

#28

Naphthalene

Concen: 1.24 ng/ul

RT: 11.04 min Scan# 1396

Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05




Tgt Ion: 128 Resp: 20952


Ion Ratio Lower Upper

128 100

129 10.3 8.3 12.5

127 13.0 10.8 16.2


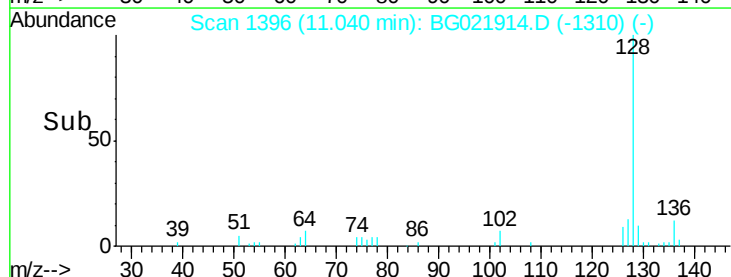
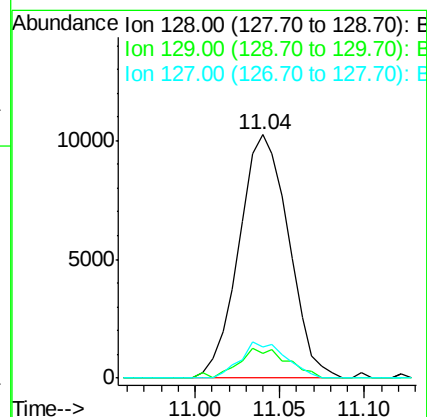



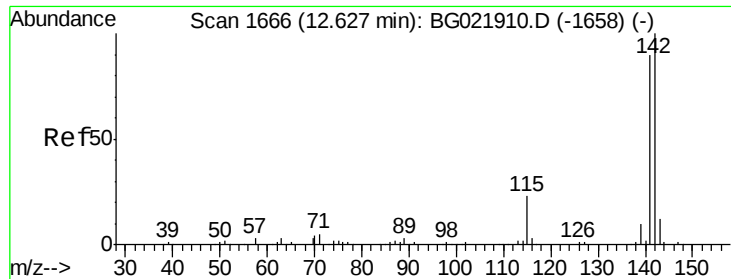

#34
2-Methylnaphthalene
Concen: 1.33 ng/ul
RT: 12.64 min Scan# 1668
Delta R.T. 0.01 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05




Instrument :
BNA_G
ClientSampleId :
D9XE2


Tot Ion:142 Resp: 16527
Ion Ratio Lower Upper
142 100
141 85.6 71.3 106.9

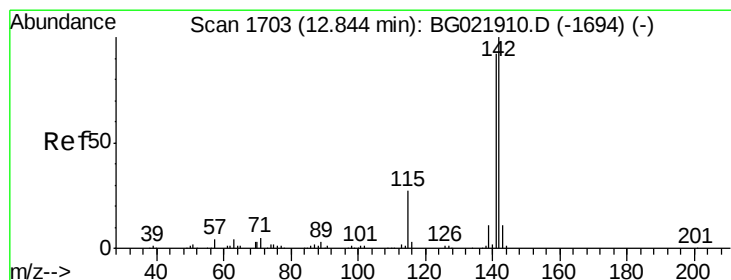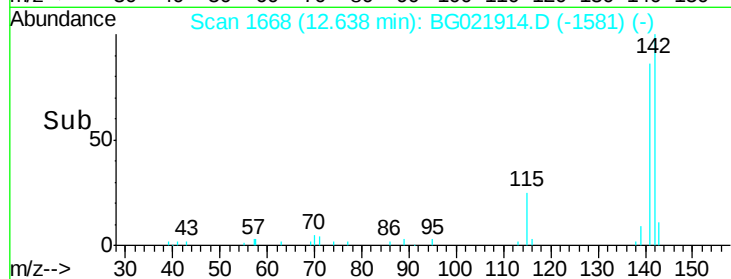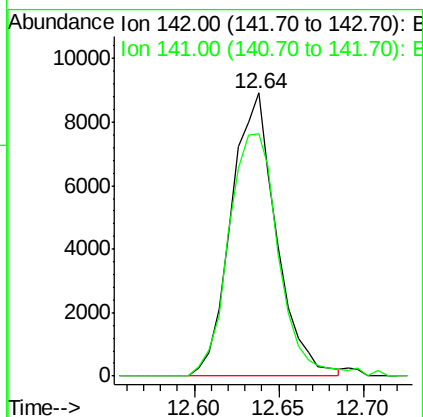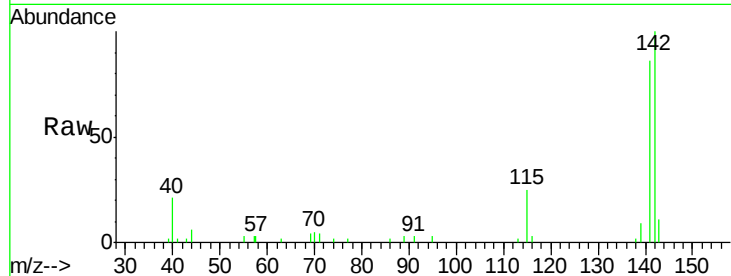

#35
1-Methylnaphthalene
Concen: 1.10 ng/ul
RT: 12.85 min Scan# 1704
Delta R.T. 0.01 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05

Tgt Ion:142 Resp: 13539
Ion Ratio Lower Upper
142 100
141 94.2 77.0 115.4
116 2.8 4.2 6.4#


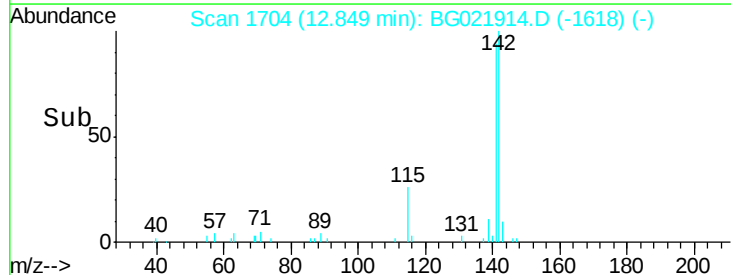
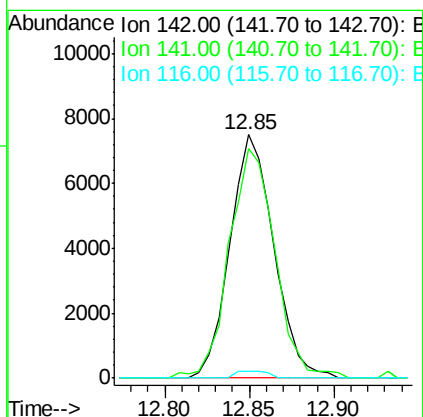



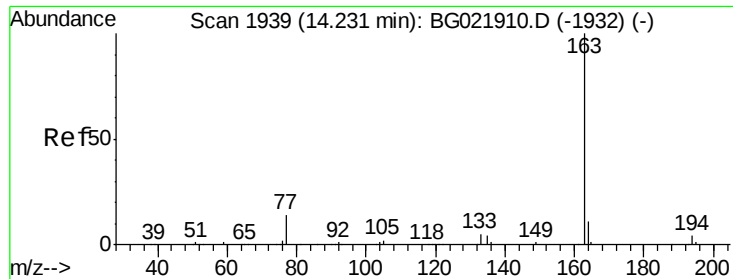

#45
Dimethylphthalate
Concen: 9.63 ng/ul
RT: 14.24 min Scan# 1940
Delta R.T. 0.01 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05




Instrument :
BNA_G
ClientSampleId :
D9XE2


Tot Ion:163 Resp: 132916
Ion Ratio Lower Upper
163 100
194 4.8 3.9 5.9
164 9.7 8.7 13.1

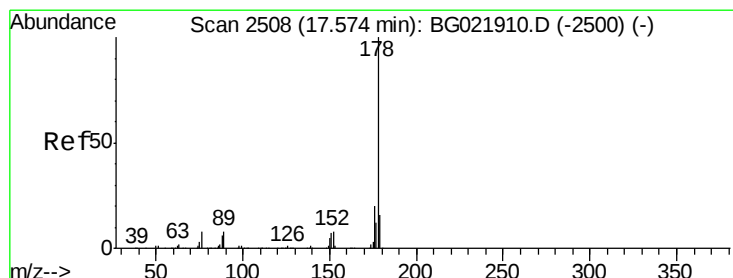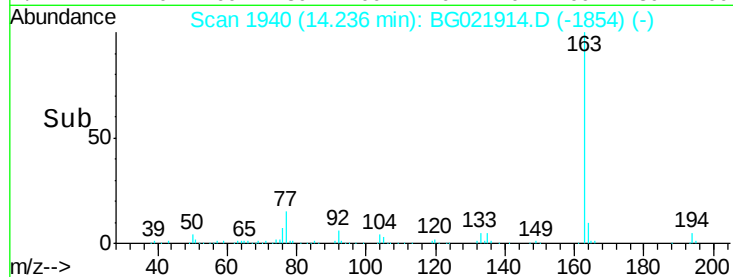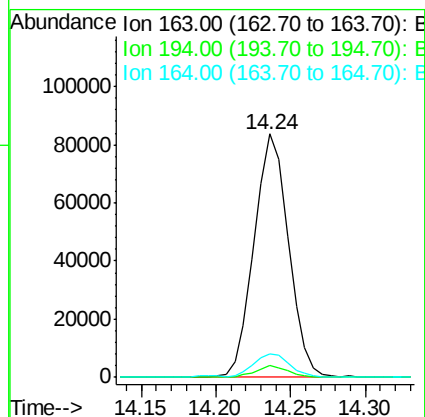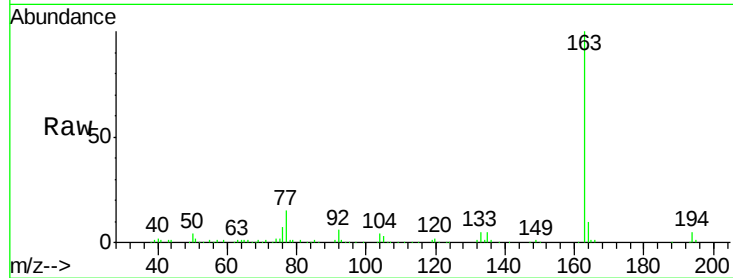

#70
Phenanthrene
Concen: 6.68 ng/ul
RT: 17.58 min Scan# 2509
Delta R.T. 0.01 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05

Tgt Ion:178 Resp: 143980
Ion Ratio Lower Upper
178 100
179 16.6 11.8 17.8
176 19.8 14.8 22.2

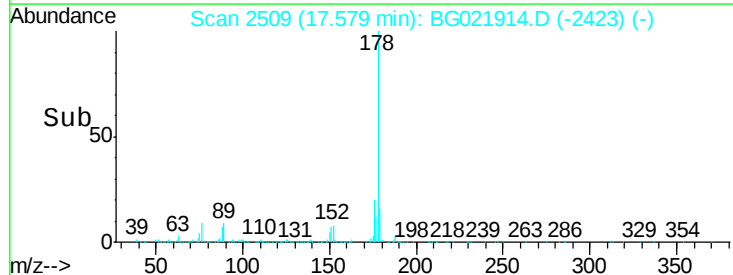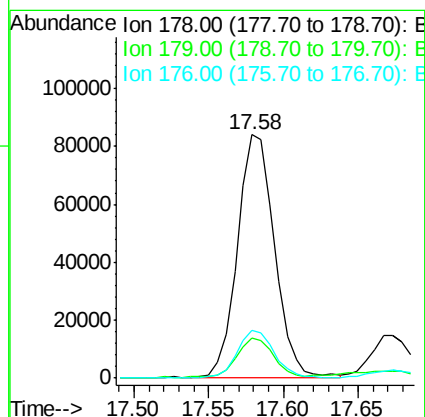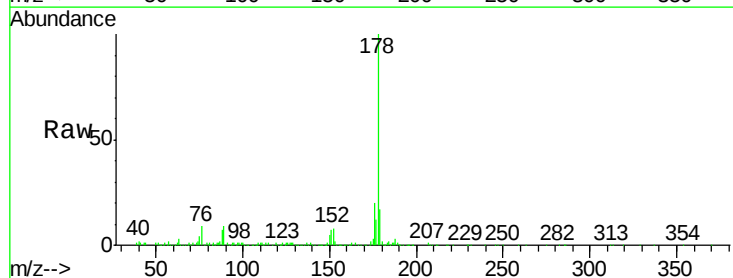

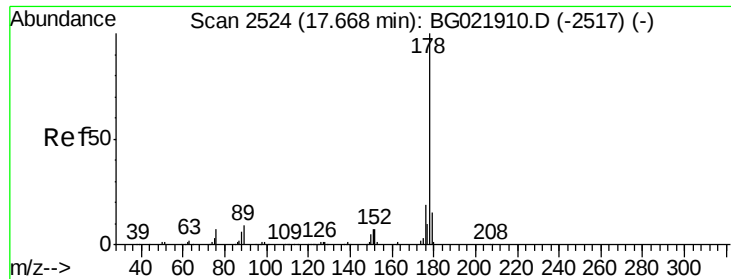

#72

Anthracene

Concen: 1.20 ng/ul

RT: 17.67 min Scan# 2524

Delta R.T. -0.00 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Instrument :

BNA_G

ClientSampleId :

D9XE2


Tot Ion:178 Resp: 26340

Ion Ratio Lower Upper

178 100

179 16.3 12.9 19.3




176 16.6 15.6 23.4

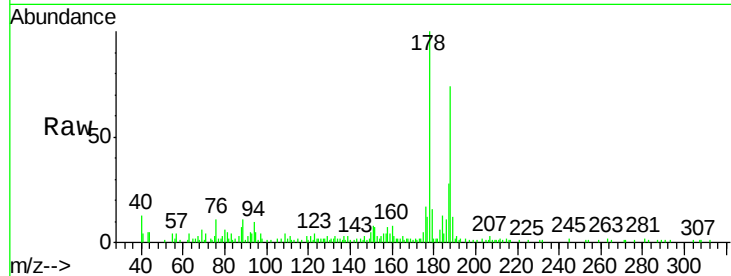

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

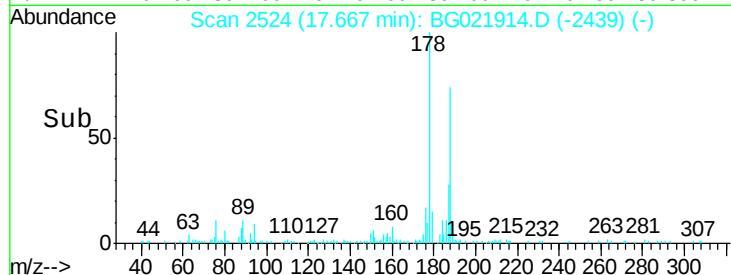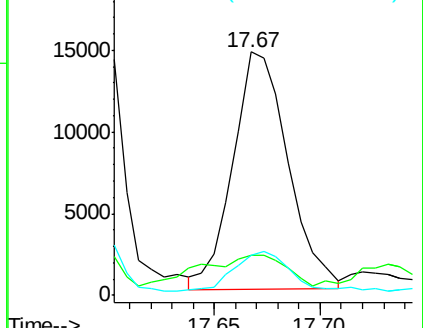

#74

Di-n-butylphthalate

Concen: 5.99 ng/ul

RT: 18.48 min Scan# 2662

Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05


Tgt Ion:149 Resp: 103256

Ion Ratio Lower Upper

149 100

150 8.8 7.5 11.3



104 3.7 5.4 8.2#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E



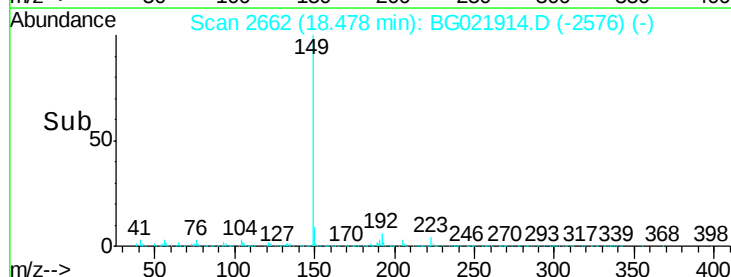
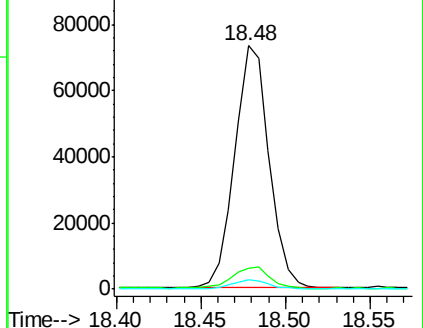


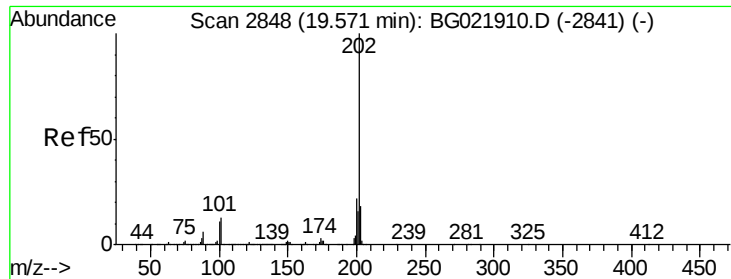

#75
Fluoranthene
Concen: 12.38 ng/ul
RT: 19.58 min Scan# 2850
Delta R.T. 0.01 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05




Instrument :
BNA_G
ClientSampleId :
D9XE2


Tot Ion	Ratio	Lower	Upper
202	100		
101	12.8	8.9	13.3
100	10.3	7.0	10.4

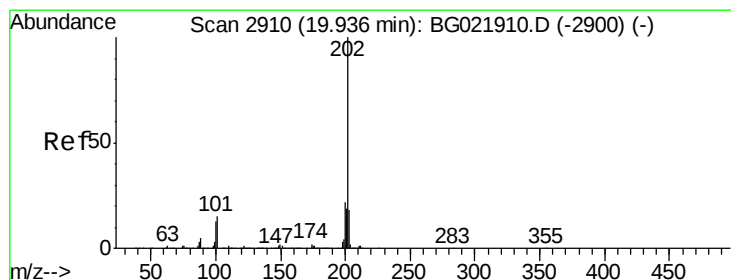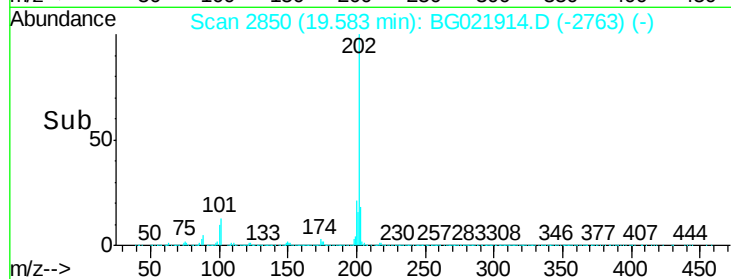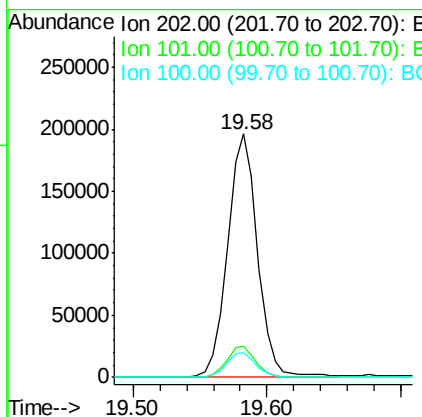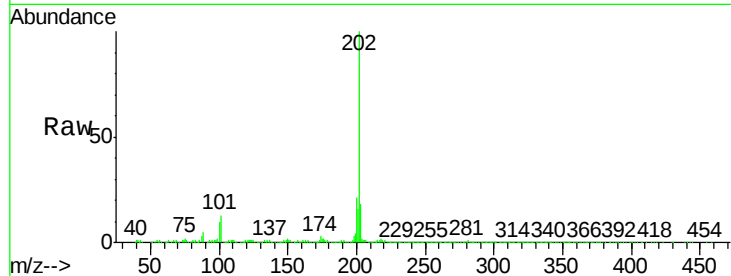

#78
Pyrene
Concen: 12.18 ng/ul
RT: 19.95 min Scan# 2912
Delta R.T. 0.01 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05

Tgt Ion	Ratio	Lower	Upper
202	100		
101	13.9	9.8	14.8
100	12.3	9.3	13.9

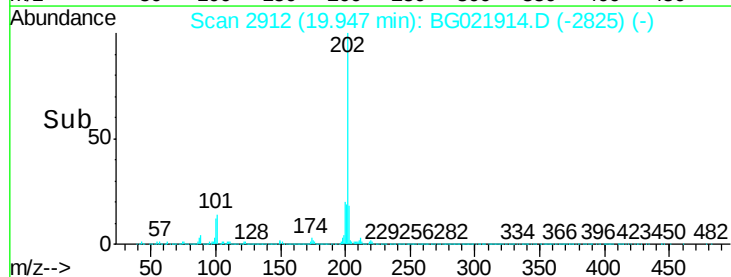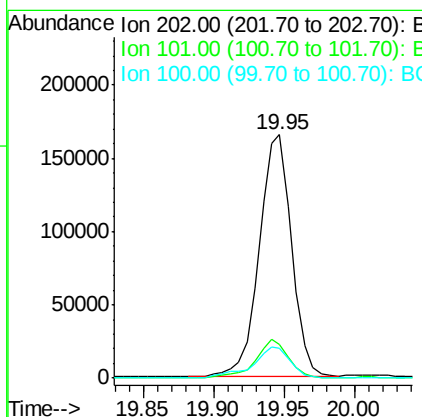

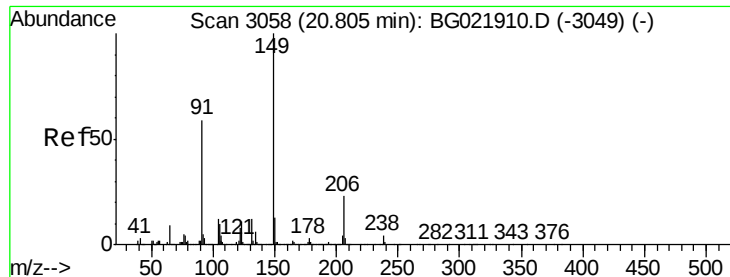

#79

Butylbenzylphthalate

Concen: 255.37 ng/ul

RT: 20.82 min Scan# 3060

Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Instrument :

BNA_G

ClientSampleId :

D9XE2


Tot Ion:149 Resp: 1236629

Ion Ratio Lower Upper

149 100

91 64.5 65.8 98.8#




206 27.2 15.5 23.3#

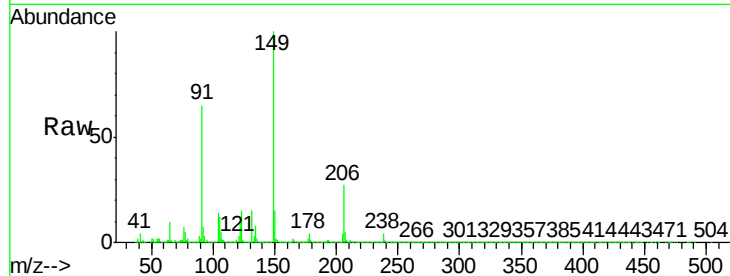

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BG021910.D (-3049) (-)

Ion 206.00 (205.70 to 206.70): E

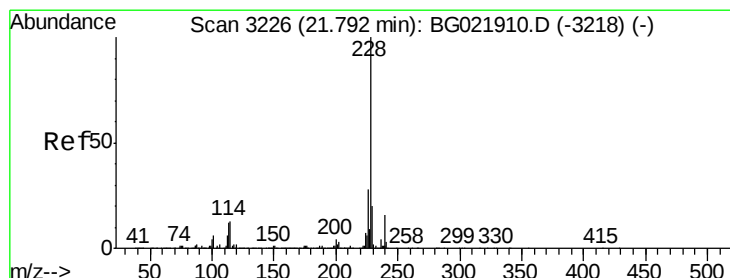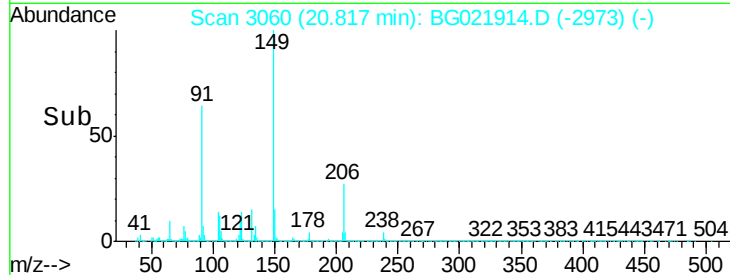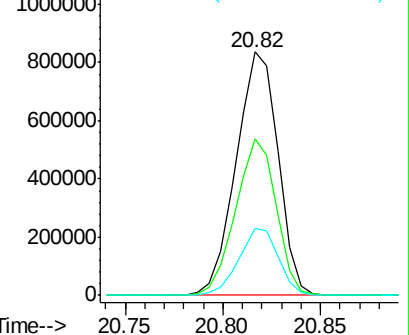

#81

Benzo(a)anthracene

Concen: 7.50 ng/ul

RT: 21.80 min Scan# 3228

Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05


Tgt Ion:228 Resp: 157963

Ion Ratio Lower Upper

228 100

229 22.5 16.6 25.0



226 27.9 21.0 31.4

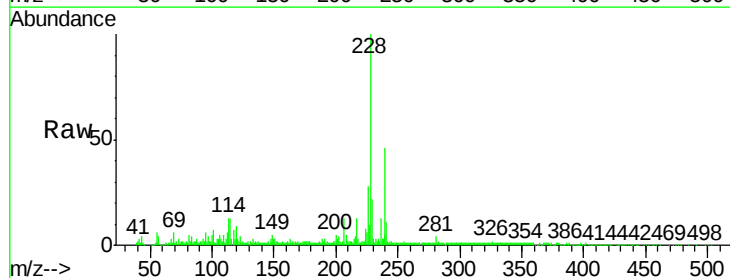


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

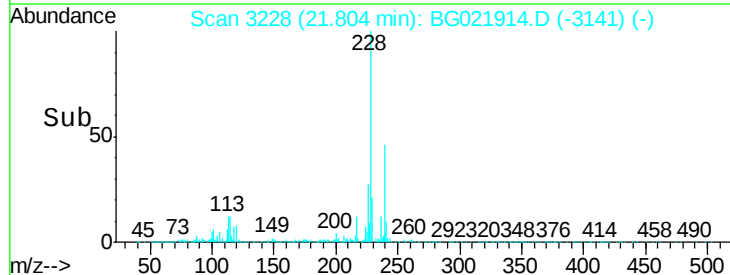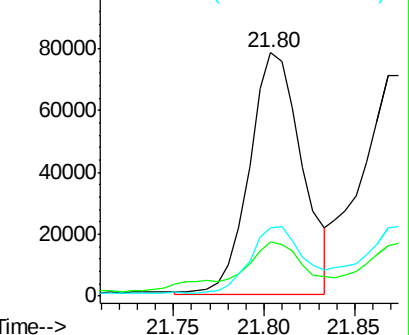

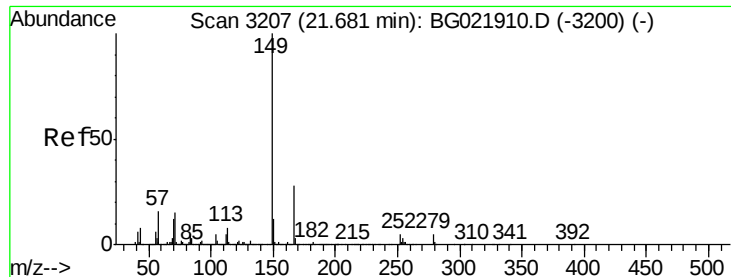

#82

Bis(2-ethylhexyl)phthalate

Concen: 25.99 ng/ul

RT: 21.69 min Scan# 3208

Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Instrument :


BNA_G

ClientSampleId :

D9XE2

Tot Ion:149 Resp: 205457


Ion	Ratio	Lower	Upper
149	100		
167	27.4	20.5	30.7
279	5.5	3.7	5.5





Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

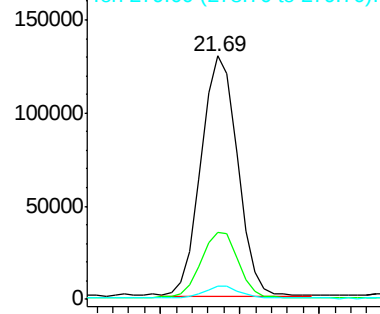

Time-->

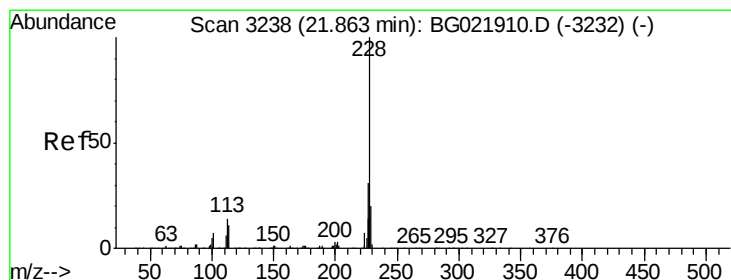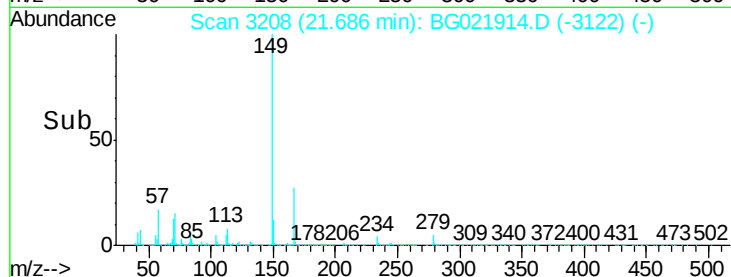

#83

Chrysene

Concen: 7.99 ng/ul

RT: 21.87 min Scan# 3240


Delta R.T. 0.01 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Tgt Ion:228 Resp: 166457


Ion	Ratio	Lower	Upper
228	100		
226	31.8	23.4	35.2
229	24.1	16.2	24.2




Abundance Ion 228.00 (227.70 to 228.70): E


Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

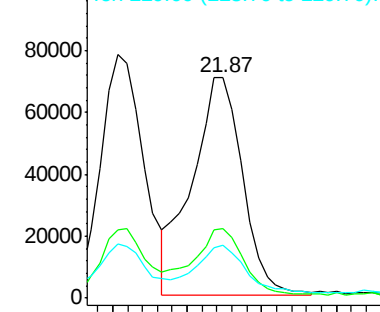

Time-->

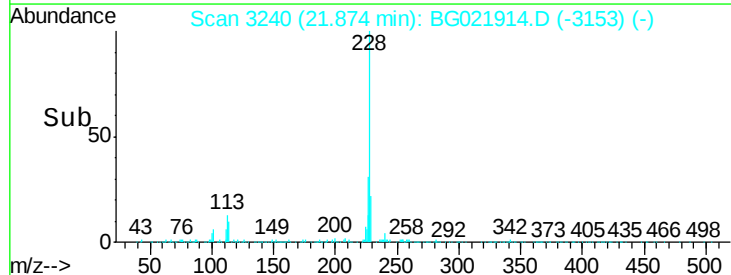


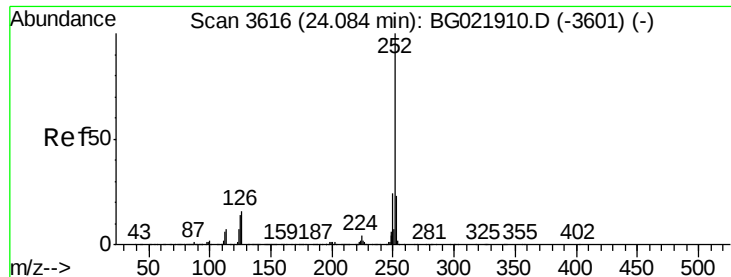




#86
Benzo(b)fluoranthene
Concen: 11.79 ng/ul
RT: 24.11 min Scan# 3620
Delta R.T. 0.02 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05

Instrument :
BNA_G
ClientSampleId :
D9XE2

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.6	18.1	27.1
125	14.9	7.6	11.4

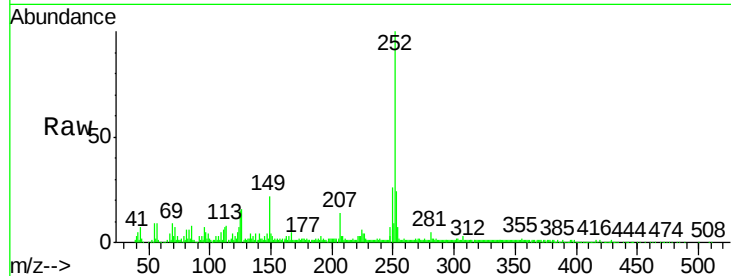


Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

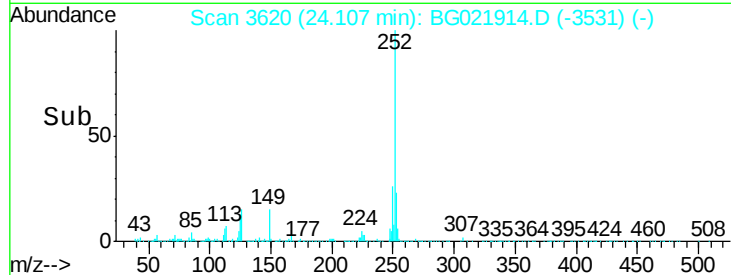
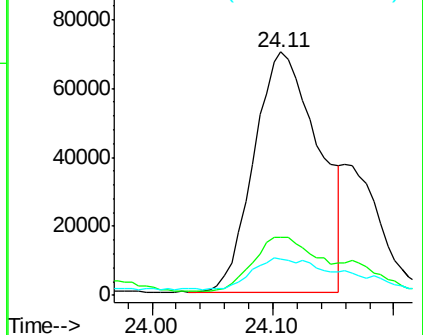



#87
Benzo(k)fluoranthene
Concen: 11.02 ng/ul
RT: 24.11 min Scan# 3620
Delta R.T. -0.05 min
Lab File: BG021914.D
Acq: 16 May 2016 20:05

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	17.8	26.8
125	14.9	7.7	11.5

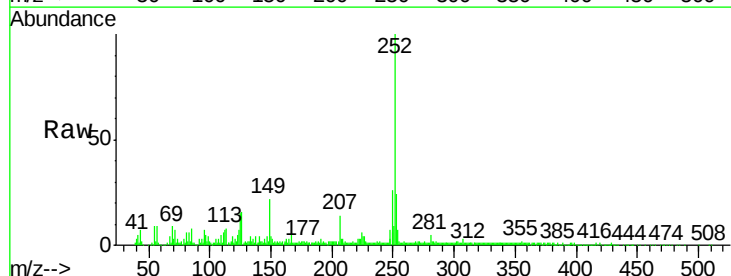

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

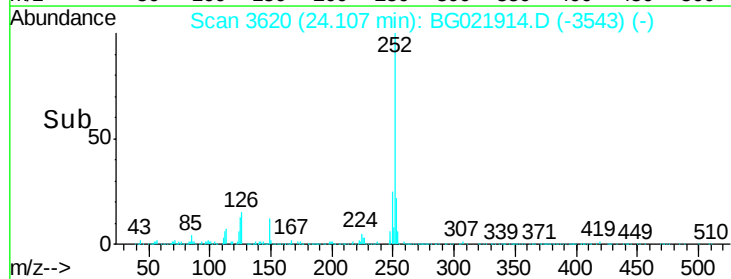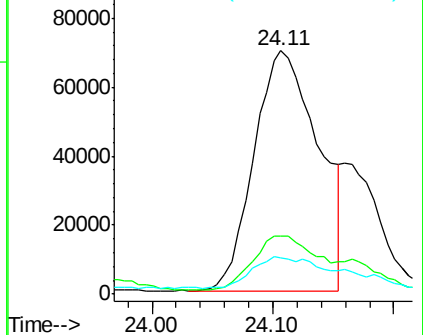

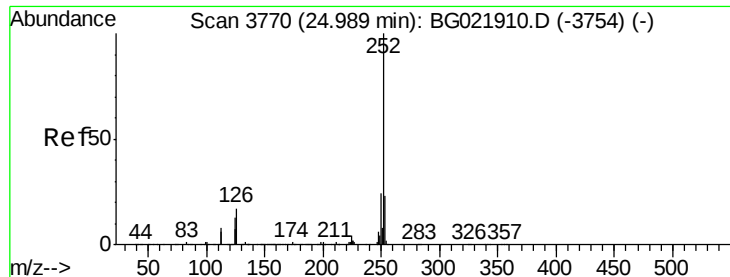

#89

Benzo(a)pyrene

Concen: 7.54 ng/ul

RT: 25.01 min Scan# 3774

Delta R.T. 0.02 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Instrument :

BNA_G

ClientSampleId :

D9XE2


Tot Ion:252 Resp: 164593

Ion Ratio Lower Upper

252 100

253 22.9 17.4 26.0




125 15.5 8.2 12.2#

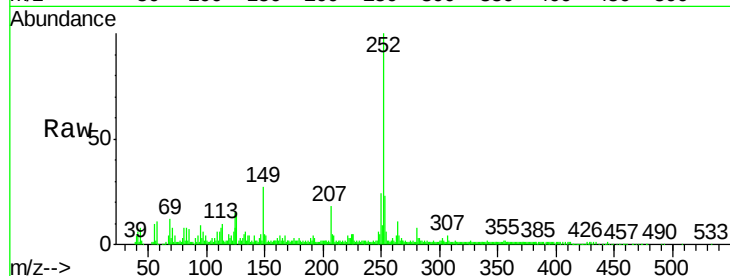

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

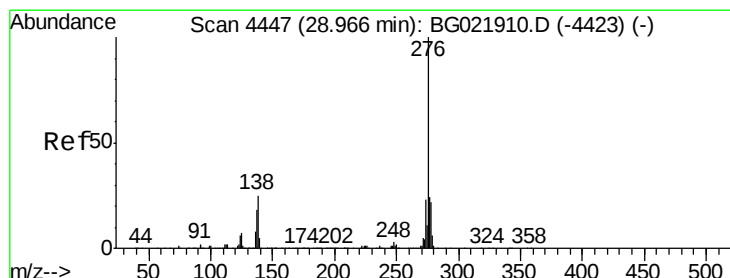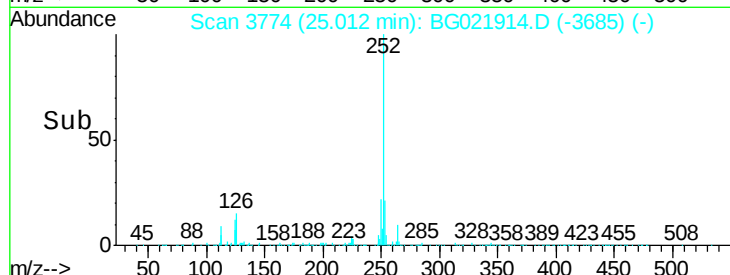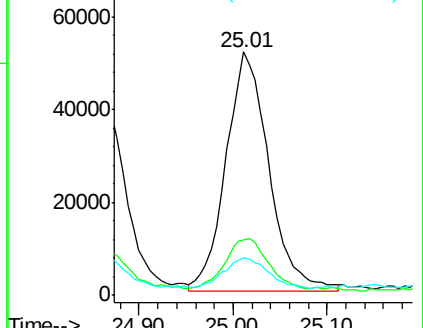

#90

Indeno(1,2,3-cd)pyrene

Concen: 3.71 ng/ul

RT: 29.01 min Scan# 4454

Delta R.T. 0.04 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05


Tgt Ion:276 Resp: 96130

Ion Ratio Lower Upper

276 100

138 26.3 15.8 23.6#



277 26.7 19.0 28.6

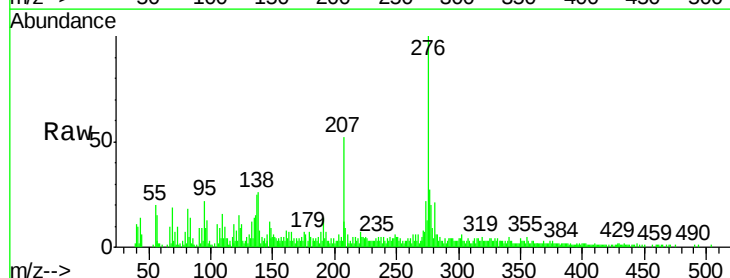


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

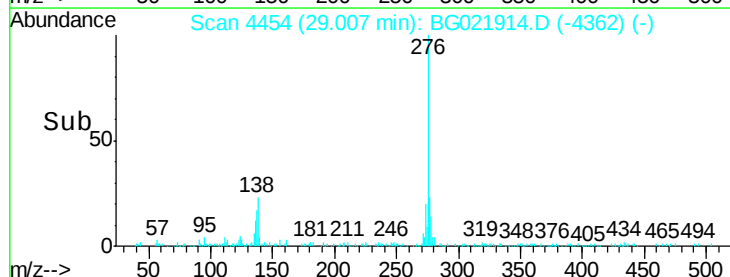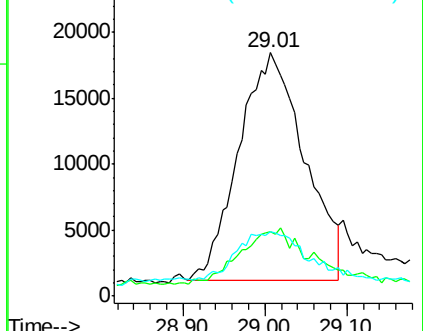

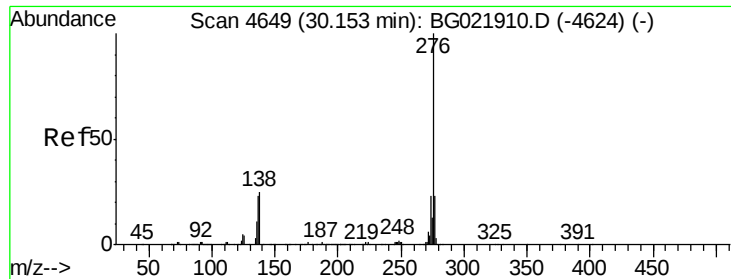

#92

Benzo(a,h,i)perylene

Concen: 1.95 ng/ul

RT: 30.19 min Scan# 4656

Delta R.T. 0.04 min

Lab File: BG021914.D

Acq: 16 May 2016 20:05

Instrument :

BNA_G

ClientSampleId :

D9XE2


Tot Ion: 276 Resp: 41661

Ion Ratio Lower Upper

276 100

138 27.2 13.9 20.9#

277 26.9 19.8 29.6



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

