

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051616\
 Data File : BG021915.D
 Acq On : 16 May 2016 20:45
 Operator : UM/SJ
 Sample : H3095-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9XE3

Quant Time: May 17 01:37:41 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 01:35:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	68038	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	325292	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	190330	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.54	188	380959	20.00	ng/ul	0.00
76) Chrysene-d12	21.82	240	366993	20.00	ng/ul	0.00
84) Perylene-d12	25.17	264	369865	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	5230	3.71	ng/uL	0.00
5) Phenol-d5	7.32	99	111331	22.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	53808	21.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	105976	27.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	77804	18.35	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	54196	25.34	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	59247	43.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	599	0.16	ng/ul	0.12
29) 4-Chloroaniline-d4	11.12	131	77823	18.91	ng/ul	0.00
44) Dimethylphthalate-d6	14.19	166	333417	24.94	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	463260	24.41	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	34634	15.11	ng/ul	0.02
58) Fluorene-d10	15.78	176	311037	22.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	31369	29.73	ng/ul	0.00
71) Anthracene-d10	17.63	188	432365	23.32	ng/ul	0.00
77) Pyrene-d10	19.91	212	446998	26.02	ng/ul	0.00
88) Benzo(a)pyrene-d12	24.94	264	422174	24.02	ng/ul	0.03

Target Compounds


						Ovalue
4) Benzaldehyde	7.70	77	1594	2.90	ng/ul	88
45) Dimethylphthalate	14.24	163	123013	9.03	ng/ul#	98
64) 4,6-Dinitro-2-methylphenol	15.83	198	1555	1.35	ng/ul#	75
70) Phenanthrene	17.58	178	85845	4.12	ng/ul	96
72) Anthracene	17.58	178	85845	4.06	ng/ul	99
75) Fluoranthene	19.58	202	175399	7.41	ng/ul#	94
78) Pyrene	19.58	202	175399	8.26	ng/ul	96
81) Benzo(a)anthracene	21.81	228	95014	4.65	ng/ul	94
82) Bis(2-ethylhexyl)phthalate	21.69	149	74354	9.70	ng/ul	97
83) Chrysene	21.87	228	112344	5.56	ng/ul	96
86) Benzo(b)fluoranthene	24.10	252	185500	8.76	ng/ul#	92
87) Benzo(k)fluoranthene	24.10	252	185500	8.18	ng/ul#	92
89) Benzo(a)pyrene	25.01	252	107663	5.11	ng/ul#	95
90) Indeno(1,2,3-cd)pyrene	29.00	276	63070	2.53	ng/ul#	89
92) Benzo(g,h,i)perylene	30.19	276	41977	2.04	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051616\
Data File : BG021915.D
Acq On : 16 May 2016 20:45
Operator : UM/SJ
Sample : H3095-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9XE3

Quant Time: May 17 01:37:41 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 01:35:08 2016
Response via : Initial Calibration

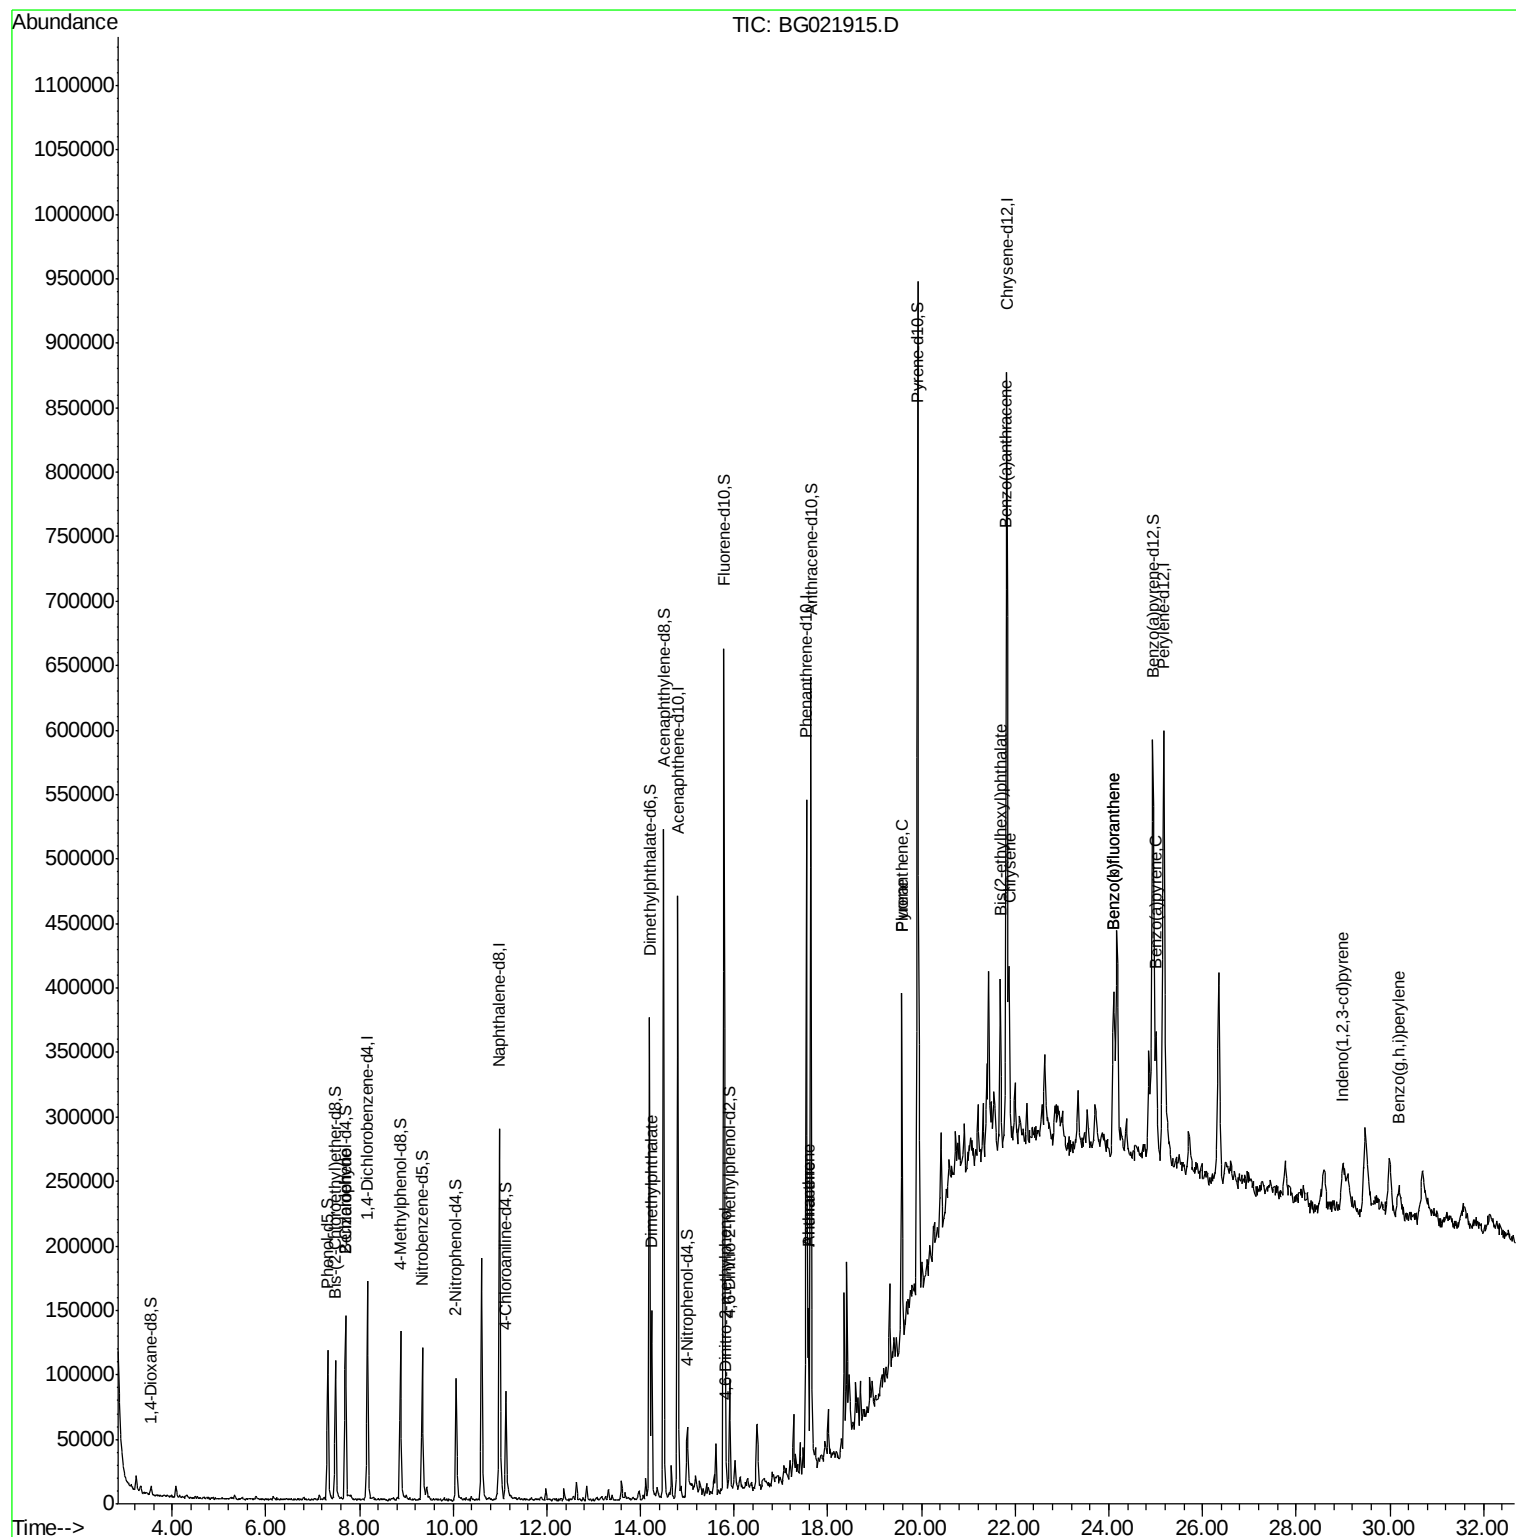

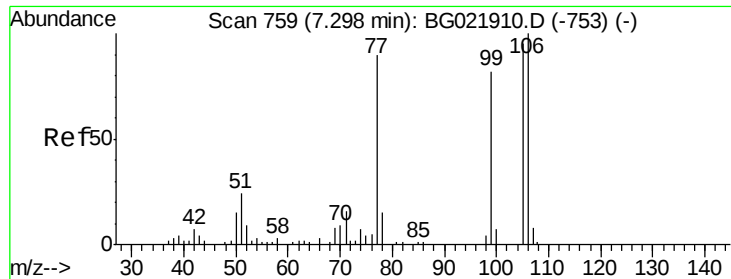

#4

Benzaldehyde

Concen: 2.90 ng/ul

RT: 7.70 min Scan# 827

Delta R.T. 0.40 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampled :

D9XE3


Tot Ion: 77 Resp: 1594

Ion Ratio Lower Upper

77 100

105 75.5 68.5 102.7




106 69.5 65.0 97.4

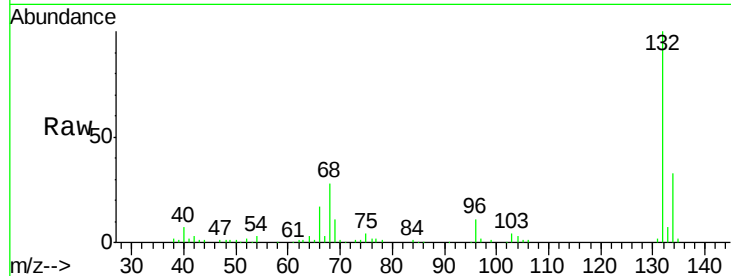

Abundance Ion 77.00 (76.70 to 77.70): B

Ion 105.00 (104.70 to 105.70): B

Ion 106.00 (105.70 to 106.70): B

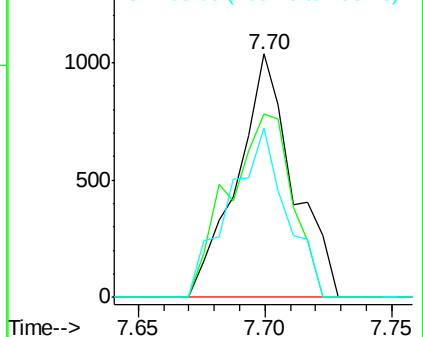

#45

Dimethylphthalate

Concen: 9.03 ng/ul

RT: 14.24 min Scan# 1940

Delta R.T. 0.01 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45


Tgt Ion: 163 Resp: 123013

Ion Ratio Lower Upper

163 100

194 3.8 3.9 5.9#



164 10.4 8.7 13.1




Abundance Ion 163.00 (162.70 to 163.70): B

Ion 194.00 (193.70 to 194.70): B

Ion 164.00 (163.70 to 164.70): B

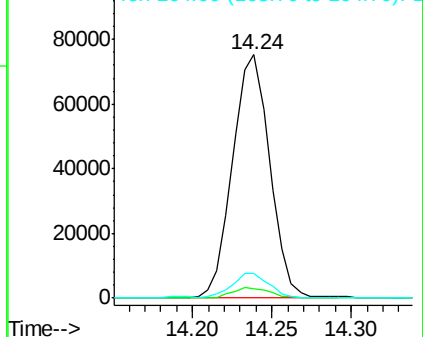

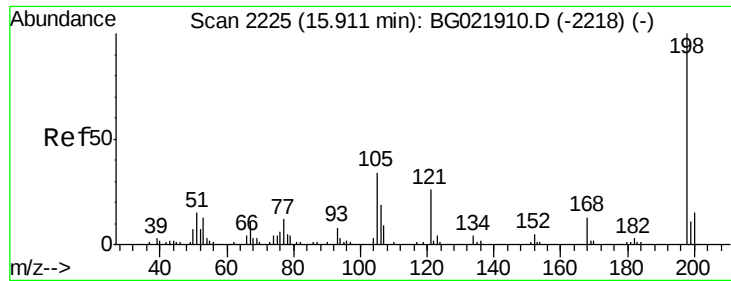

#64

4,6-Dinitro-2-methylphenol

Concen: 1.35 ng/ul

RT: 15.83 min Scan# 2210

Delta R.T. -0.09 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampled :

D9XE3


Tot Ion:198 Resp: 1555

Ion Ratio Lower Upper

198 100

182 17.7 3.8 5.8#

77 17.7 24.2 36.4#



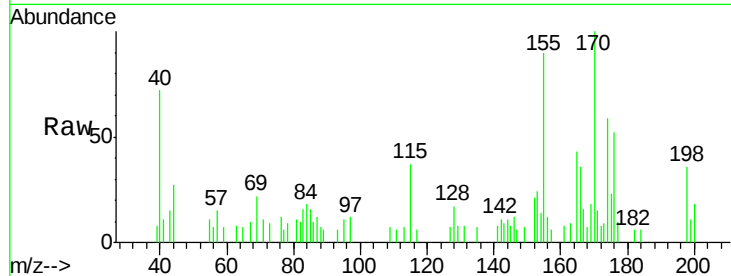


Abundance Ion 198.00 (197.70 to 198.70): E

Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): B

Time-->

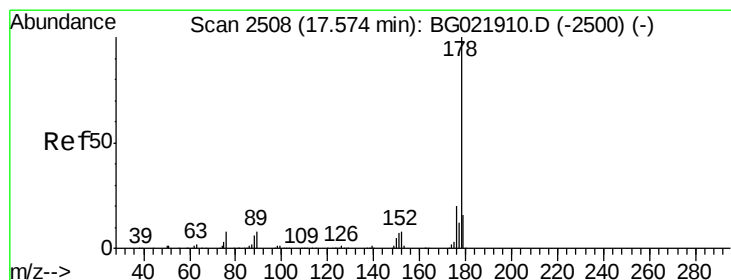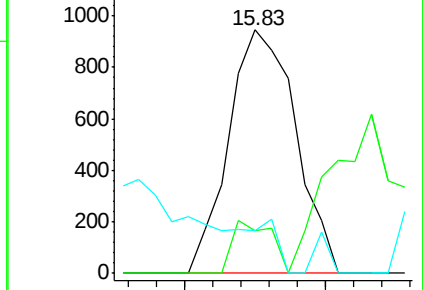

#70

Phenanthrene

Concen: 4.12 ng/ul

RT: 17.58 min Scan# 2509

Delta R.T. 0.01 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45


Tgt Ion:178 Resp: 85845

Ion Ratio Lower Upper

178 100

179 16.2 11.8 17.8

176 20.5 14.8 22.2






Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

Time-->

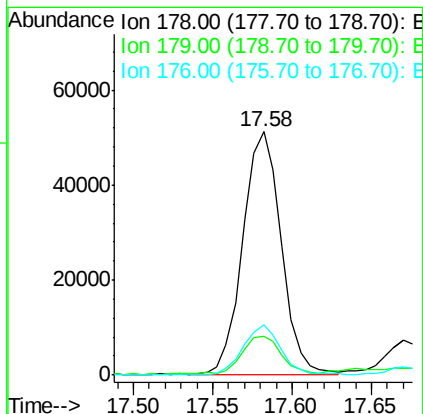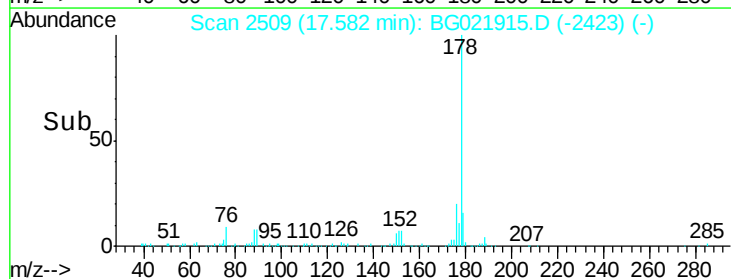



#72

Anthracene

Concen: 4.06 ng/ul

RT: 17.58 min Scan# 2509

Delta R.T. -0.09 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampleId :

D9XE3


Tot Ion:178 Resp: 85845

Ion Ratio Lower Upper




178 100

179 16.2 12.9 19.3

176 20.5 15.6 23.4



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

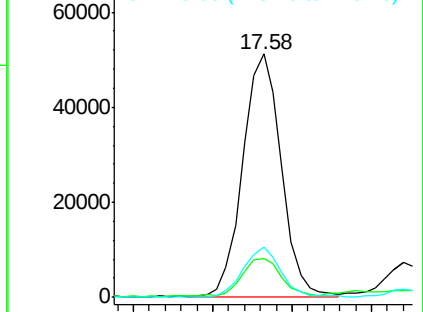

#75

Fluoranthene

Concen: 7.41 ng/ul

RT: 19.58 min Scan# 2849

Delta R.T. 0.01 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45


Tgt Ion:202 Resp: 175399

Ion Ratio Lower Upper



202 100


101 13.9 8.9 13.3#

100 10.2 7.0 10.4



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

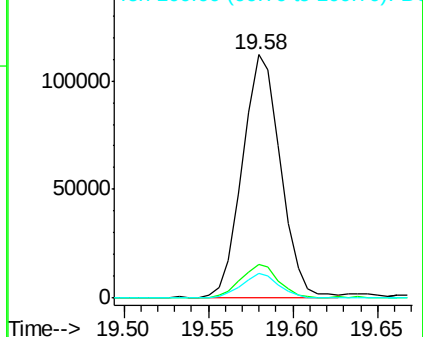

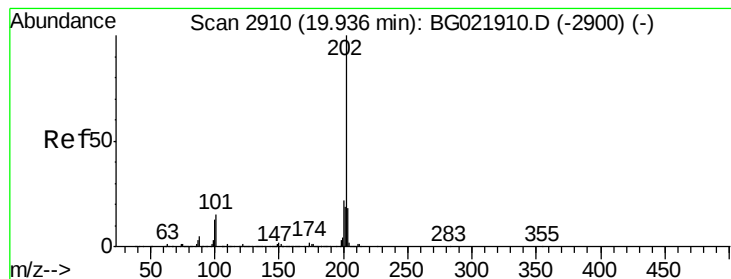

#78

Pvrene

Concen: 8.26 ng/ul

RT: 19.58 min Scan# 2849

Delta R.T. -0.36 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampleId :

D9XE3


Tot Ion:202 Resp: 175399

Ion Ratio Lower Upper

202 100

101 13.9 9.8 14.8




100 10.2 9.3 13.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

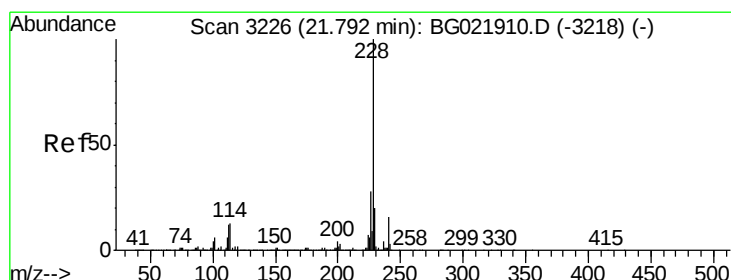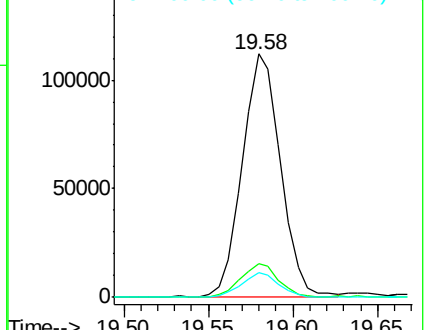

#81

Benzo(a)anthracene

Concen: 4.65 ng/ul

RT: 21.81 min Scan# 3228

Delta R.T. 0.01 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45


Tgt Ion:228 Resp: 95014

Ion Ratio Lower Upper

228 100

229 22.8 16.6 25.0



226 29.8 21.0 31.4

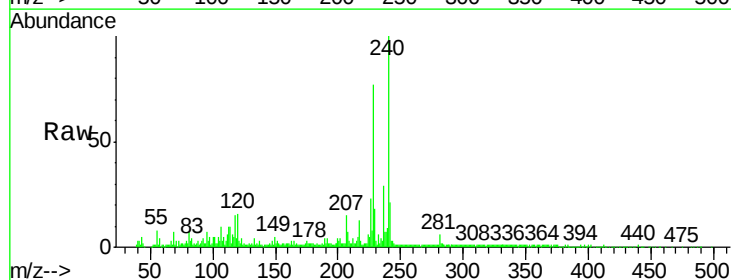


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

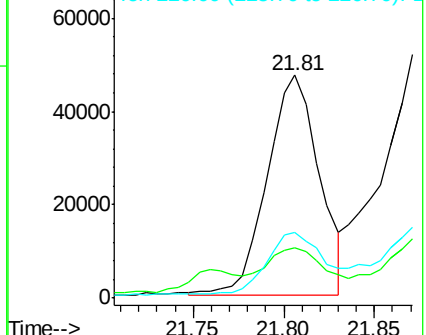

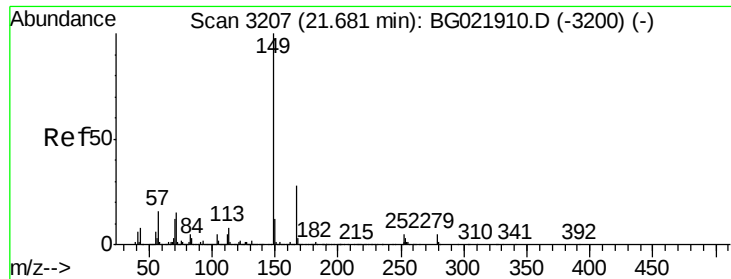

#82

Bis(2-ethylhexyl)phthalate

Concen: 9.70 ng/ul

RT: 21.69 min Scan# 3208

Delta R.T. 0.01 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampleId :

D9XE3


Tot Ion:149 Resp: 74354

Ion Ratio Lower Upper

149 100

167 27.2 20.5 30.7




279 5.4 3.7 5.5

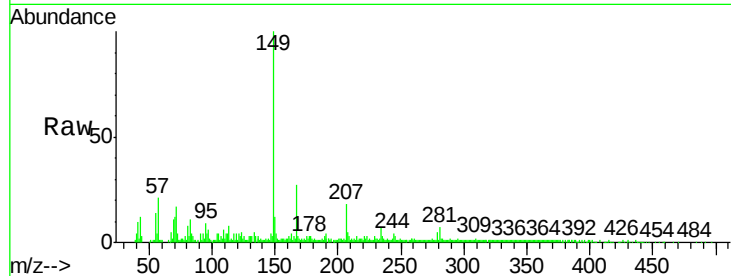

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

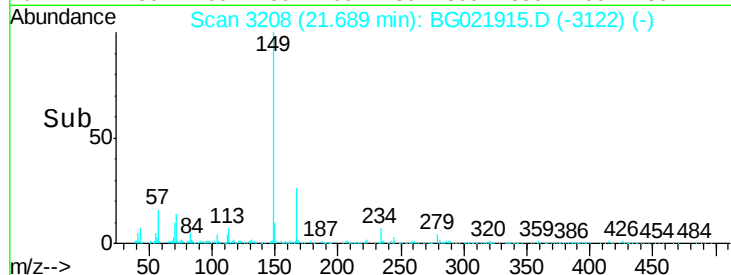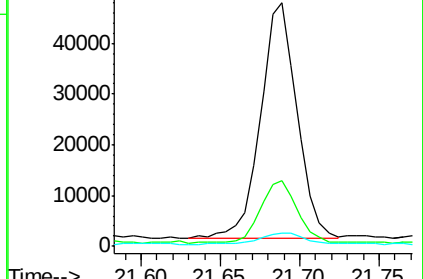

#83

Chrysene

Concen: 5.56 ng/ul

RT: 21.87 min Scan# 3239

Delta R.T. 0.01 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45


Tgt Ion:228 Resp: 112344

Ion Ratio Lower Upper

228 100

226 29.0 23.4 35.2



229 24.2 16.2 24.2




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




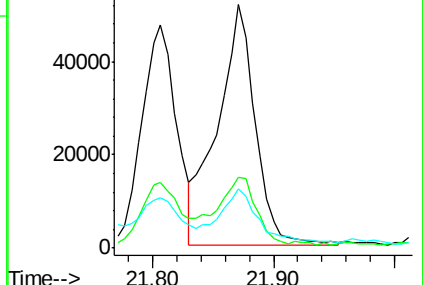


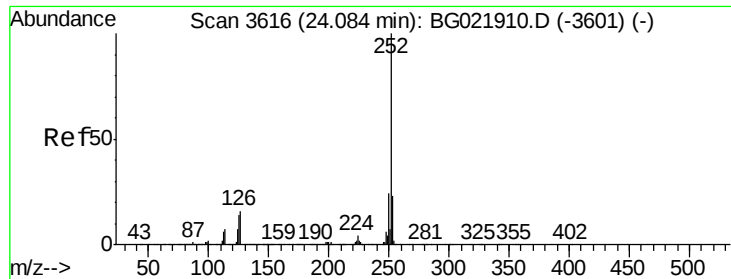

#86
Benzo(b)fluoranthene
Concen: 8.76 ng/ul
RT: 24.10 min Scan# 3619
Delta R.T. 0.02 min
Lab File: BG021915.D
Acq: 16 May 2016 20:45




Instrument :
BNA_G
ClientSampleId :
D9XE3


Tot Ion	Ratio	Lower	Upper
252	100		
253	24.4	18.1	27.1
125	16.0	7.6	11.4

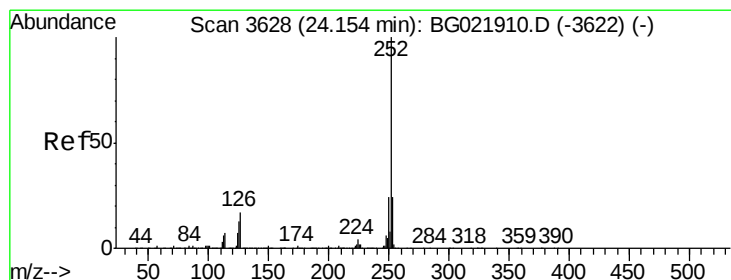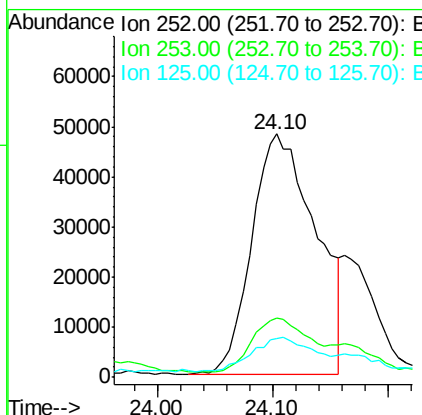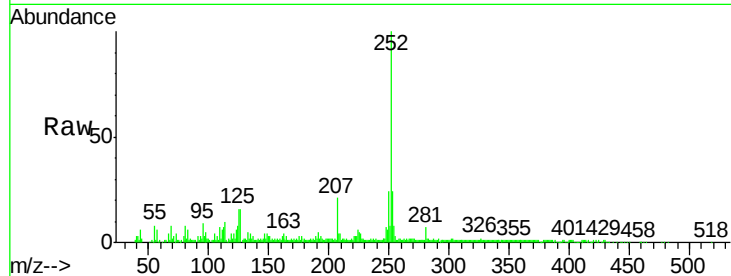

#87
Benzo(k)fluoranthene
Concen: 8.18 ng/ul
RT: 24.10 min Scan# 3619
Delta R.T. -0.05 min
Lab File: BG021915.D
Acq: 16 May 2016 20:45

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.4	17.8	26.8
125	16.0	7.7	11.5

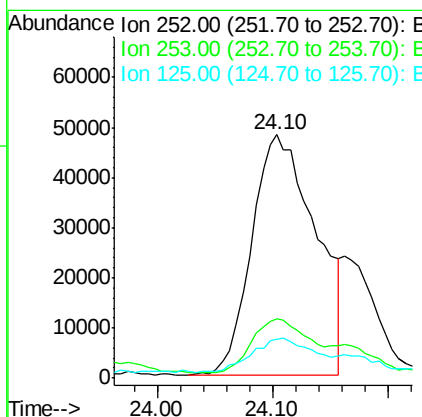

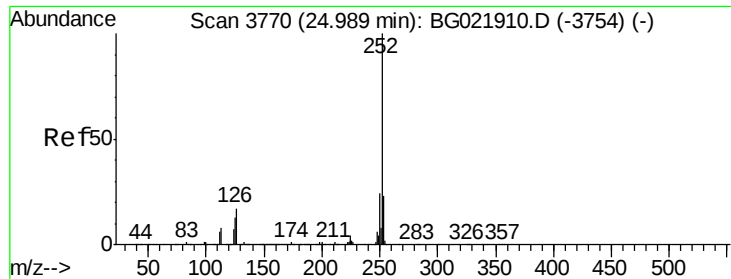

#89

Benzo(a)pyrene

Concen: 5.11 ng/ul

RT: 25.01 min Scan# 3774

Delta R.T. 0.03 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampleId :

D9XE3


Tot Ion:252 Resp: 107663

Ion Ratio Lower Upper

252 100

253 22.4 17.4 26.0




125 14.5 8.2 12.2#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

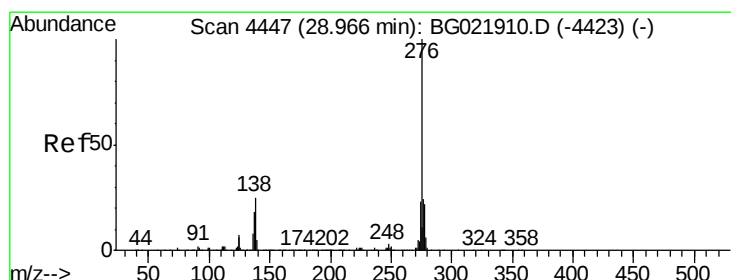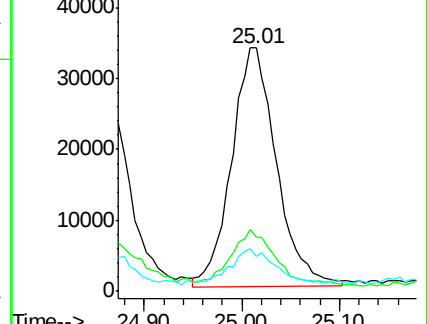

#90

Indeno(1,2,3-cd)pyrene

Concen: 2.53 ng/ul

RT: 29.00 min Scan# 4452

Delta R.T. 0.03 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45


Tgt Ion:276 Resp: 63070

Ion Ratio Lower Upper

276 100

138 27.7 15.8 23.6#



277 26.8 19.0 28.6




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

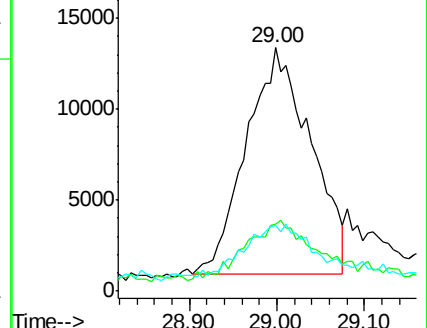

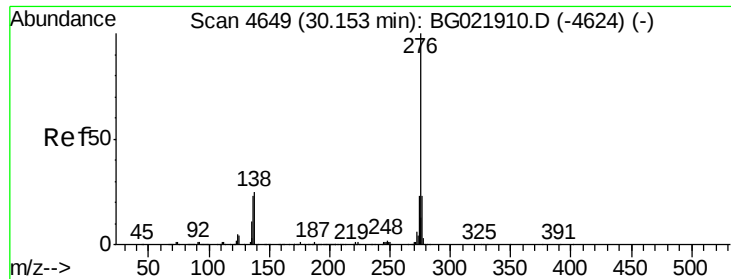

#92

Benzo(a,h,i)perylene

Concen: 2.04 ng/ul

RT: 30.19 min Scan# 4655

Delta R.T. 0.04 min

Lab File: BG021915.D

Acq: 16 May 2016 20:45

Instrument :

BNA_G

ClientSampleId :

D9XE3


Tot Ion:276 Resp: 41977

Ion Ratio Lower Upper

276 100

138 25.2 13.9 20.9#

277 25.0 19.8 29.6



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

