

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051616\
 Data File : BG021918.D
 Acq On : 16 May 2016 22:45
 Operator : UM/SJ
 Sample : H3095-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9XE6

Manual Integrations
 APPROVED

umangi
 5/17/2016 7:20:40 PM

Quant Time: May 17 03:56:10 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 01:35:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	74874	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	346455	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.80	164	198468	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.54	188	404682	20.00	ng/ul	0.00
76) Chrysene-d12	21.82	240	388644	20.00	ng/ul	0.00
84) Perylene-d12	25.18	264	398734	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	5383	3.47	ng/uL	0.00
5) Phenol-d5	7.32	99	120986	21.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	55044	19.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	109045	25.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	103082	22.09	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	54513	23.93	ng/ul	0.01
22) 2-Nitrophenol-d4	10.07	143	60467	42.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.61	165	108586m	26.69	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	82989	18.94	ng/ul	0.00
44) Dimethylphthalate-d6	14.19	166	332271	23.84	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	458863	23.18	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	39677	16.60	ng/ul	0.02
58) Fluorene-d10	15.78	176	316725	21.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	32638	29.12	ng/ul	0.00
71) Anthracene-d10	17.64	188	432427	21.95	ng/ul	0.00
77) Pyrene-d10	19.91	212	442207	24.31	ng/ul	0.00
88) Benzo(a)pyrene-d12	24.94	264	417426	22.03	ng/ul	0.02

Target Compounds

						Ovalue
45) Dimethylphthalate	14.24	163	57429	4.04	ng/ul	99
70) Phenanthrene	17.58	178	29176	1.32	ng/ul	98
75) Fluoranthene	19.58	202	48904	1.95	ng/ul	96
78) Pyrene	19.94	202	43733	1.94	ng/ul	95
79) Butylbenzylphthalate	20.81	149	6803	1.37	ng/ul	92
81) Benzo(a)anthracene	21.81	228	26331	1.22	ng/ul#	86
82) Bis(2-ethylhexyl)phthalate	21.69	149	102135	12.59	ng/ul	95
83) Chrysene	21.87	228	28666	1.34	ng/ul#	88
86) Benzo(b)fluoranthene	24.11	252	50486	2.21	ng/ul#	75
89) Benzo(a)pyrene	25.02	252	28815	1.27	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG051616\
Data File : BG021918.D
Acq On : 16 May 2016 22:45
Operator : UM/SJ
Sample : H3095-09
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
D9XE6

Manual Integrations
APPROVED

umangi
5/17/2016 7:20:40 PM

Quant Time: May 17 03:56:10 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG050916.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 01:35:08 2016
Response via : Initial Calibration

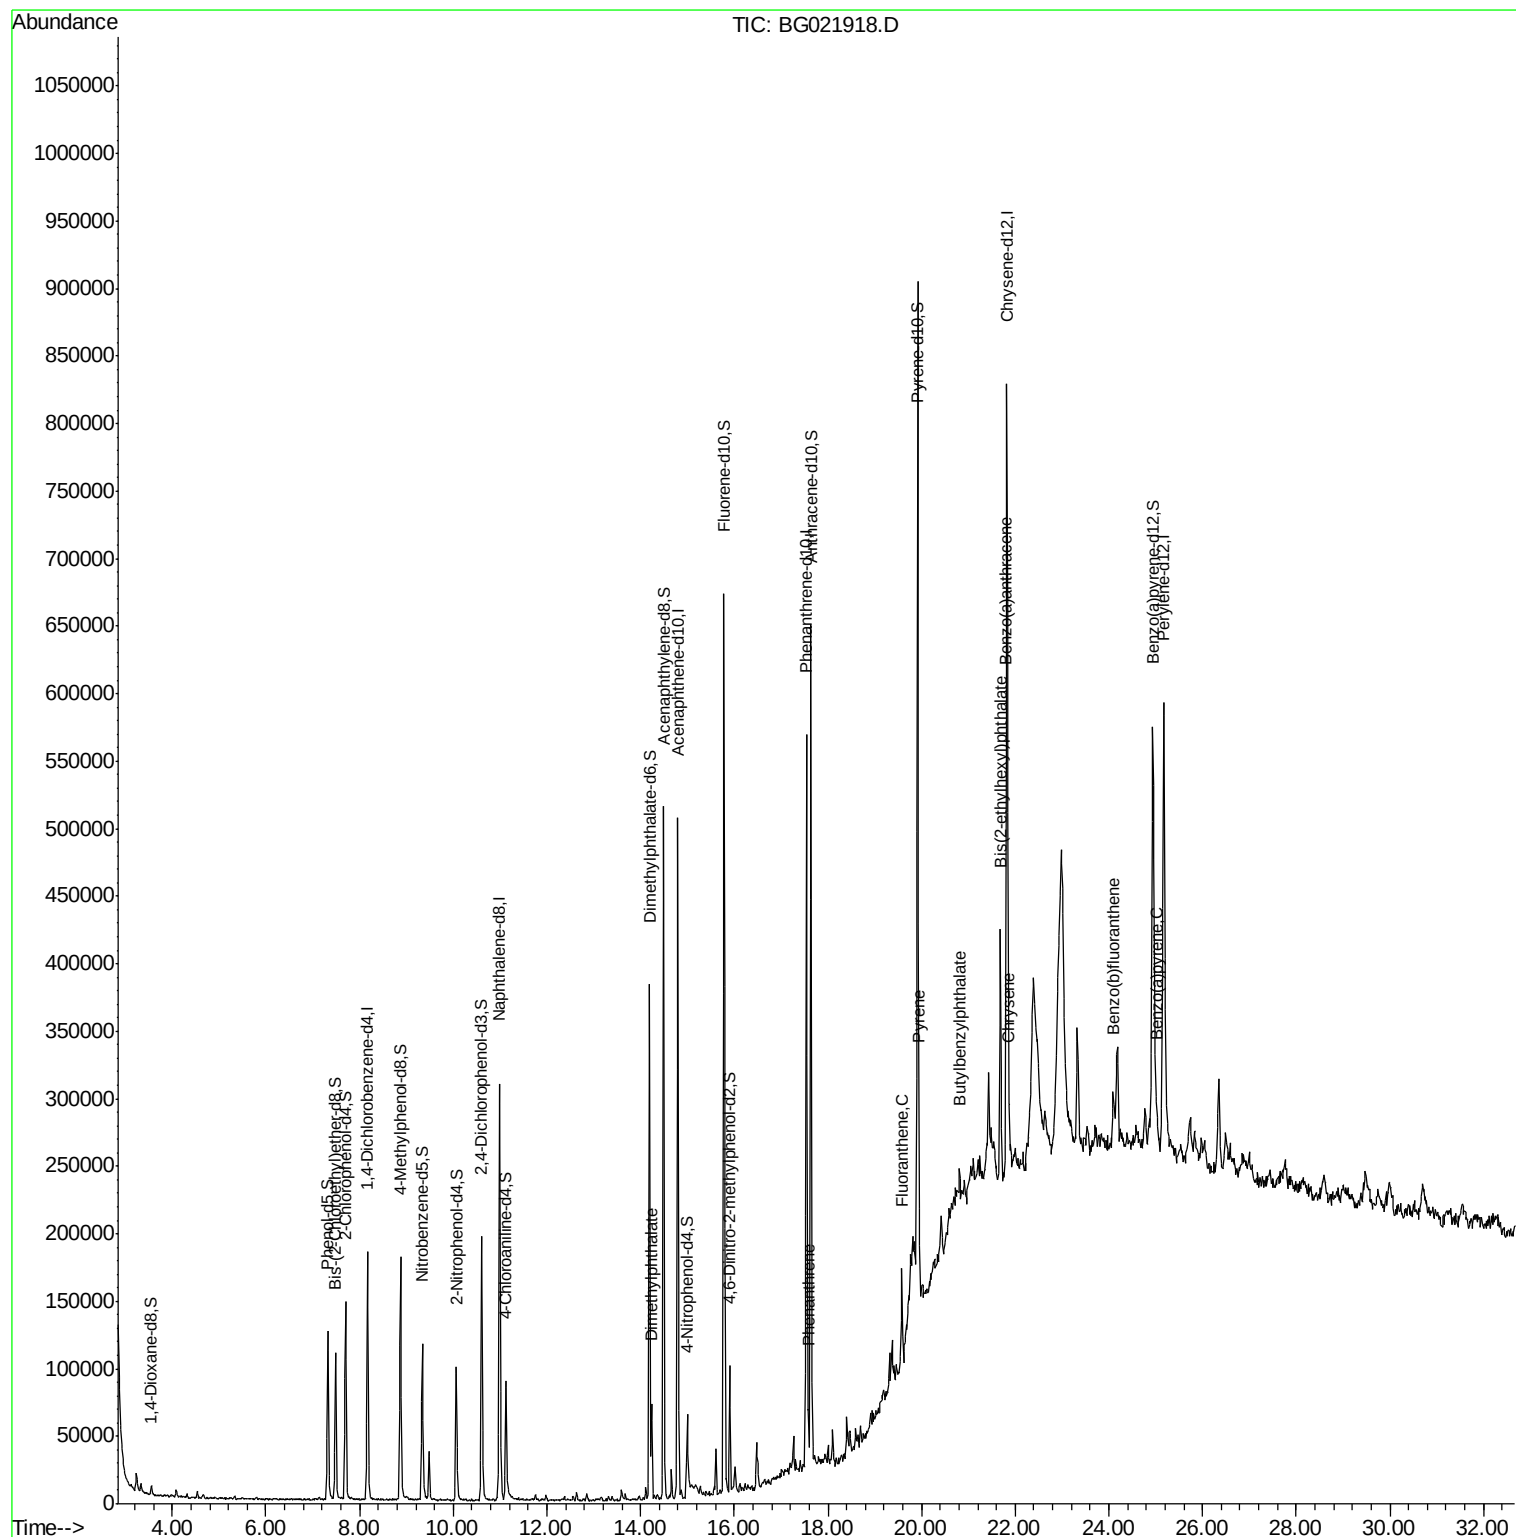

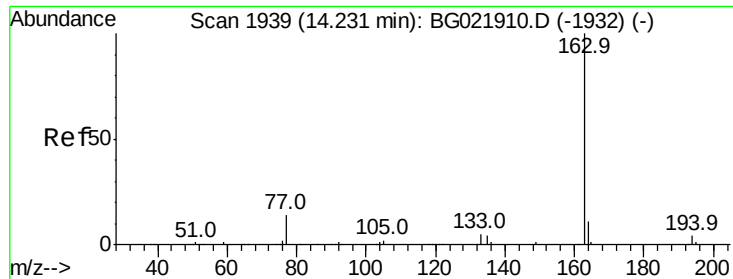

#45

Dimethylphthalate

Concen: 4.04 ng/ul

RT: 14.24 min Scan# 1940

Delta R.T. 0.01 min

Lab File: BG021918.D

Acq: 16 May 2016 22:45

Instrument :

BNA_G





ClientSampleId :

D9XE6

Tot Ion:	163	Resp:	57429
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.9	5.9
164	10.7	8.7	13.1

Manual Integrations
APPROVED

umangi
5/17/2016 7:20:40 PM

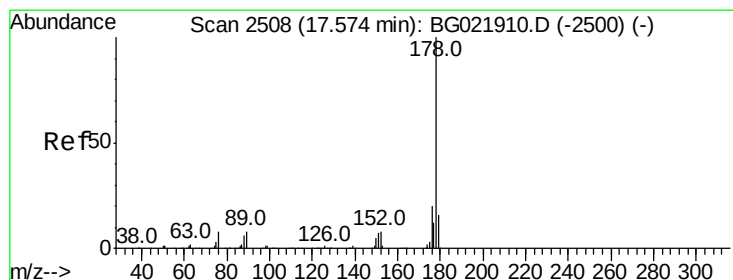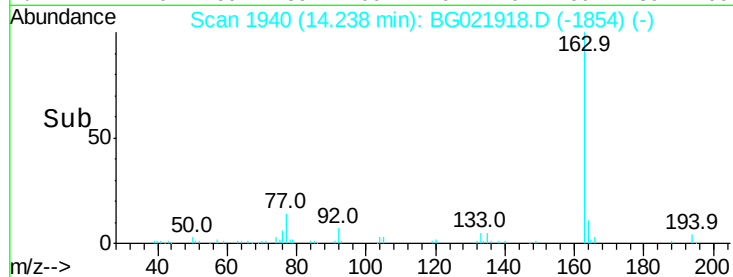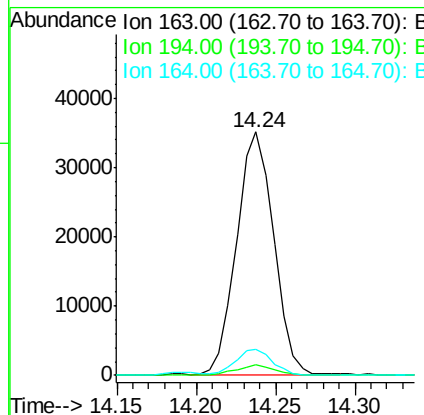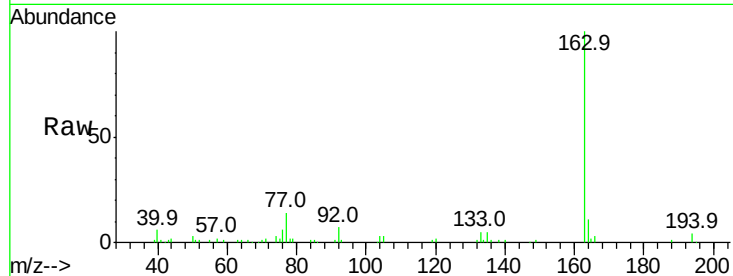

#70

Phenanthrene

Concen: 1.32 ng/ul




RT: 17.58 min Scan# 2509


Delta R.T. 0.01 min

Lab File: BG021918.D

Acq: 16 May 2016 22:45

Tgt Ion:	178	Resp:	29176
Ion Ratio	Lower	Upper	
178	100		
179	16.0	11.8	17.8
176	19.3	14.8	22.2

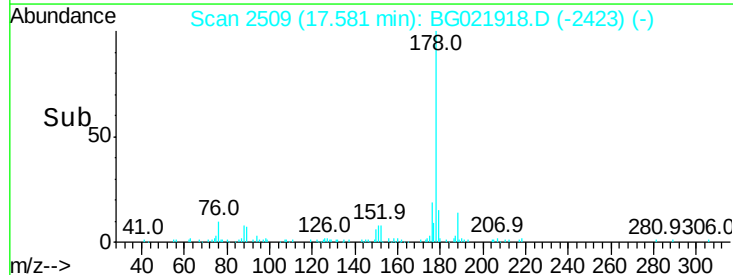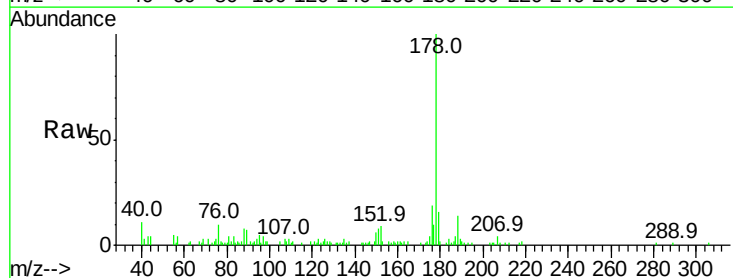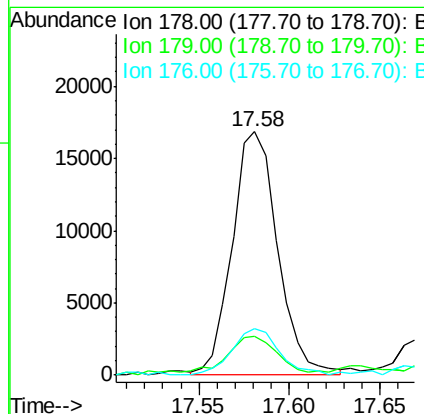

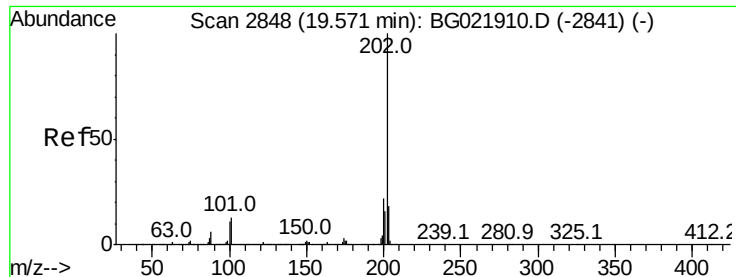

#75

Fluoranthene

Concen: 1.95 ng/ul

RT: 19.58 min Scan# 2849

Delta R.T. 0.01 min

Lab File: BG021918.D

Acq: 16 May 2016 22:45

Instrument :

BNA_G





ClientSampleId :

D9XE6

Tot Ion:	202	Resp:	48904
Ion Ratio	Lower	Upper	
202	100		
101	12.8	8.9	13.3
100	9.8	7.0	10.4

Manual Integrations
APPROVED

umangi
5/17/2016 7:20:40 PM

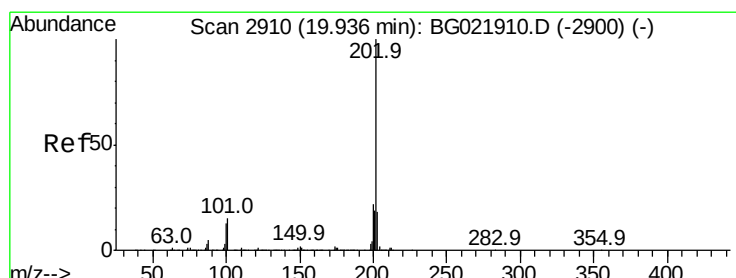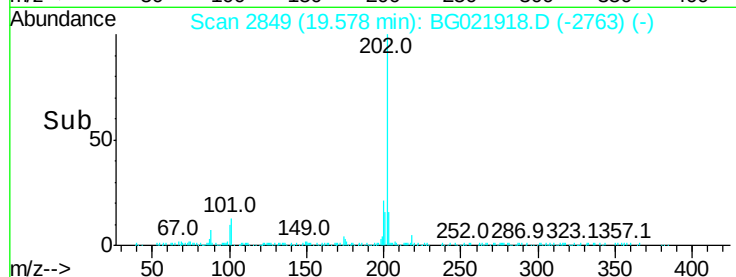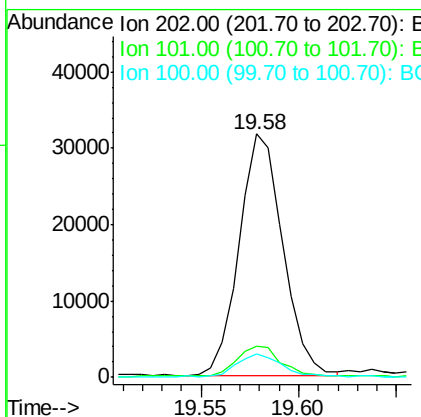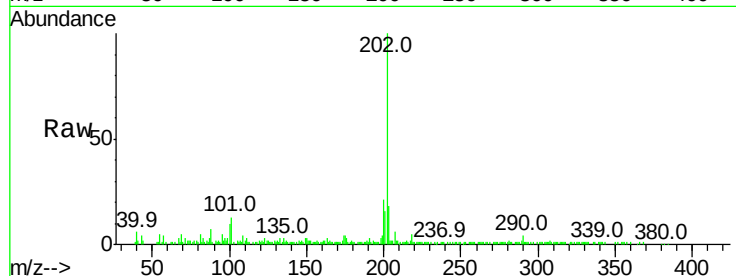

#78

Pyrene

Concen: 1.94 ng/ul




RT: 19.94 min Scan# 2911


Delta R.T. 0.01 min

Lab File: BG021918.D

Acq: 16 May 2016 22:45

Tgt Ion:	202	Resp:	43733
Ion Ratio	Lower	Upper	
202	100		
101	14.5	9.8	14.8
100	12.9	9.3	13.9

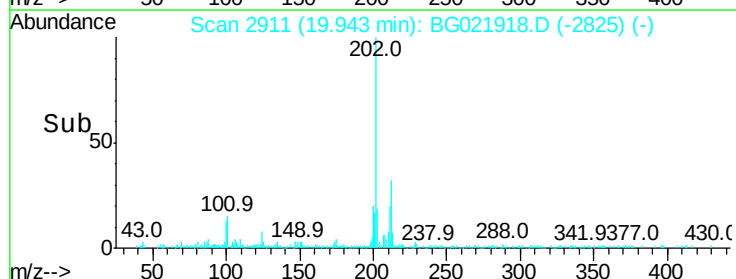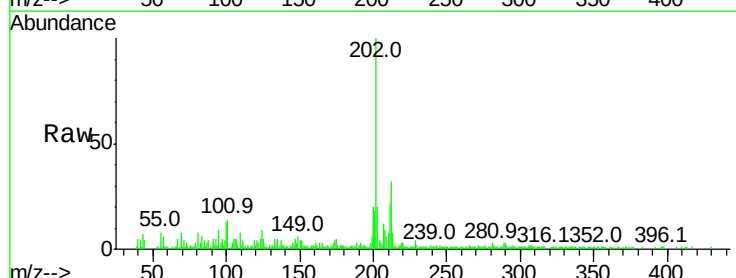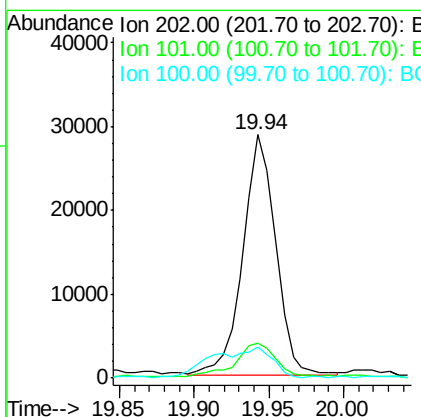

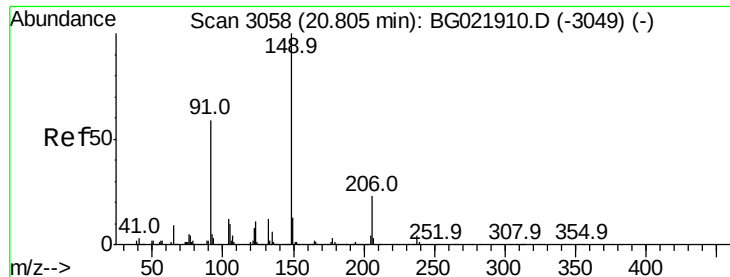





#79
Butylbenzylphthalate
Concen: 1.37 ng/ul
RT: 20.81 min Scan# 3059
Delta R.T. 0.01 min
Lab File: BG021918.D
Acq: 16 May 2016 22:45

Instrument :
BNA_G
ClientSampleId :
D9XE6

Tot Ion	Ratio	Resp	Lower	Upper
149	100	6803		
91	74.0		65.8	98.8
206	20.1		15.5	23.3




Manual Integrations
APPROVED


umangi
5/17/2016 7:20:40 PM

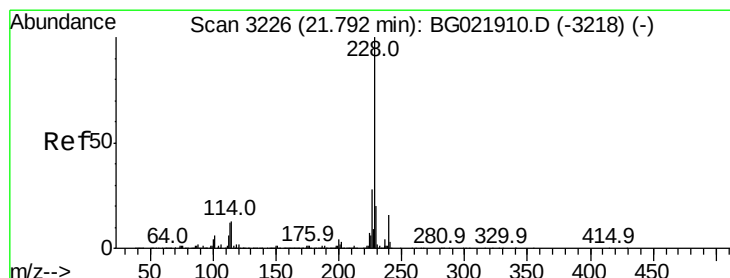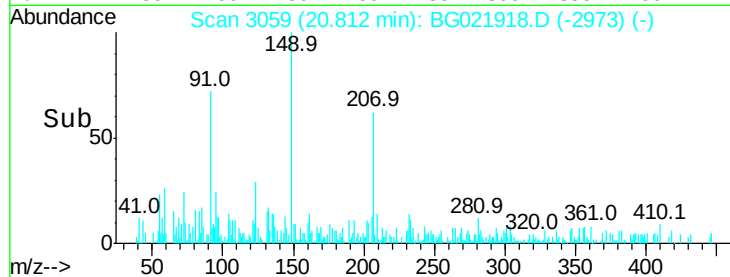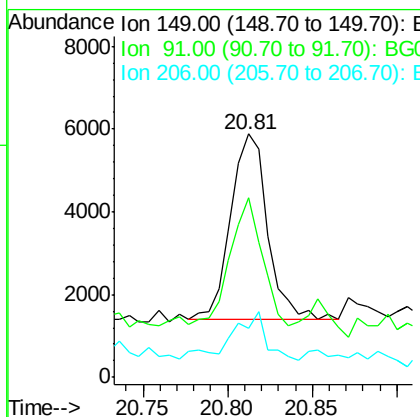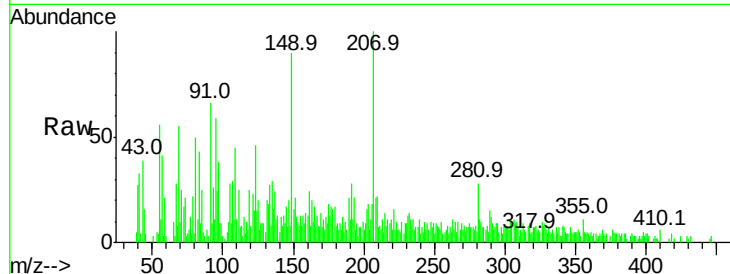

#81
Benzo(a)anthracene
Concen: 1.22 ng/ul
RT: 21.81 min Scan# 3228
Delta R.T. 0.01 min
Lab File: BG021918.D
Acq: 16 May 2016 22:45

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	26331		
229	27.7		16.6	25.0#
226	33.0		21.0	31.4#

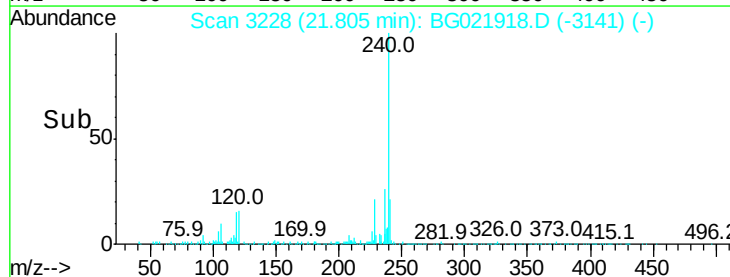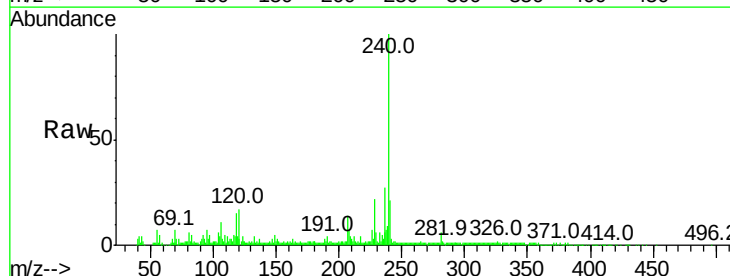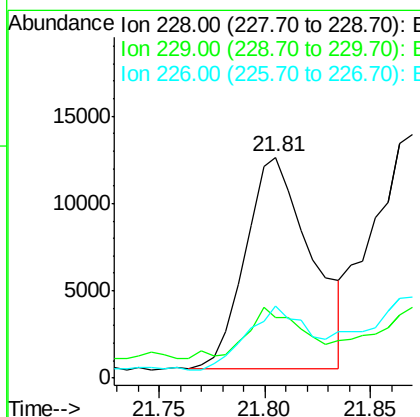

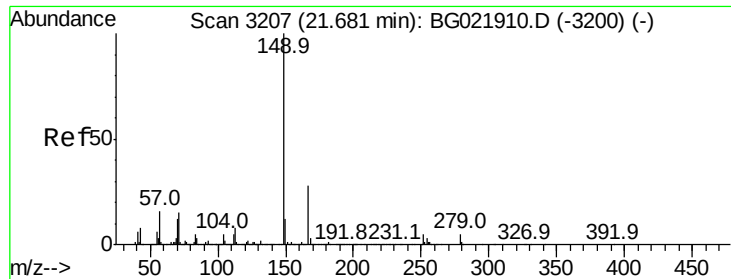





#82
 Bis(2-ethylhexyl)phthalate
 Concen: 12.59 ng/ul
 RT: 21.69 min Scan# 3208
 Delta R.T. 0.01 min
 Lab File: BG021918.D
 Acq: 16 May 2016 22:45

Instrument :
 BNA_G
 ClientSampleId :
 D9XE6

Tot Ion	Ratio	Resp Lower	Upper
149	100		
167	28.6	20.5	30.7
279	5.4	3.7	5.5




Manual Integrations
 APPROVED


umangi
 5/17/2016 7:20:40 PM

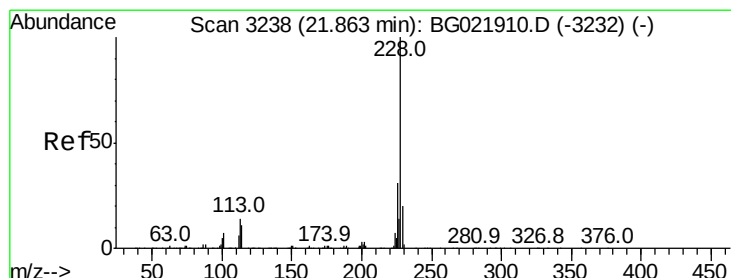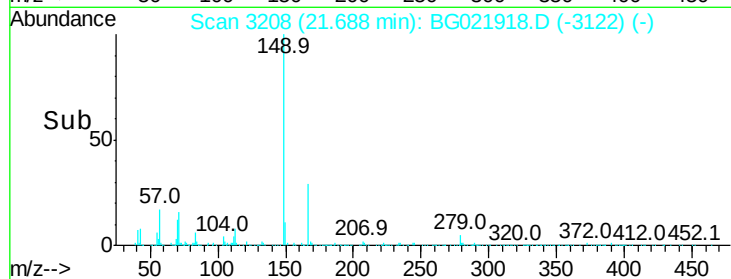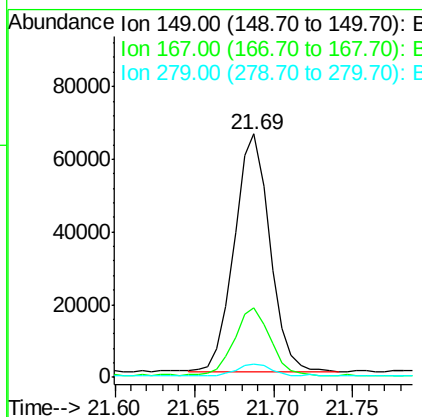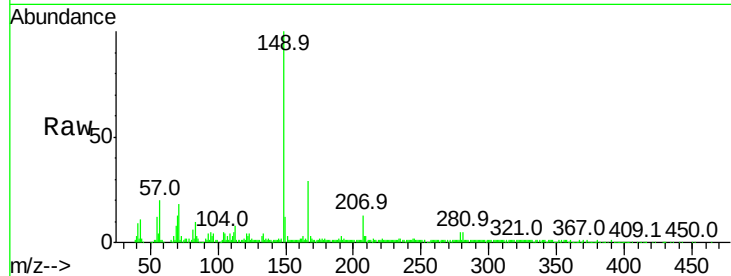

#83
 Chrysene
 Concen: 1.34 ng/ul
 RT: 21.87 min Scan# 3239
 Delta R.T. 0.01 min
 Lab File: BG021918.D
 Acq: 16 May 2016 22:45

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
226	33.0	23.4	35.2
229	29.1	16.2	24.2

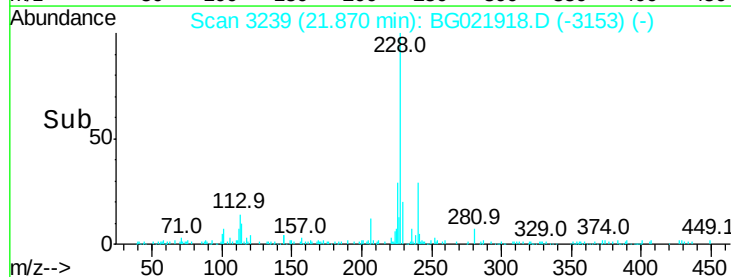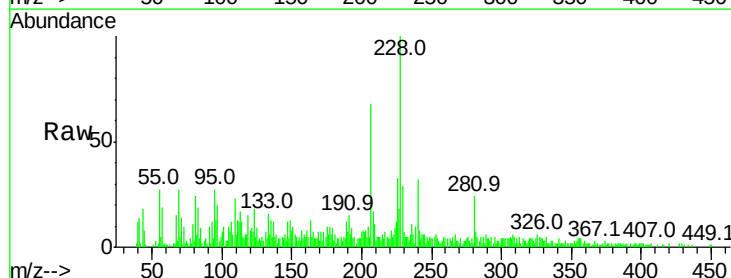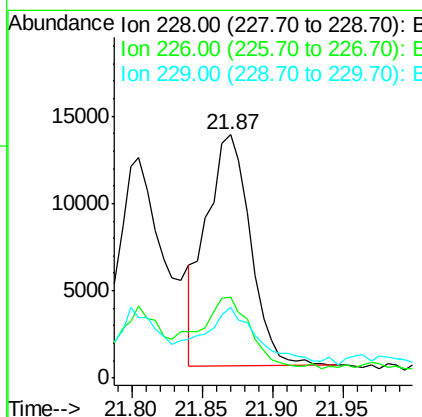

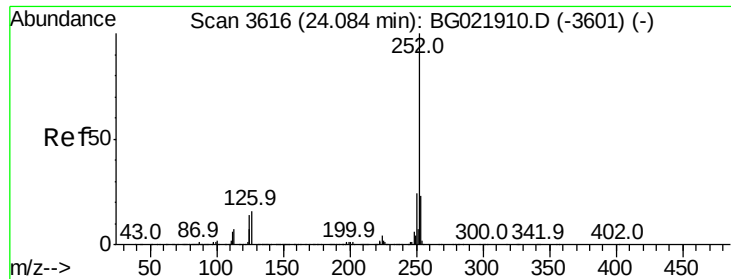

#86

Benzo(b)fluoranthene

Concen: 2.21 ng/ul

RT: 24.11 min Scan# 3620

Delta R.T. 0.02 min

Lab File: BG021918.D

Acq: 16 May 2016 22:45

Instrument :

BNA_G


ClientSampleId :

D9XE6




Tot Ion:	252	Resp:	50486
Ion Ratio	Lower	Upper	
252	100		
253	32.9	18.1	27.1#
125	22.1	7.6	11.4#

Manual Integrations
APPROVED

umangi
5/17/2016 7:20:40 PM

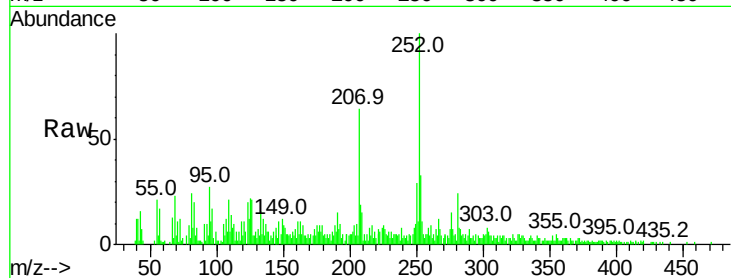

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

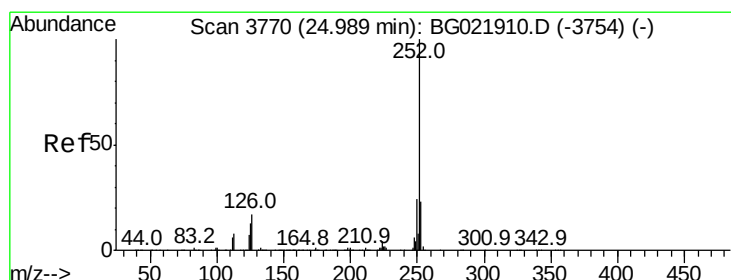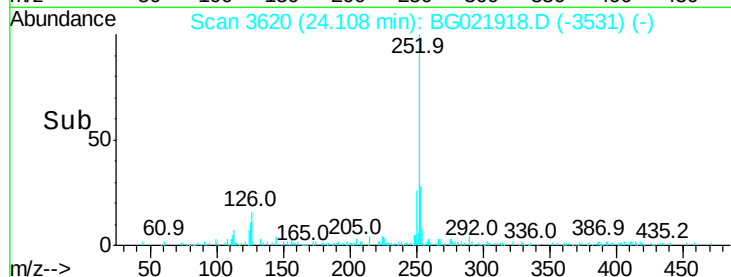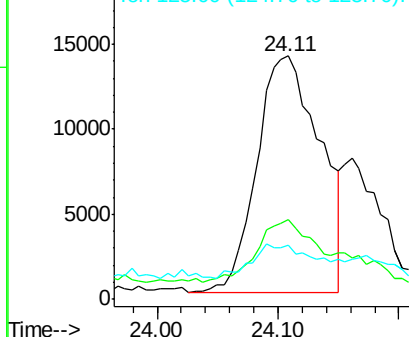

#89

Benzo(a)pyrene

Concen: 1.27 ng/ul


RT: 25.02 min Scan# 3775

Delta R.T. 0.03 min

Lab File: BG021918.D

Acq: 16 May 2016 22:45

Tgt Ion:	252	Resp:	28815
Ion Ratio	Lower	Upper	
252	100		
253	31.3	17.4	26.0#
125	26.9	8.2	12.2#

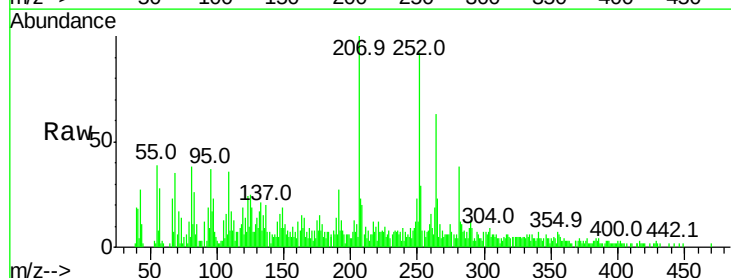

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

