

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051617\
 Data File : BG026988.D
 Acq On : 16 May 2017 21:32
 Operator : SJ/MA
 Sample : I3106-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESXS7

Quant Time: May 17 04:09:08 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 17 04:07:33 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	181976	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	871081	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.61	164	468901	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	877963	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	806507	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	810918	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	5074	1.26	ng/uL	0.00
5) Phenol-d5	7.18	99	118045	7.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	264935	27.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	309750	22.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	206714	15.34	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	197465	27.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	213973	27.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	309900	24.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	13050	0.77	ng/ul	0.02
43) Dimethylphthalate-d6	14.02	166	1063948	28.19	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1356728	28.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.86	143	32187	4.73	ng/ul	0.02
57) Fluorene-d10	15.60	176	888636	26.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	109263	20.49	ng/ul	0.00
70) Anthracene-d10	17.45	188	1241636	29.14	ng/ul	0.00
76) Pyrene-d10	19.73	212	1196562	28.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1146967	29.92	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.06	163	50110	1.36	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051617\
Data File : BG026988.D
Acq On : 16 May 2017 21:32
Operator : SJ/MA
Sample : I3106-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESXS7

Quant Time: May 17 04:09:08 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 17 04:07:33 2017
Response via : Initial Calibration

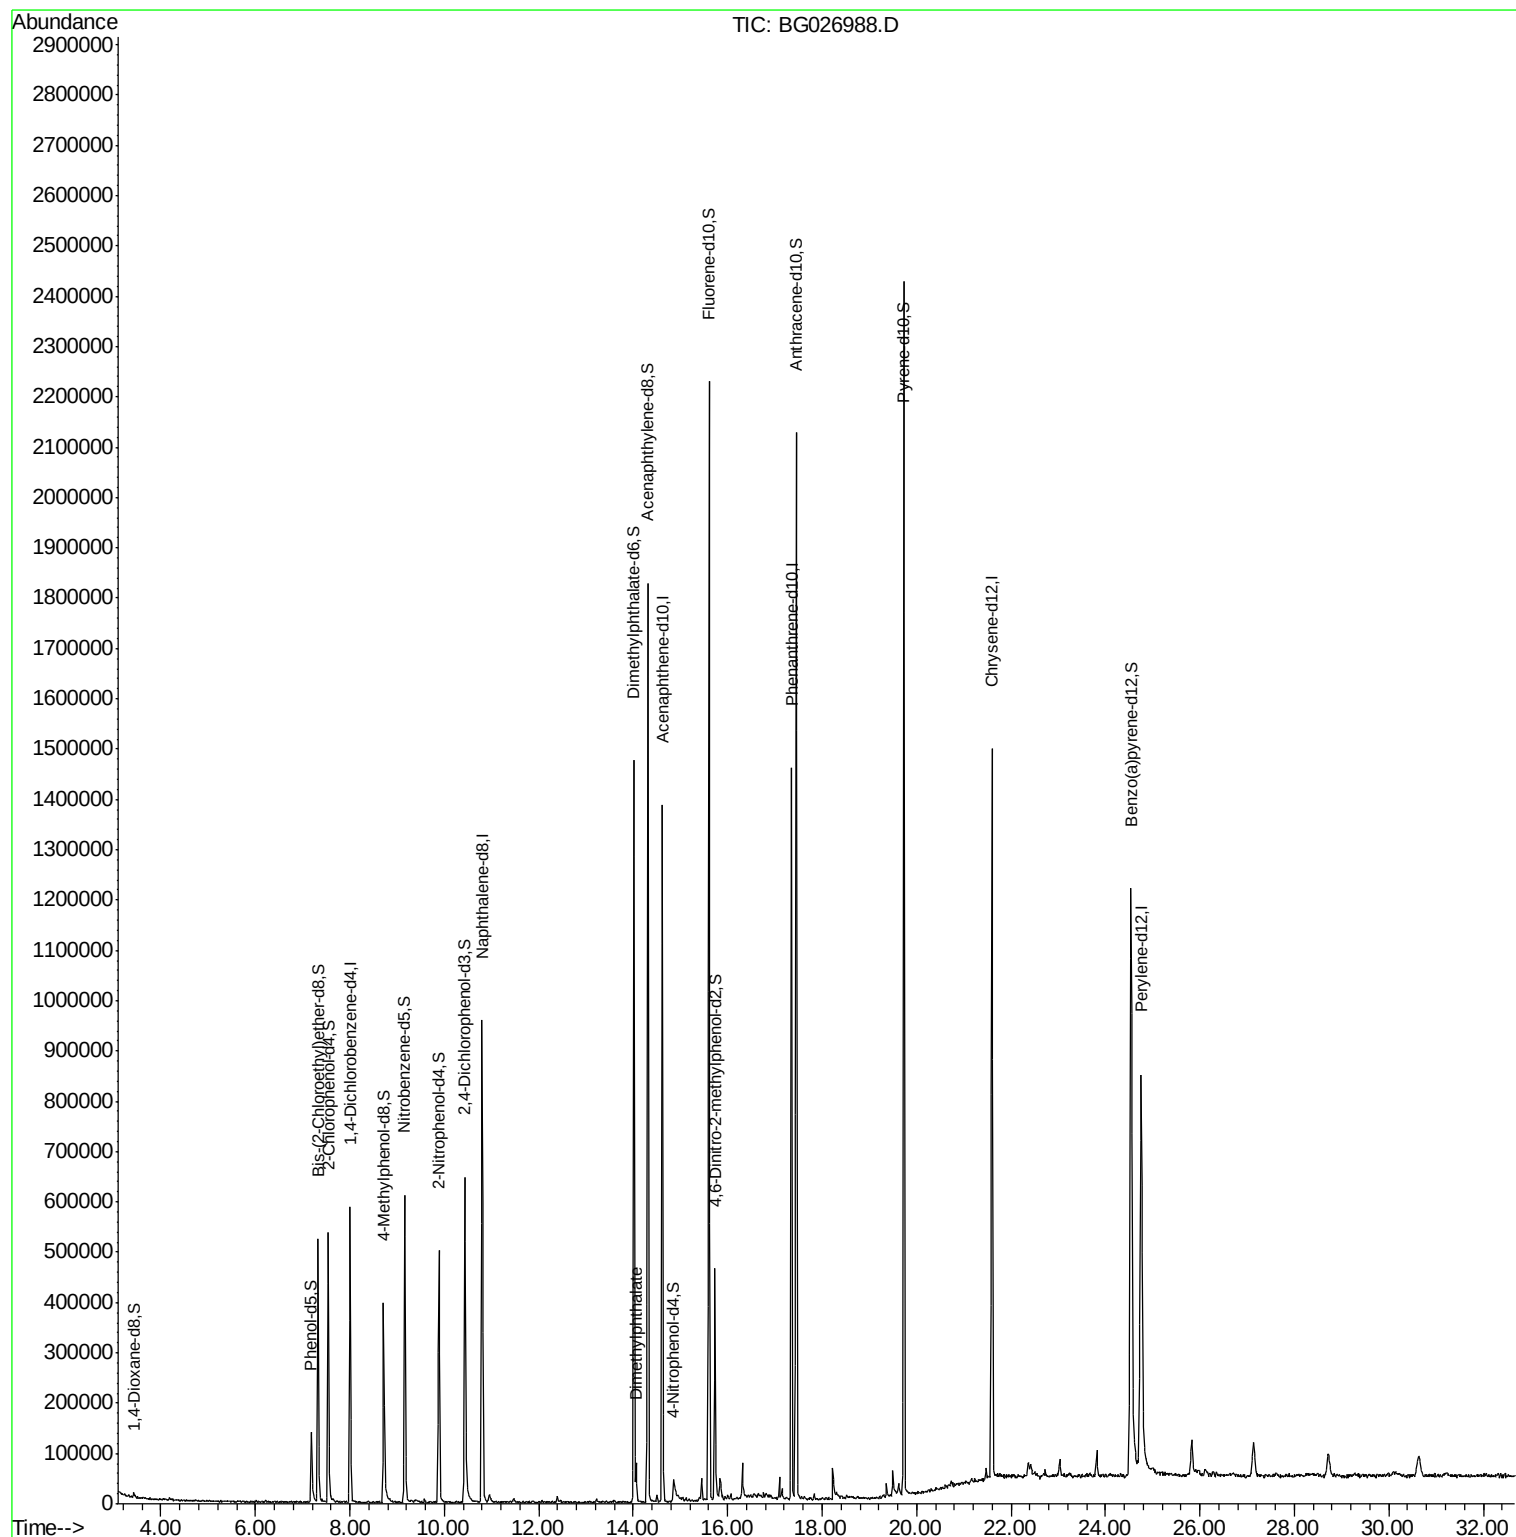

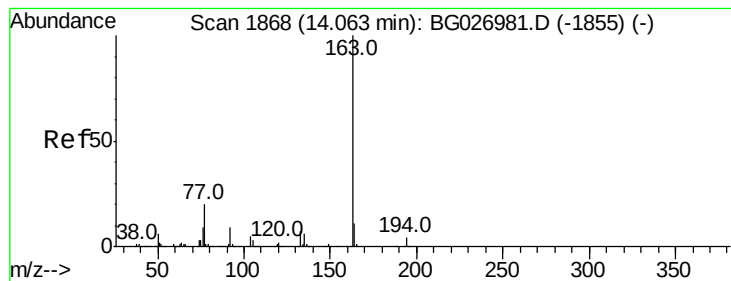

#44

Dimethylphthalate

Concen: 1.36 ng/ul

RT: 14.06 min Scan# 1868

Delta R.T. -0.00 min

Lab File: BG026988.D

Acq: 16 May 2017 21:32

Instrument :

BNA_G

ClientSampleId :

ESXS7


Tot Ion:163 Resp: 50110

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.0

164 9.4 9.0 13.4

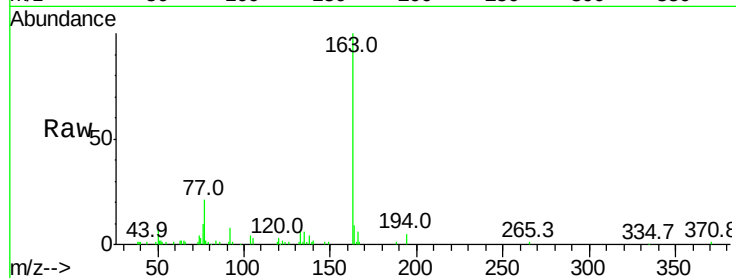

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

