

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051617\
 Data File : BG026997.D
 Acq On : 17 May 2017 3:27
 Operator : SJ/MA
 Sample : I3106-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESXN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.232	22	24	34	rVB7	4800	9568	0.20%	0.018%
2	3.432	49	58	67	rVB7	13286	35480	0.73%	0.068%
3	3.861	130	131	140	rVB6	4126	7926	0.16%	0.015%
4	3.972	143	150	151	rVB6	3085	6251	0.13%	0.012%
5	4.190	181	187	193	rBV4	5873	11083	0.23%	0.021%
6	4.718	268	277	283	rVB4	12526	26630	0.55%	0.051%
7	6.211	526	531	536	rBV5	5291	9455	0.20%	0.018%
8	7.180	690	696	712	rVV	186499	367127	7.57%	0.701%
9	7.327	712	721	733	rBV	757134	1274580	26.30%	2.434%
10	7.427	734	738	745	rVB6	5226	10519	0.22%	0.020%
11	7.539	749	757	769	rBV	749188	1354581	27.95%	2.587%
12	8.003	827	836	850	rBV	686460	1167928	24.10%	2.231%
13	8.720	950	958	984	rBV	577134	1160518	23.94%	2.217%
14	9.160	1024	1033	1051	rBV	875948	1573234	32.46%	3.005%
15	9.583	1099	1105	1109	rVB2	6574	10600	0.22%	0.020%
16	9.883	1147	1156	1171	rBV	731709	1331961	27.48%	2.544%
17	10.435	1238	1250	1272	rBV	996010	2030977	41.90%	3.879%
18	10.600	1277	1278	1285	rVB5	3557	4979	0.10%	0.010%
19	10.800	1303	1312	1328	rVB	1077853	1983082	40.91%	3.788%
20	10.952	1328	1338	1349	rBV3	17514	50565	1.04%	0.097%
21	11.311	1392	1399	1400	rVB4	2570	5387	0.11%	0.010%
22	11.458	1416	1424	1437	rVB3	18991	40623	0.84%	0.078%
23	12.063	1523	1527	1532	rVB3	4885	8623	0.18%	0.016%
24	12.386	1576	1582	1595	rVB	18731	40436	0.83%	0.077%
25	12.597	1607	1618	1626	rBV7	3137	11374	0.23%	0.022%
26	13.226	1719	1725	1730	rBV6	6823	13429	0.28%	0.026%
27	13.302	1736	1738	1744	rVB3	2601	4889	0.10%	0.009%
28	13.361	1744	1748	1752	rBV4	2719	5384	0.11%	0.010%
29	13.596	1784	1788	1793	rVB3	4835	7221	0.15%	0.014%
30	14.019	1852	1860	1877	rBV	2027893	2973755	61.35%	5.680%
31	14.143	1877	1881	1889	rVV5	3542	8397	0.17%	0.016%
32	14.313	1898	1910	1928	rBV	2528190	4009122	82.71%	7.658%
33	14.619	1954	1962	1977	rVB2	1492651	2534329	52.29%	4.841%
34	14.854	1990	2002	2022	rBV3	58200	221335	4.57%	0.423%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051617\
 Data File : BG026997.D
 Acq On : 17 May 2017 3:27
 Operator : SJ/MA
 Sample : I3106-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESXN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Title : SVOA CALIBRATION

35	14.977	2022	2023	2034	rVB7	4741	9583	0.20%	0.018%
36	15.341	2081	2085	2090	rVB6	2869	5012	0.10%	0.010%
37	15.400	2090	2095	2102	rBV3	11222	19390	0.40%	0.037%
38	15.606	2122	2130	2145	rBV	2964441	4624009	95.40%	8.832%
39	15.729	2145	2151	2165	rBV	709086	1104999	22.80%	2.111%
40	15.847	2165	2171	2176	rVB	40592	67037	1.38%	0.128%
41	16.029	2198	2202	2206	rBV4	3881	5253	0.11%	0.010%
42	16.099	2211	2214	2220	rBV6	2815	6339	0.13%	0.012%
43	16.187	2220	2229	2232	rVV6	3086	7912	0.16%	0.015%
44	16.305	2245	2249	2251	rBV4	8567	12319	0.25%	0.024%
45	16.381	2257	2262	2269	rVB8	5955	9084	0.19%	0.017%
46	16.557	2284	2292	2295	rVB6	6642	13051	0.27%	0.025%
47	16.657	2304	2309	2316	rVB7	3556	9666	0.20%	0.018%
48	16.939	2351	2357	2361	rVB7	3982	7444	0.15%	0.014%
49	17.139	2387	2391	2397	rVV2	9679	16942	0.35%	0.032%
50	17.351	2417	2427	2437	rBV2	1711852	2644567	54.56%	5.051%
51	17.451	2437	2444	2463	rVB	3010180	4531389	93.49%	8.655%
52	17.738	2488	2493	2495	rBV6	5306	7702	0.16%	0.015%
53	18.003	2534	2538	2541	rBV6	8851	12186	0.25%	0.023%
54	18.232	2572	2577	2582	rBV8	11590	22819	0.47%	0.044%
55	18.302	2584	2589	2594	rVB2	7360	15601	0.32%	0.030%
56	18.426	2606	2610	2612	rBV4	4797	8097	0.17%	0.015%
57	18.596	2630	2639	2643	rBV4	7268	18923	0.39%	0.036%
58	18.731	2655	2662	2666	rBV8	8476	17519	0.36%	0.033%
59	18.814	2675	2676	2680	rVB4	6415	7625	0.16%	0.015%
60	18.849	2680	2682	2684	rBV3	6154	6482	0.13%	0.012%
61	19.266	2749	2753	2754	rBV4	5256	6597	0.14%	0.013%
62	19.366	2765	2770	2773	rBV	40813	64072	1.32%	0.122%
63	19.395	2773	2775	2784	rVB	34838	54613	1.13%	0.104%
64	19.495	2788	2792	2800	rBV9	18152	35518	0.73%	0.068%
65	19.548	2800	2801	2805	rBV4	7902	6692	0.14%	0.013%
66	19.624	2809	2814	2822	rVB	33570	59400	1.23%	0.113%
67	19.730	2822	2832	2845	rBV	3290468	4839062	99.83%	9.243%
68	20.018	2879	2881	2884	rBV4	5799	6204	0.13%	0.012%
69	20.053	2886	2887	2890	rBV3	4970	5906	0.12%	0.011%
70	20.224	2909	2916	2917	rBV7	10174	17506	0.36%	0.033%
71	20.318	2929	2932	2934	rVB4	6409	6370	0.13%	0.012%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051617\
 Data File : BG026997.D
 Acq On : 17 May 2017 3:27
 Operator : SJ/MA
 Sample : I3106-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ESXN6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Title : SVOA CALIBRATION

72	20.494	2961	2962	2967	rVB5	7122	8515	0.18%	0.016%
73	20.547	2968	2971	2975	rBV6	10036	15264	0.31%	0.029%
74	21.011	3047	3050	3052	rBV4	6179	7884	0.16%	0.015%
75	21.152	3072	3074	3079	rBV6	10691	16348	0.34%	0.031%
76	21.469	3125	3128	3133	rVB3	13526	16151	0.33%	0.031%
77	21.593	3141	3149	3162	rBV	1642672	2780330	57.36%	5.311%
78	22.362	3275	3280	3284	rBV7	27729	50759	1.05%	0.097%
79	23.032	3389	3394	3403	rVB4	39212	72427	1.49%	0.138%
80	23.767	3512	3519	3520	rBV7	17405	31810	0.66%	0.061%
81	23.814	3521	3527	3534	rVB4	68600	147117	3.04%	0.281%
82	24.542	3639	3651	3674	rBV2	1557394	4847080	100.00%	9.258%
83	24.760	3676	3688	3716	rVB3	891473	2986154	61.61%	5.704%
84	25.829	3862	3870	3879	rBV3	69681	205955	4.25%	0.393%
85	27.133	4084	4092	4102	rVB4	62974	193165	3.99%	0.369%
86	27.398	4134	4137	4141	rBV6	11978	20483	0.42%	0.039%
87	28.720	4353	4362	4375	rVB5	44288	182679	3.77%	0.349%
88	30.629	4677	4687	4699	rVB4	35635	148555	3.06%	0.284%


Sum of corrected areas: 52354914

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051617\
Data File : BG026997.D
Acq On : 17 May 2017 3:27
Operator : SJ/MA
Sample : I3106-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ESXN6

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

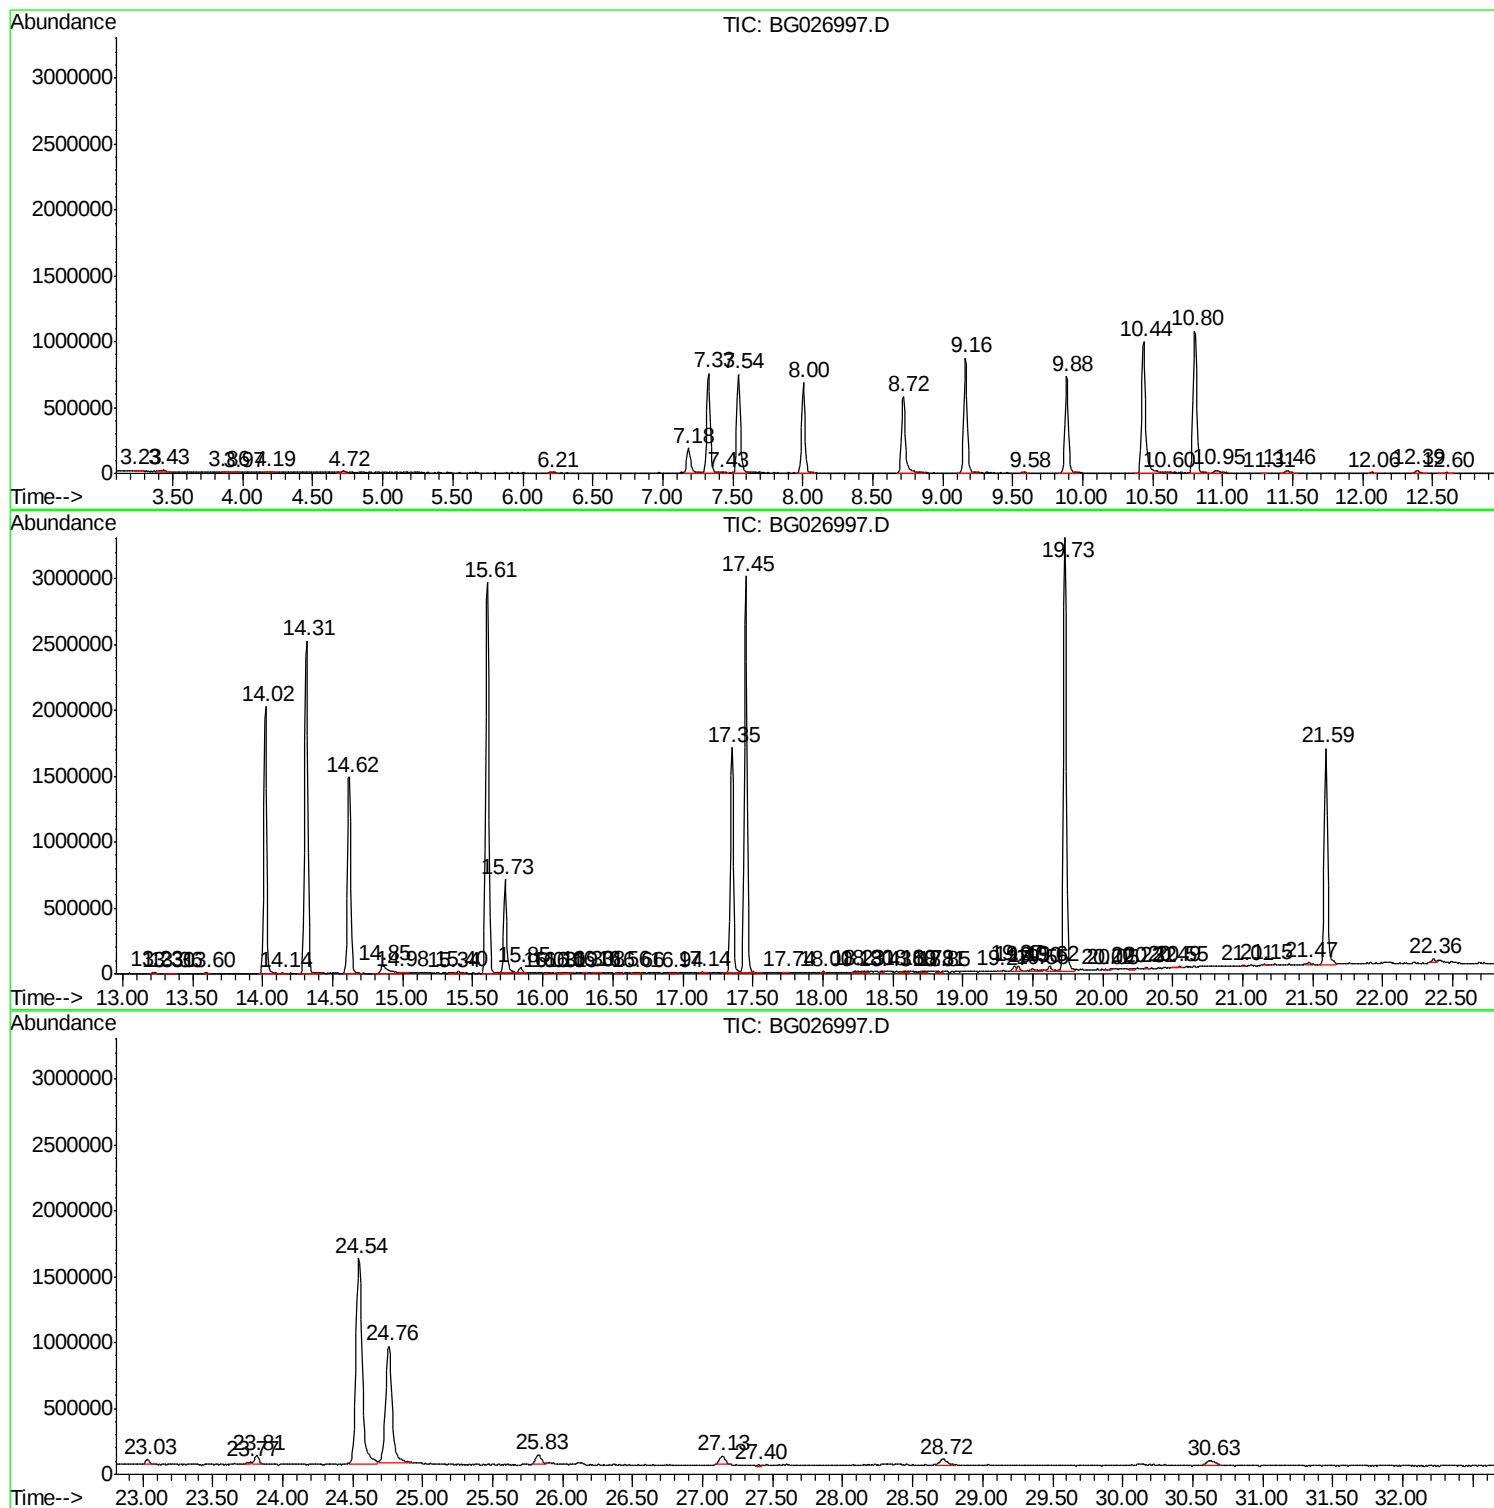

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG051617\
Data_File : BG026997.D
Acq_On : 17 May, 2017 3:27
Operator : SJ/MAA
Sample : I3106-099
Misc :
ALS_Vial : 18 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
ESXN6

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.MM
Quant_Title : SVOA CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
