
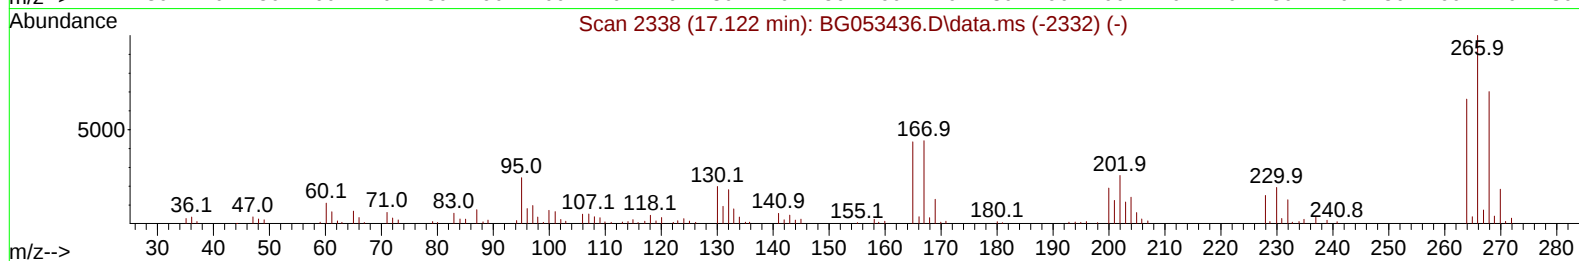
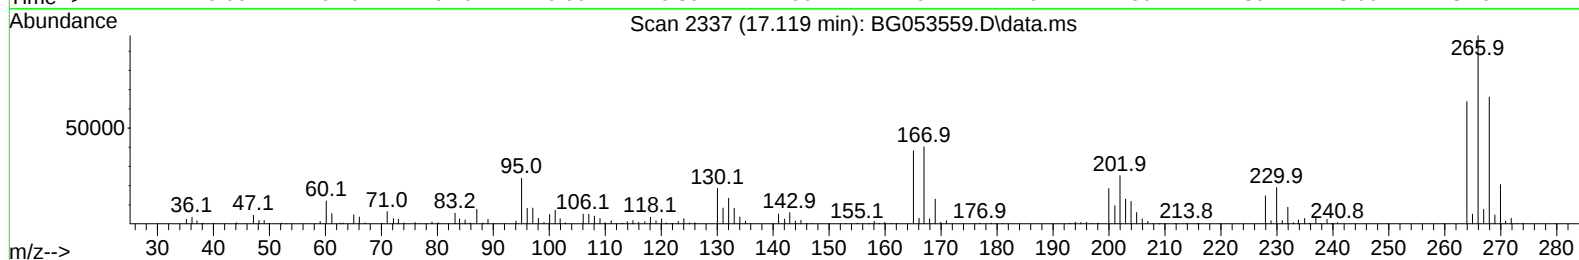


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053559.D
Acq On : 16 May 2022 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 15:29:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

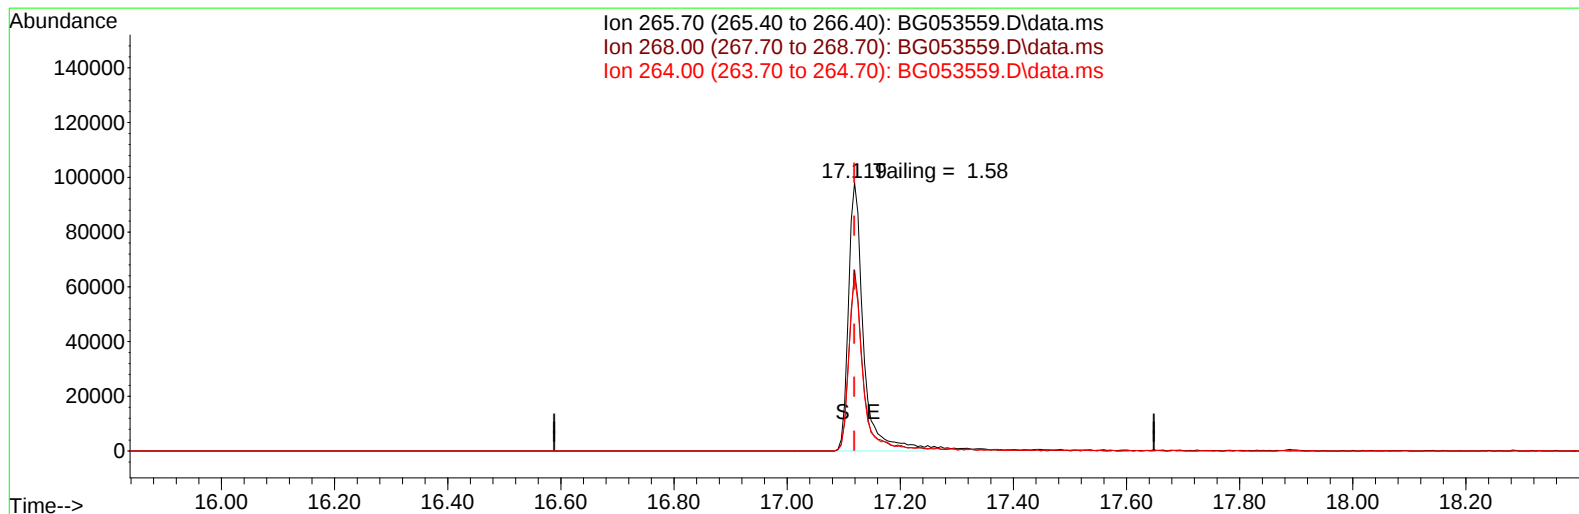

TIC: BG053559.D\data.ms

(70) Pentachlorophenol (C)




17.119min (+ 0.001) 32707.83 ng

response 181048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.38
264.00	66.20	65.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053559.D
Acq On : 16 May 2022 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 15:29:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

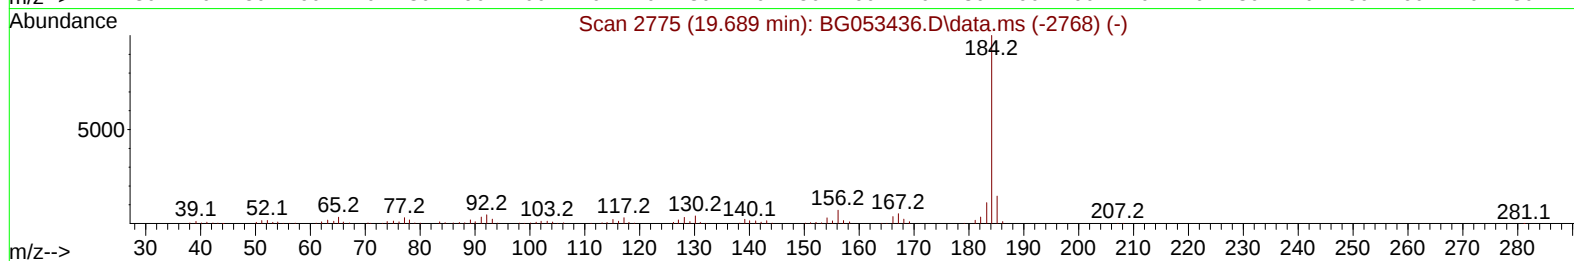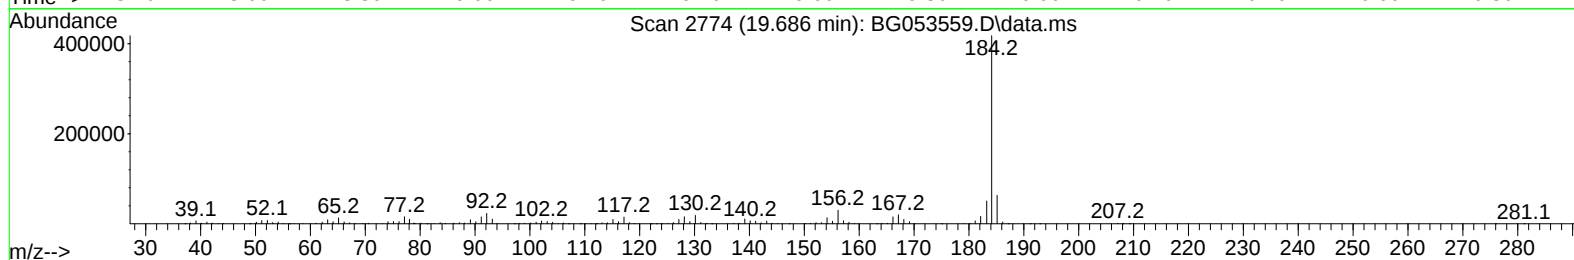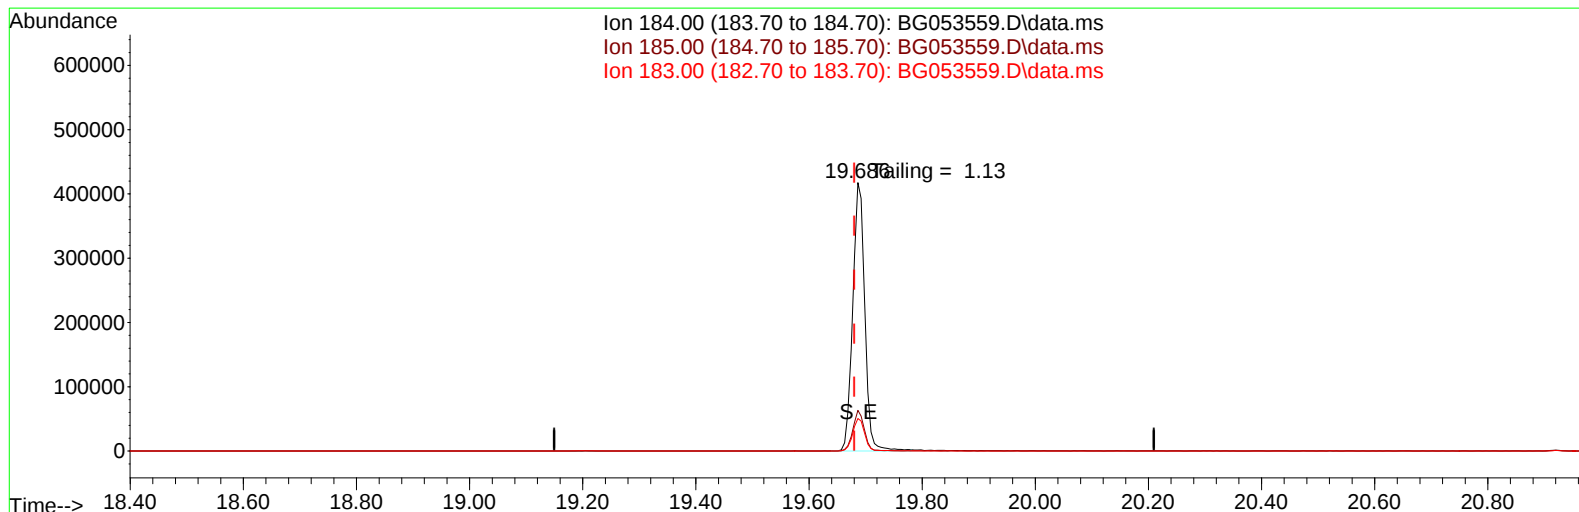

TIC: BG053559.D\data.ms

(77) Benzidine

19.686min (+ 0.007) 489535.77 ng

response 622527

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.18
183.00	11.10	12.10
0.00	0.00	0.00