

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
 Data File : BG053561.D
 Acq On : 16 May 2022 10:54
 Operator : CG/JU
 Sample : PB144792BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB144792BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.657	379	386	402	rBV	513395	843552	28.90%	7.891%
2	7.255	651	658	671	rBV	546875	959941	32.88%	8.980%
3	8.089	793	800	808	rBV	88026	154595	5.30%	1.446%
4	9.252	989	998	1009	rBV	339006	625895	21.44%	5.855%
5	10.903	1271	1279	1288	rBV	125576	230577	7.90%	2.157%
6	13.335	1686	1693	1703	rBV	968556	1547283	53.00%	14.475%
7	14.716	1921	1928	1936	rBV	239225	378121	12.95%	3.537%
8	16.202	2175	2181	2201	rBV	840245	1379243	47.25%	12.903%
9	17.459	2389	2395	2403	rBV	352406	535336	18.34%	5.008%
10	20.067	2832	2839	2845	rBV	2239369	2919190	100.00%	27.309%
11	21.741	3117	3124	3134	rVB	331928	568087	19.46%	5.314%
12	25.025	3674	3683	3697	rVB3	184907	547622	18.76%	5.123%




Sum of corrected areas: 10689442

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053561.D
Acq On : 16 May 2022 10:54
Operator : CG/JU
Sample : PB144792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB144792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

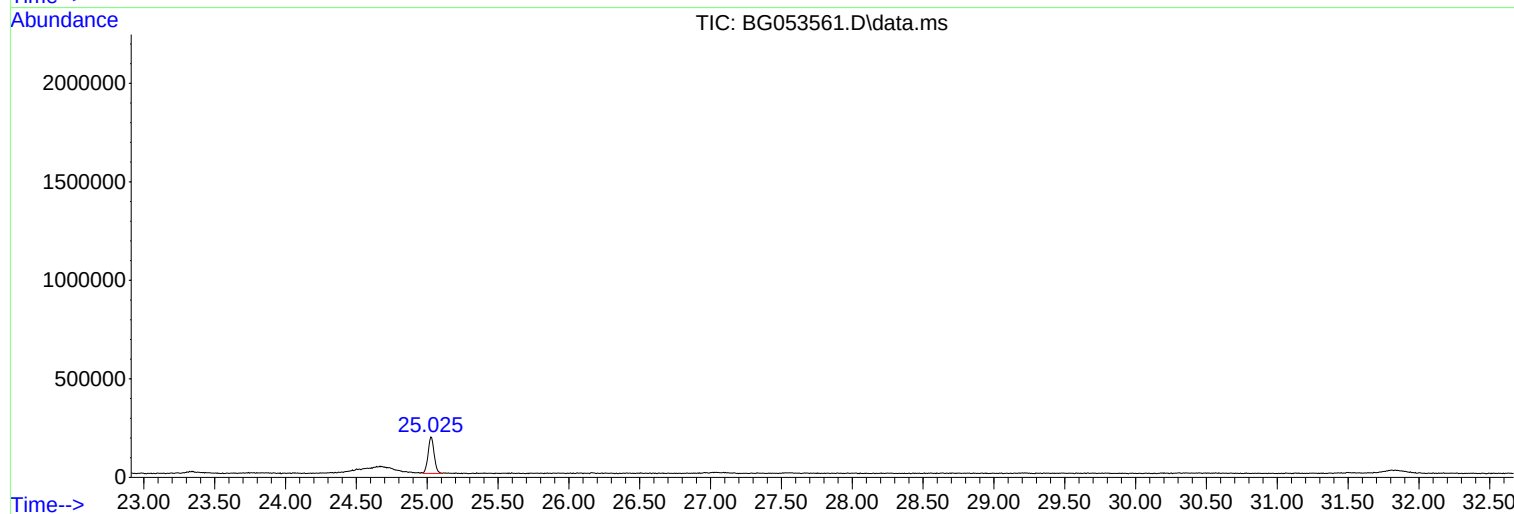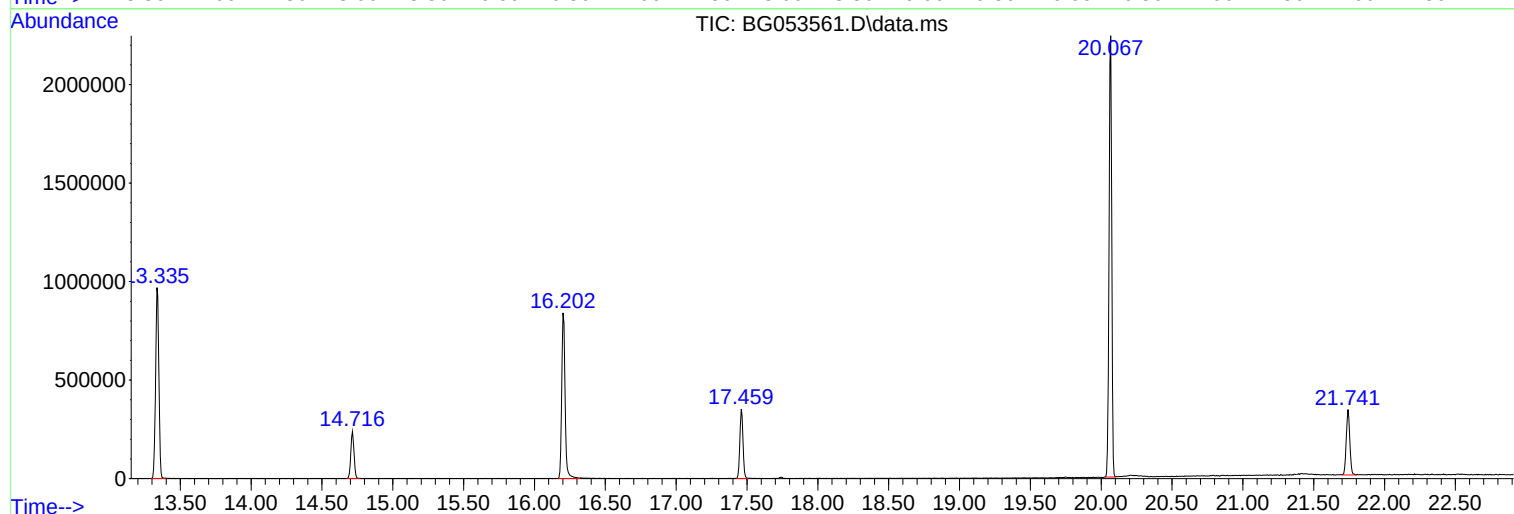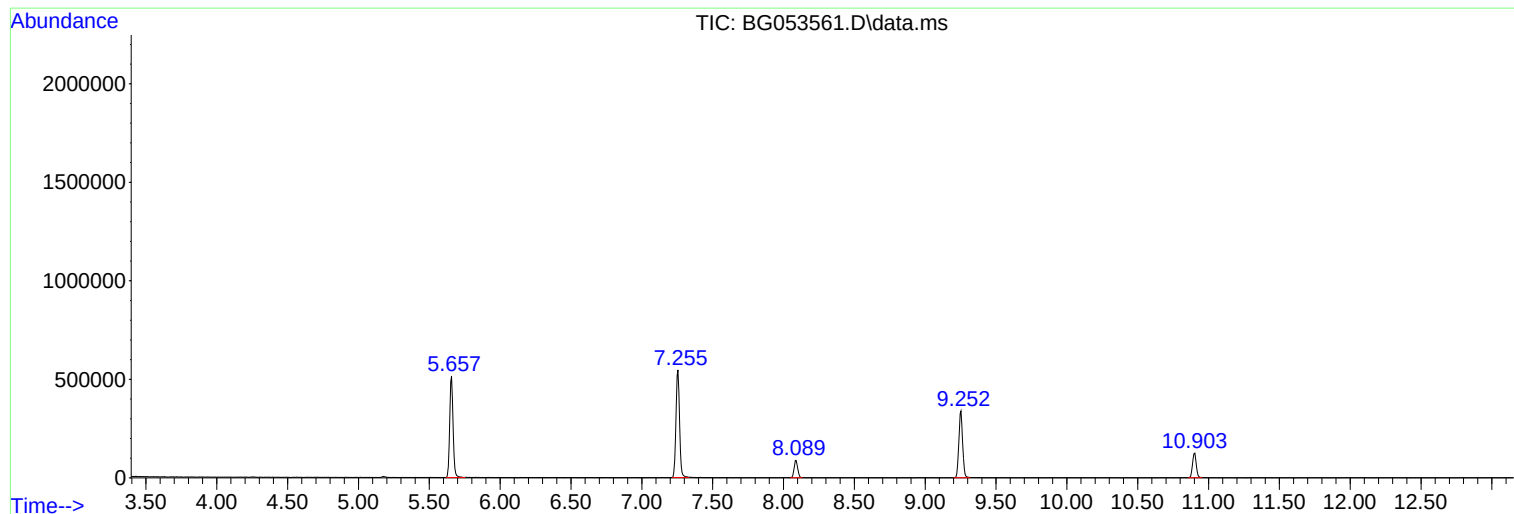

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053561.D
Acq On : 16 May 2022 10:54
Operator : CG/JU
Sample : PB144792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB144792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053561.D
Acq On : 16 May 2022 10:54
Operator : CG/JU
Sample : PB144792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB144792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------