

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
 Data File : BG053568.D
 Acq On : 16 May 2022 15:37
 Operator : CG/JU
 Sample : N2832-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.652	380	385	397	rBV	197647	341685	31.19%	6.500%
2	7.249	651	657	671	rBV	211792	387723	35.39%	7.376%
3	8.089	793	800	809	rBV	79254	139321	12.72%	2.650%
4	9.247	991	997	1008	rBV	126020	238628	21.78%	4.539%
5	10.897	1271	1278	1286	rBV	97797	185493	16.93%	3.529%
6	13.335	1685	1693	1700	rBV	342278	540388	49.33%	10.280%
7	14.716	1921	1928	1937	rVB	176585	286425	26.14%	5.449%
8	16.202	2175	2181	2200	rBV	319906	574834	52.47%	10.935%
9	17.459	2383	2395	2403	rBV	276921	442499	40.39%	8.418%
10	20.061	2832	2838	2846	rVB	859729	1095529	100.00%	20.840%
11	21.366	3056	3060	3073	rBV7	13305	34744	3.17%	0.661%
12	21.742	3118	3124	3133	rVB	299824	500289	45.67%	9.517%
13	25.025	3674	3683	3698	rVB3	165495	489258	44.66%	9.307%




Sum of corrected areas: 5256816

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053568.D
Acq On : 16 May 2022 15:37
Operator : CG/JU
Sample : N2832-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

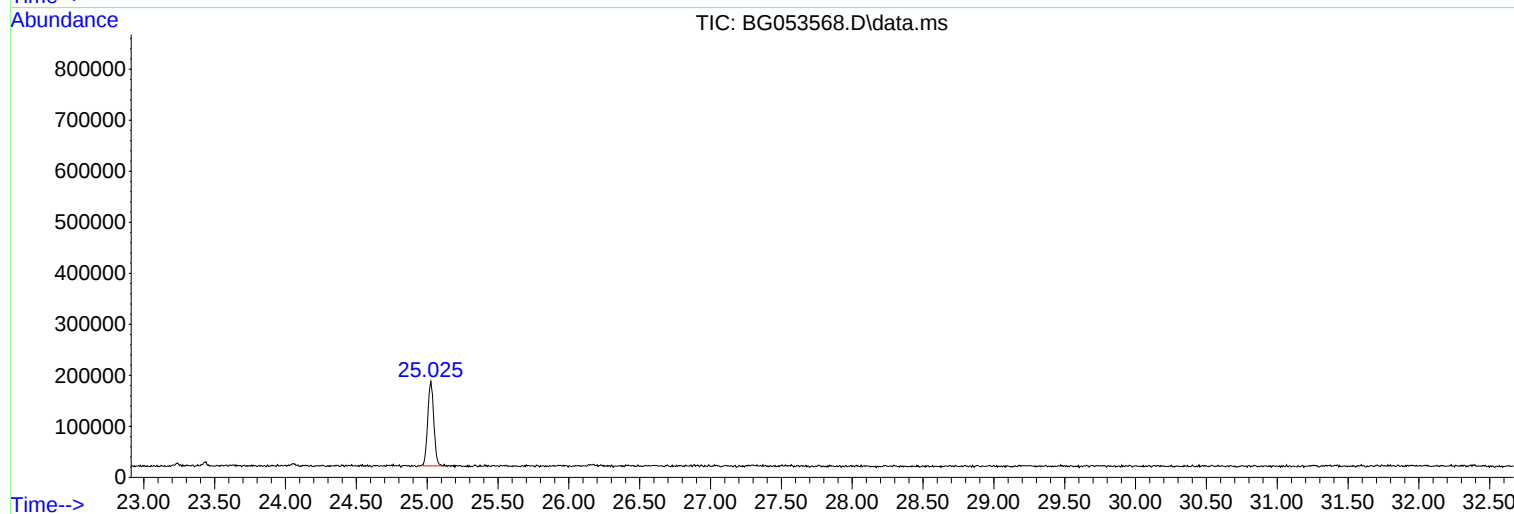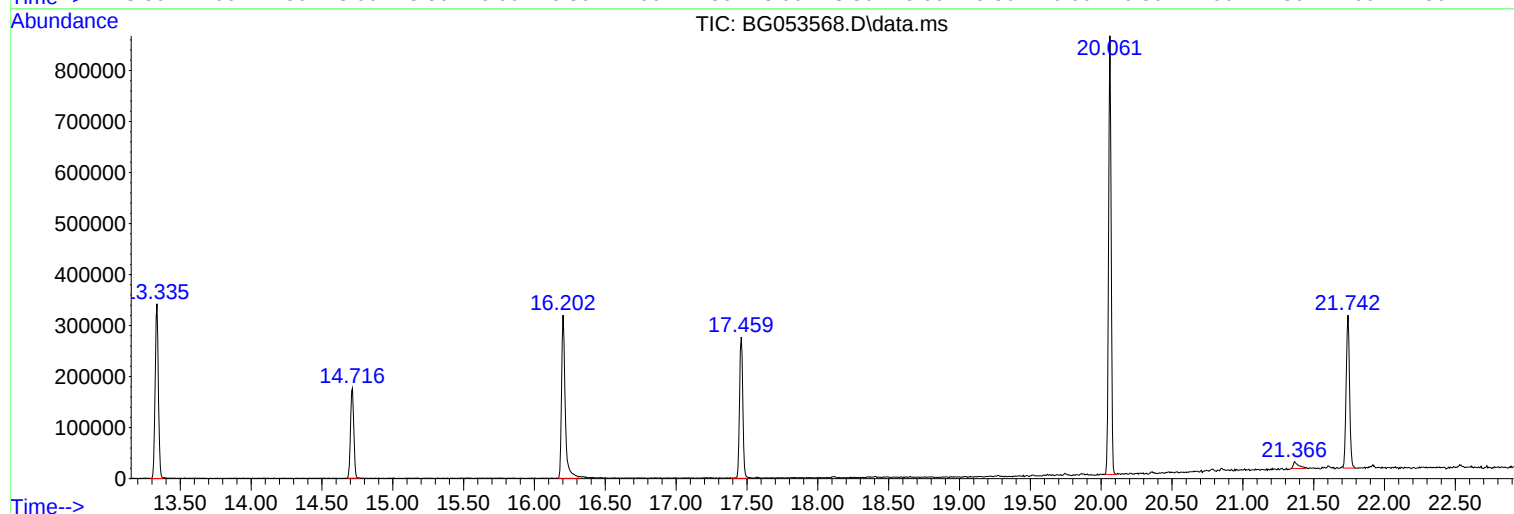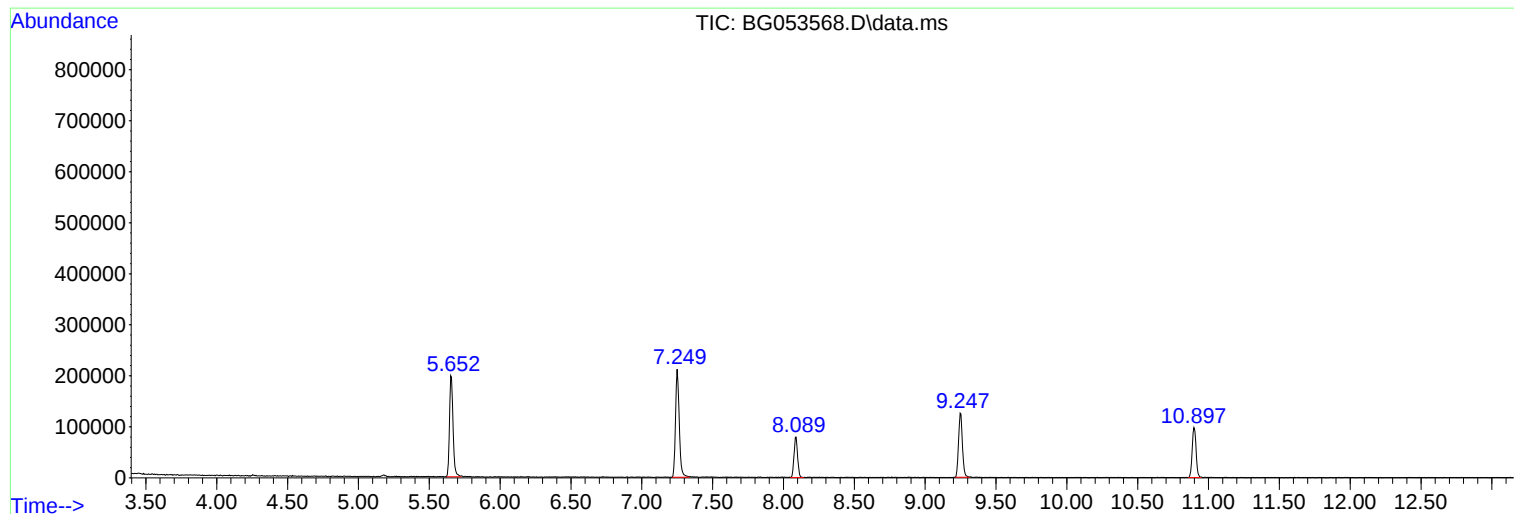

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053568.D
Acq On : 16 May 2022 15:37
Operator : CG/JU
Sample : N2832-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053568.D
Acq On : 16 May 2022 15:37
Operator : CG/JU
Sample : N2832-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------