

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
 Data File : BG053571.D
 Acq On : 16 May 2022 17:36
 Operator : CG/JU
 Sample : N2832-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.656	379	386	400	rBV	289097	484660	31.51%	6.899%
2	7.248	651	657	672	rBV	313636	567295	36.88%	8.075%
3	8.088	793	800	807	rVB	94055	161093	10.47%	2.293%
4	9.251	989	998	1008	rBV	186330	361644	23.51%	5.148%
5	10.896	1271	1278	1286	rBV	124425	228633	14.86%	3.255%
6	13.334	1686	1693	1703	rBV	552957	853911	55.52%	12.155%
7	14.715	1921	1928	1939	rBV	225950	366003	23.80%	5.210%
8	16.201	2175	2181	2200	rBV	450679	794253	51.64%	11.306%
9	17.458	2388	2395	2406	rBV	336688	515027	33.49%	7.331%
10	20.060	2832	2838	2844	rBV	1195175	1538066	100.00%	21.894%
11	21.370	3056	3061	3071	rBV8	16181	48002	3.12%	0.683%
12	21.740	3116	3124	3131	rBV	337352	560816	36.46%	7.983%
13	25.024	3673	3683	3696	rVB2	184123	545661	35.48%	7.767%




Sum of corrected areas: 7025064

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053571.D
Acq On : 16 May 2022 17:36
Operator : CG/JU
Sample : N2832-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

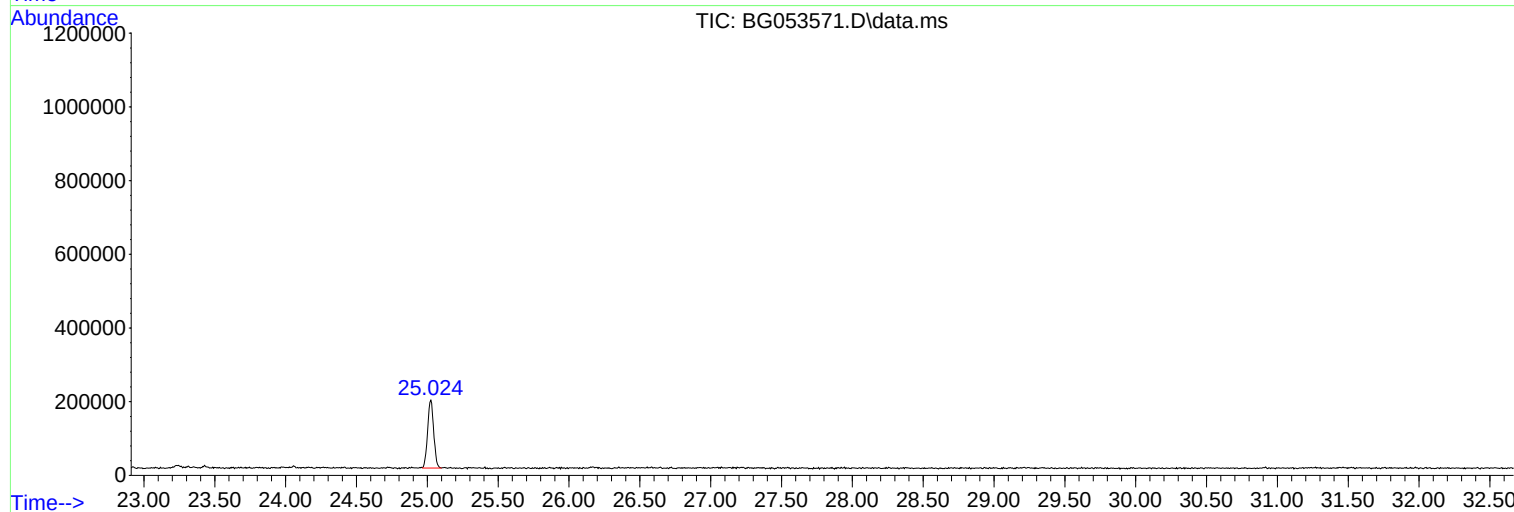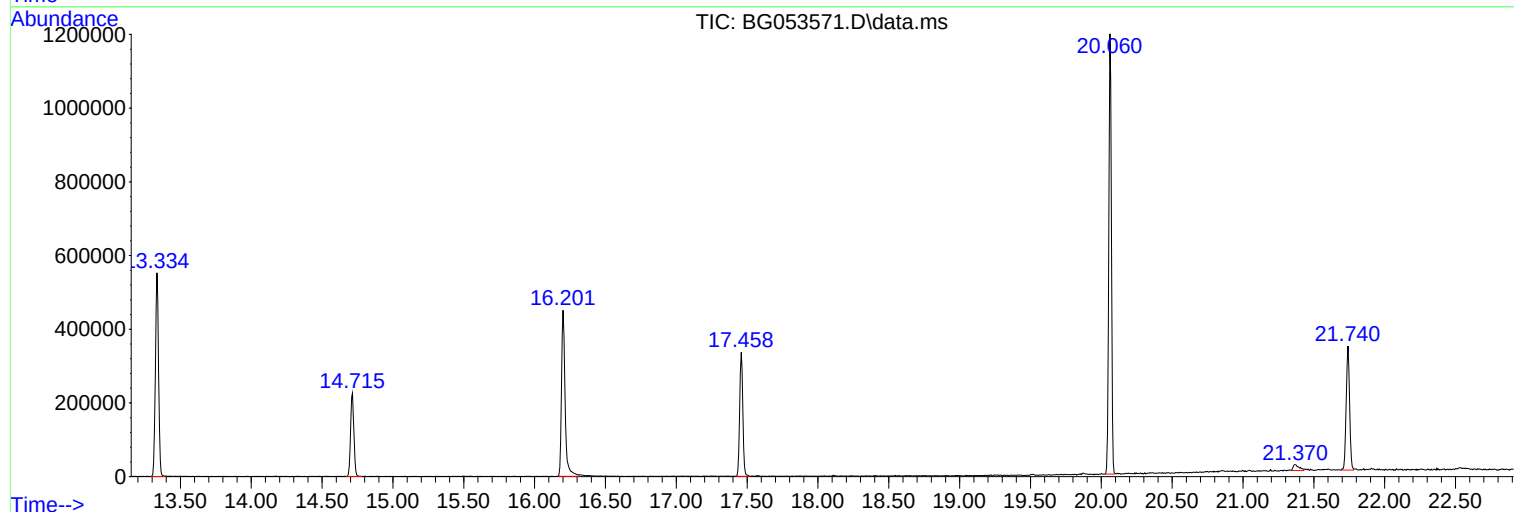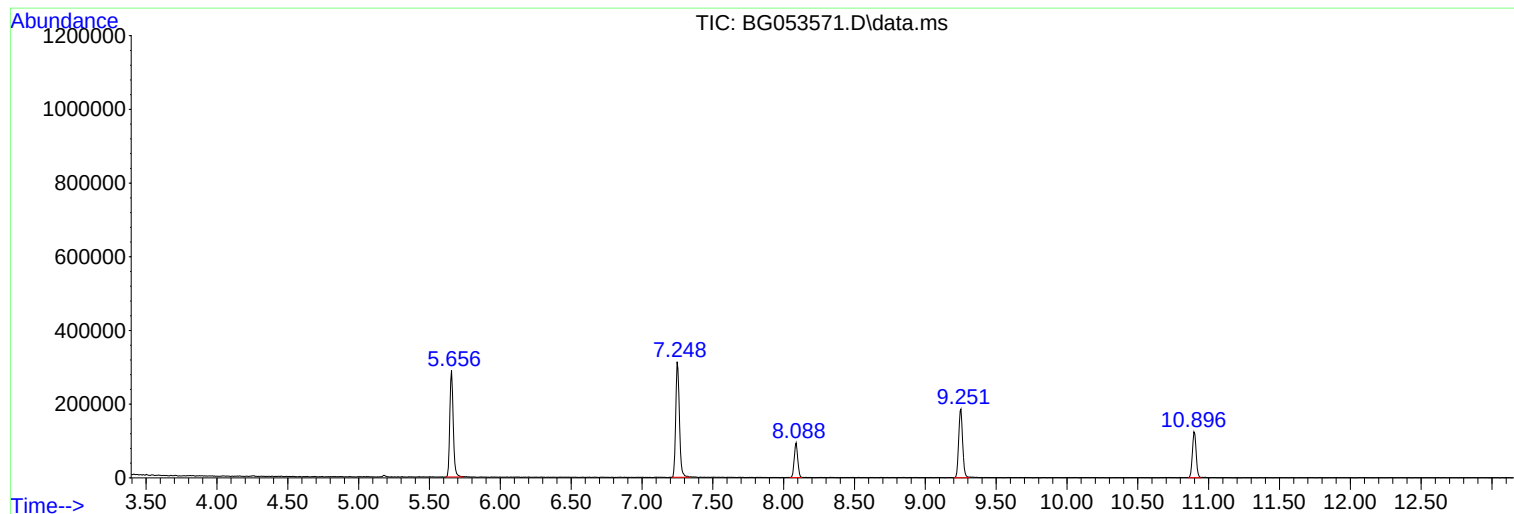

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053571.D
Acq On : 16 May 2022 17:36
Operator : CG/JU
Sample : N2832-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053571.D
Acq On : 16 May 2022 17:36
Operator : CG/JU
Sample : N2832-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------