

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
 Data File : BG053577.D
 Acq On : 16 May 2022 21:34
 Operator : CG/JU
 Sample : N2829-01 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-02-051222

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.656	381	386	396	rBV	44797	81961	14.33%	2.087%
2	7.254	651	658	673	rBV2	51062	105908	18.51%	2.697%
3	8.088	793	800	810	rBV	127407	219712	38.41%	5.596%
4	9.257	990	999	1008	rBV2	30262	64156	11.21%	1.634%
5	10.896	1271	1278	1292	rBV	173401	316510	55.33%	8.061%
6	13.334	1687	1693	1703	rBV	97047	153084	26.76%	3.899%
7	14.714	1919	1928	1935	rBV	281247	450749	78.79%	11.480%
8	14.779	1935	1939	1943	rVB2	4180	6147	1.07%	0.157%
9	15.760	2100	2106	2112	rBV3	4434	8838	1.54%	0.225%
10	16.206	2177	2182	2194	rBV2	48814	92868	16.23%	2.365%
11	17.193	2345	2350	2355	rBV2	3472	5992	1.05%	0.153%
12	17.457	2388	2395	2400	rBV	337333	528940	92.46%	13.472%
13	17.499	2400	2402	2409	rVB	38822	51162	8.94%	1.303%
14	17.593	2414	2418	2421	rBV2	7213	8989	1.57%	0.229%
15	17.863	2460	2464	2469	rBV6	4099	7034	1.23%	0.179%
16	17.933	2471	2476	2480	rVB4	4355	6314	1.10%	0.161%
17	18.339	2539	2545	2548	rBV4	9372	14293	2.50%	0.364%
18	18.380	2548	2552	2560	rVV4	9686	19786	3.46%	0.504%
19	18.474	2563	2568	2570	rVB5	4715	6565	1.15%	0.167%
20	18.532	2572	2578	2582	rVV4	13174	26106	4.56%	0.665%
21	18.568	2582	2584	2590	rVB6	7041	8979	1.57%	0.229%
22	18.626	2590	2594	2597	rBV3	5257	5976	1.04%	0.152%
23	18.826	2623	2628	2631	rBV4	5240	7874	1.38%	0.201%
24	19.126	2676	2679	2682	rBV4	4972	6615	1.16%	0.168%
25	19.249	2695	2700	2705	rBV4	13243	20258	3.54%	0.516%
26	19.508	2739	2744	2752	rBV	69246	99933	17.47%	2.545%
27	19.566	2752	2754	2757	rBV4	5495	6070	1.06%	0.155%
28	19.831	2797	2799	2801	rBV3	12034	13401	2.34%	0.341%
29	19.872	2801	2806	2814	rVB	61045	102809	17.97%	2.618%
30	19.948	2814	2819	2825	rBV10	7318	12655	2.21%	0.322%
31	20.060	2833	2838	2843	rBV	183894	233362	40.79%	5.944%
32	20.207	2861	2863	2868	rVB6	8785	11204	1.96%	0.285%
33	20.359	2884	2889	2893	rVB3	21048	28427	4.97%	0.724%
34	20.559	2922	2923	2928	rVB5	7627	7198	1.26%	0.183%
35	20.659	2937	2940	2944	rBV4	11240	19195	3.36%	0.489%
36	20.847	2971	2972	2976	rVB4	9414	9414	1.65%	0.240%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053577.D
Acq On : 16 May 2022 21:34
Operator : CG/JU
Sample : N2829-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-02-051222

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.364	3056	3060	3066	rBV9	16715	33730	5.90%	0.859%
38	21.599	3098	3100	3101	rBV2	8143	5906	1.03%	0.150%
39	21.740	3116	3124	3130	rBV2	312924	572067	100.00%	14.570%
40	25.030	3675	3684	3695	rVB2	184361	538565	94.14%	13.717%
41	29.482	4440	4442	4443	rBV2	9762	7540	1.32%	0.192%




Sum of corrected areas: 3926292

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053577.D
Acq On : 16 May 2022 21:34
Operator : CG/JU
Sample : N2829-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-02-051222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

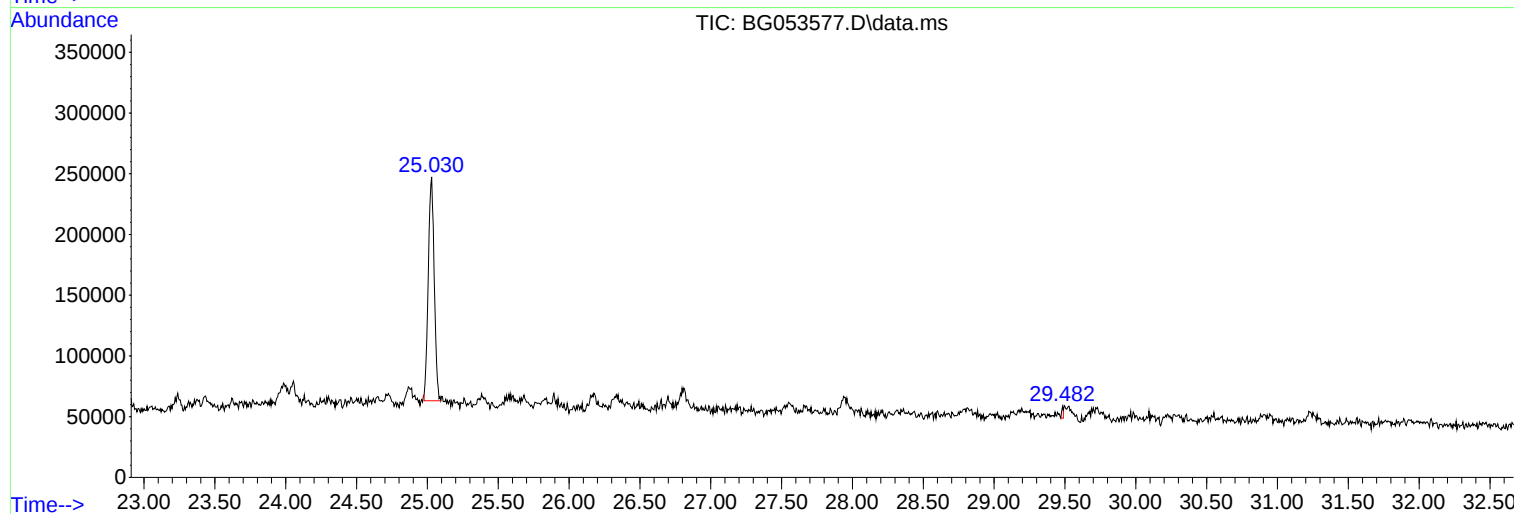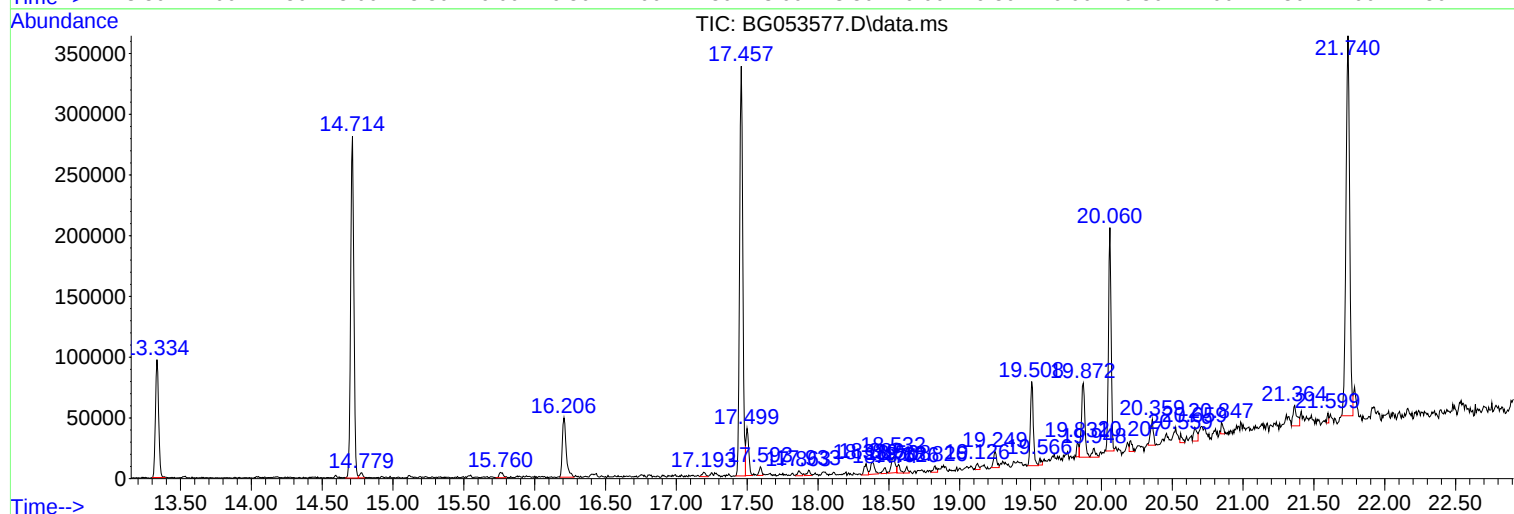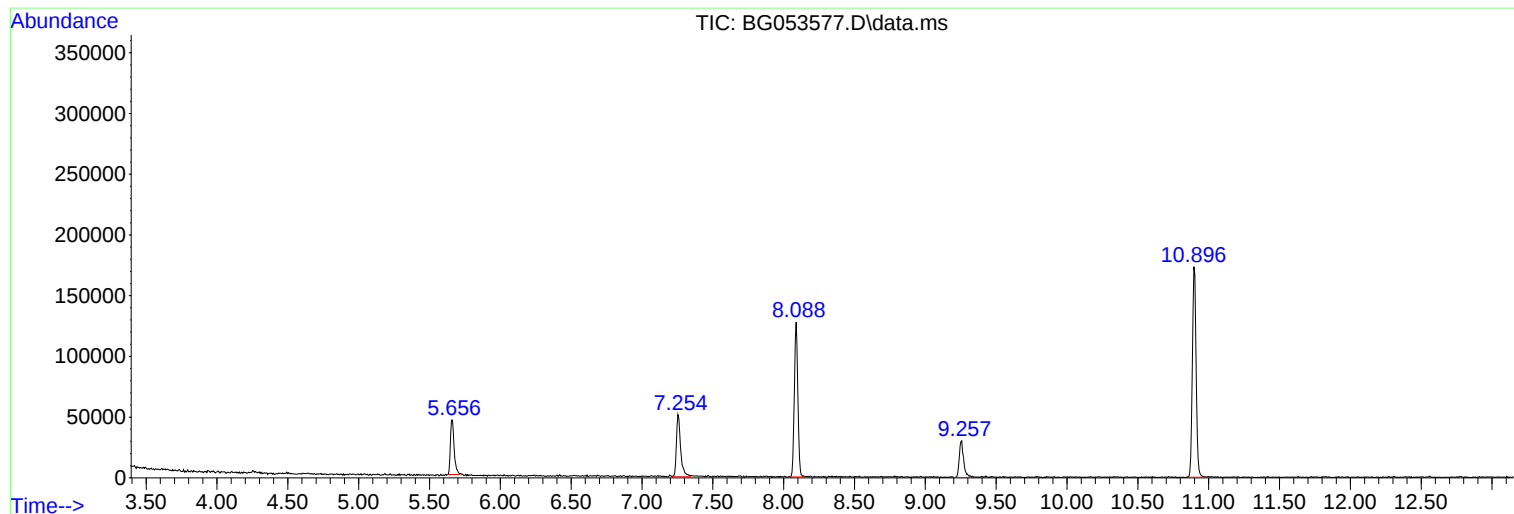

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053577.D
Acq On : 16 May 2022 21:34
Operator : CG/JU
Sample : N2829-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-02-051222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053577.D
Acq On : 16 May 2022 21:34
Operator : CG/JU
Sample : N2829-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-02-051222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------