
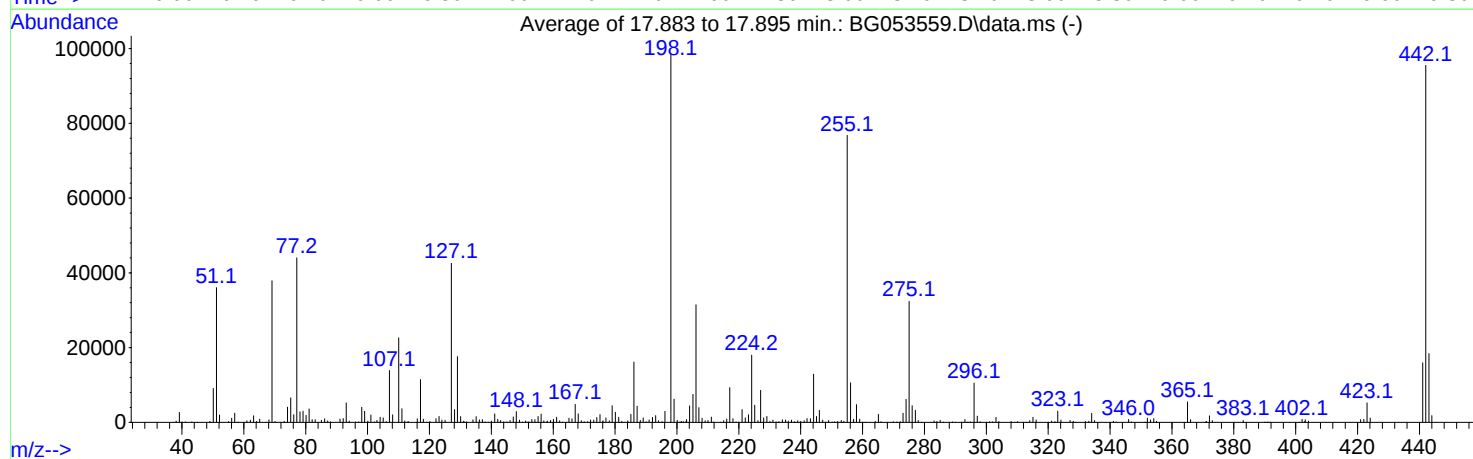


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
 Data File : BG053559.D
 Acq On : 16 May 2022 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 11 06:00:46 2022

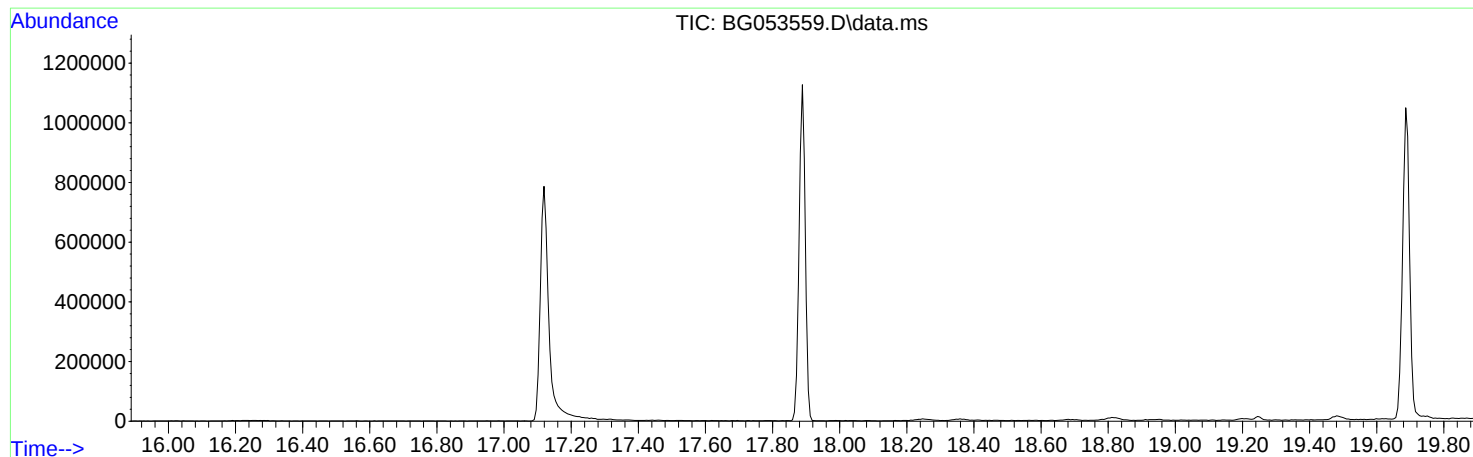




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	36032	PASS
68	69	0.00	2	1.8	677	PASS
69	198	0.00	100	38.5	37896	PASS
70	69	0.00	2	0.7	271	PASS
127	198	10	80	43.2	42552	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98408	PASS
199	198	5	9	6.3	6196	PASS
275	198	10	60	32.9	32379	PASS
365	198	1	100	5.6	5465	PASS
441	198	0.01	100	16.2	15917	PASS
442	442	50	100	100.0	95485	PASS
443	442	15	24	19.3	18426	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053559.D
Acq On : 16 May 2022 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 15:29:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

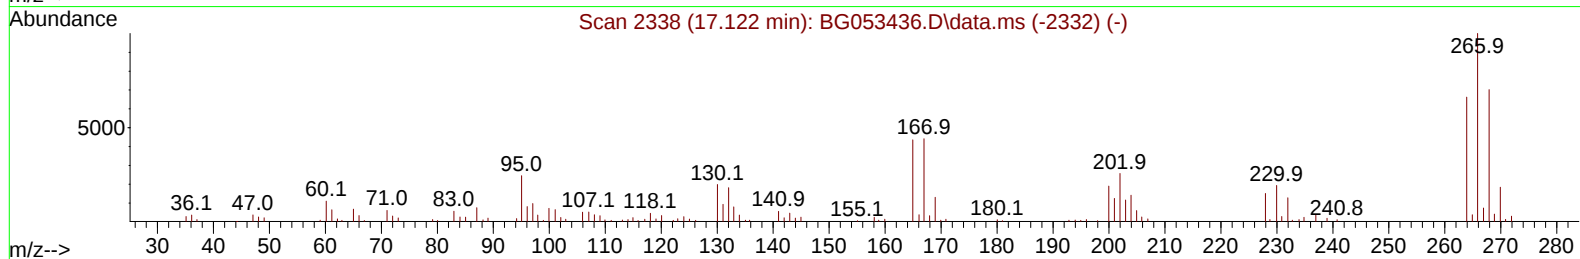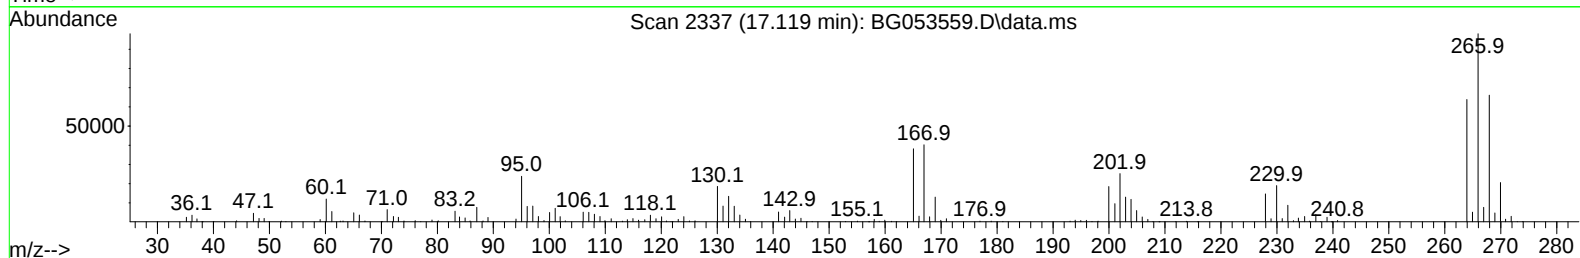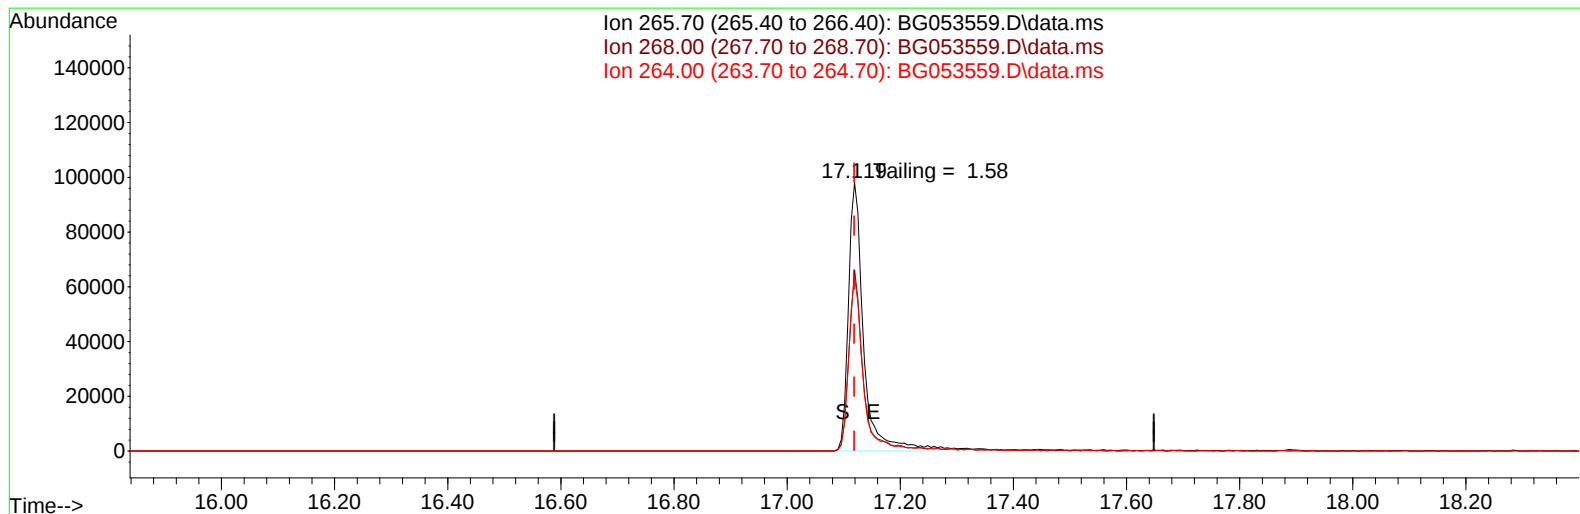

TIC: BG053559.D\data.ms

(70) Pentachlorophenol (C)

17.119min (+ 0.001) 32707.83 ng




response 181048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.38
264.00	66.20	65.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051622\
Data File : BG053559.D
Acq On : 16 May 2022 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 15:29:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

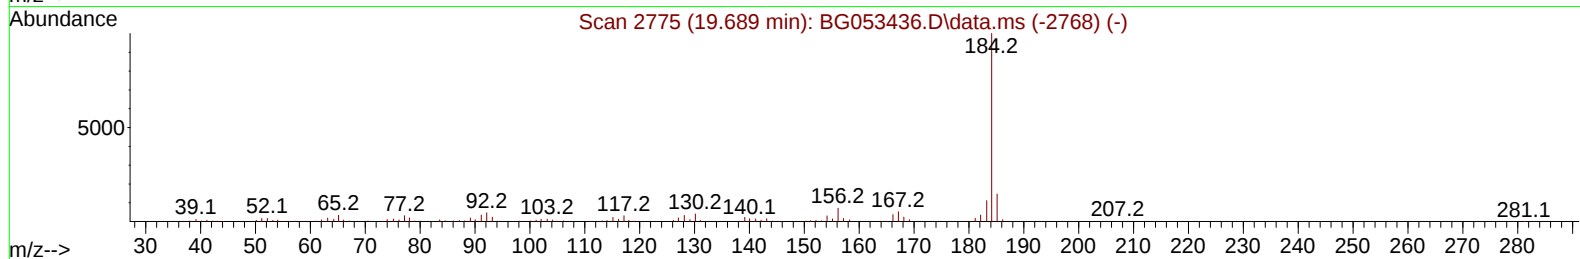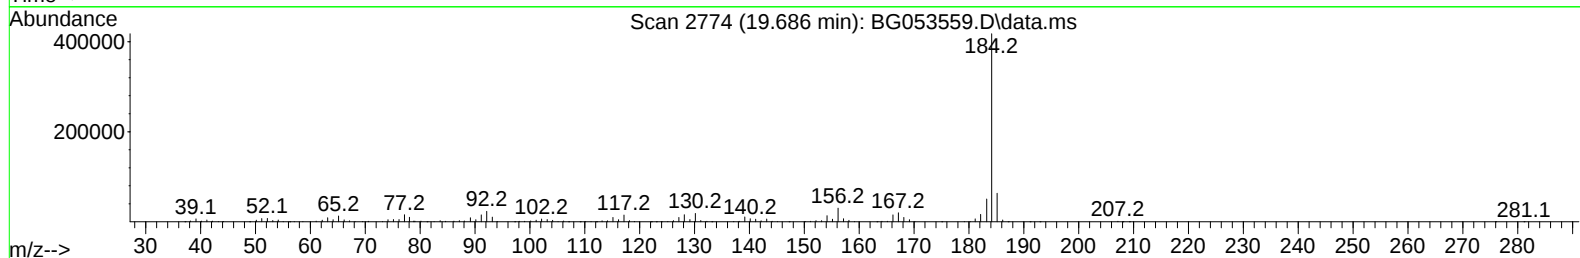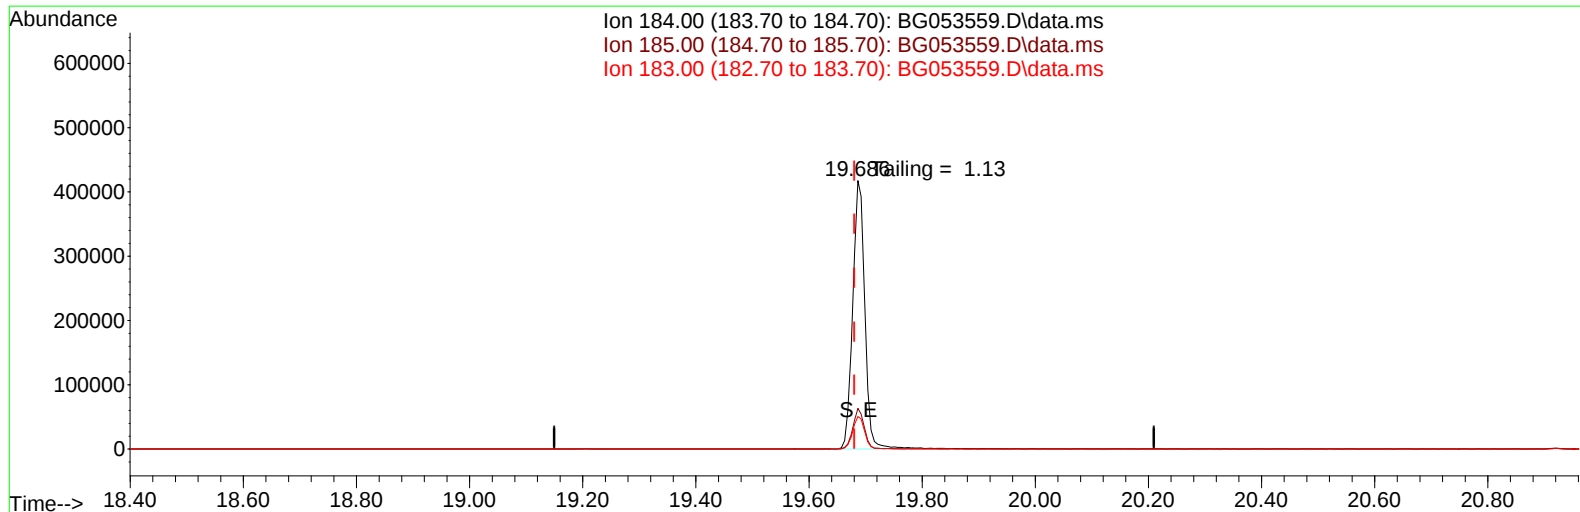

TIC: BG053559.D\data.ms

(77) Benzidine

19.686min (+ 0.007) 489535.77 ng

response 622527

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.18
183.00	11.10	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/16/2022	BNA_G	<u>BG053559.D</u>
Compound Name	Response	Retention Time
DDT	319826	20.92
DDD	10498	20.479
DDE	1001	19.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11499	331325	3.47

Instrument :
BNA_G
ClientSampleId :
DFTPP