
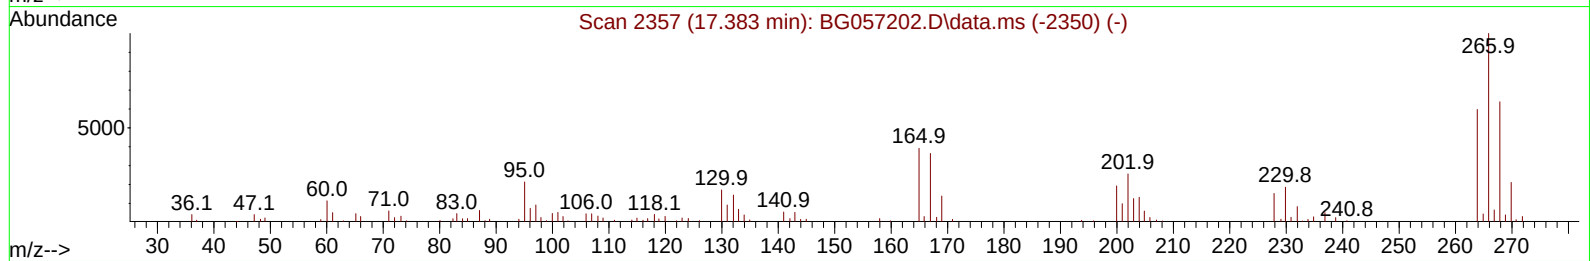
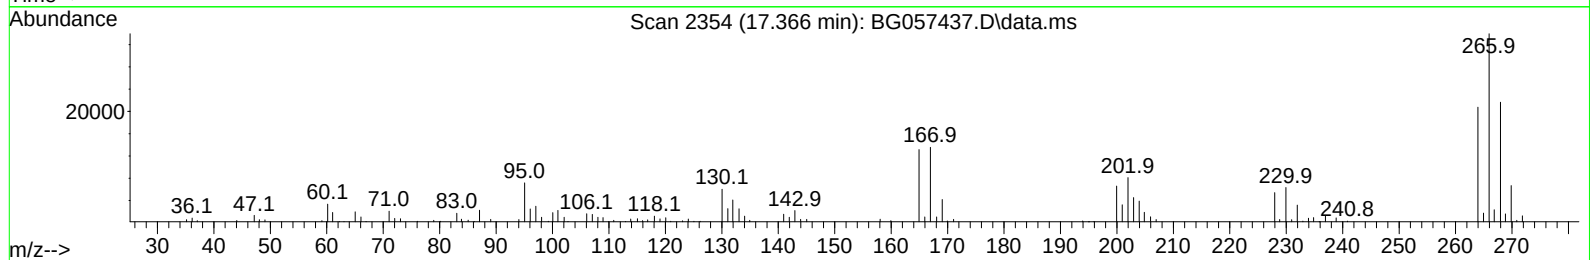


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051623\
Data File : BG057437.D
Acq On : 16 May 2023 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 12:58:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

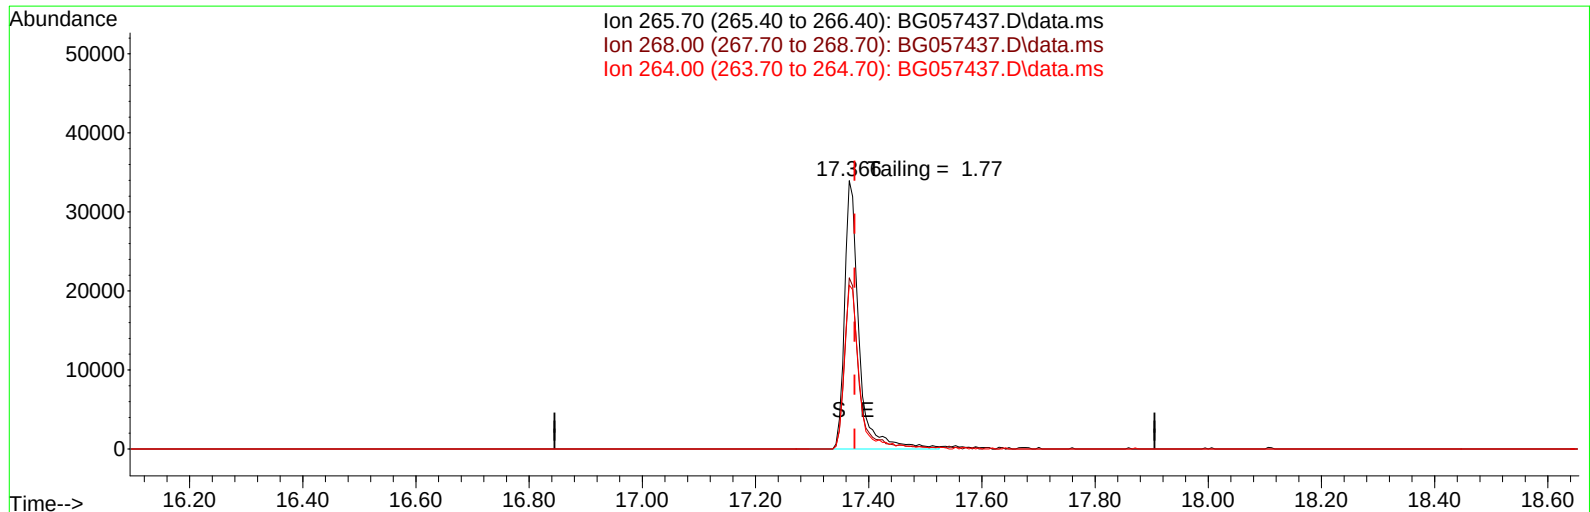

TIC: BG057437.D\data.ms

(70) Pentachlorophenol (C)




17.366min (-0.009) 35669.73 ng

response 60235

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.77
264.00	59.70	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051623\
Data File : BG057437.D
Acq On : 16 May 2023 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 12:58:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

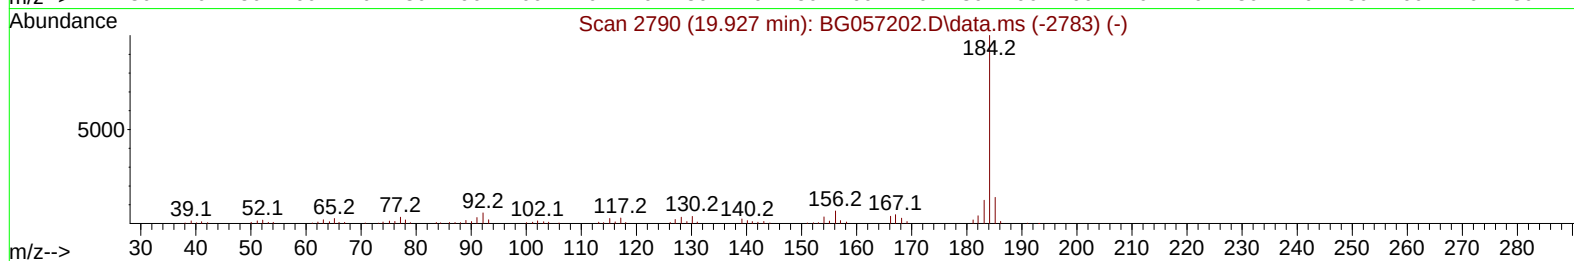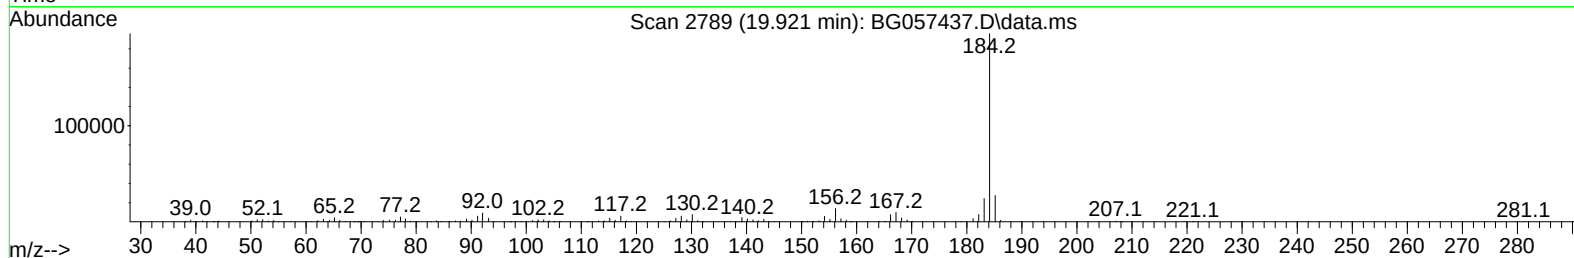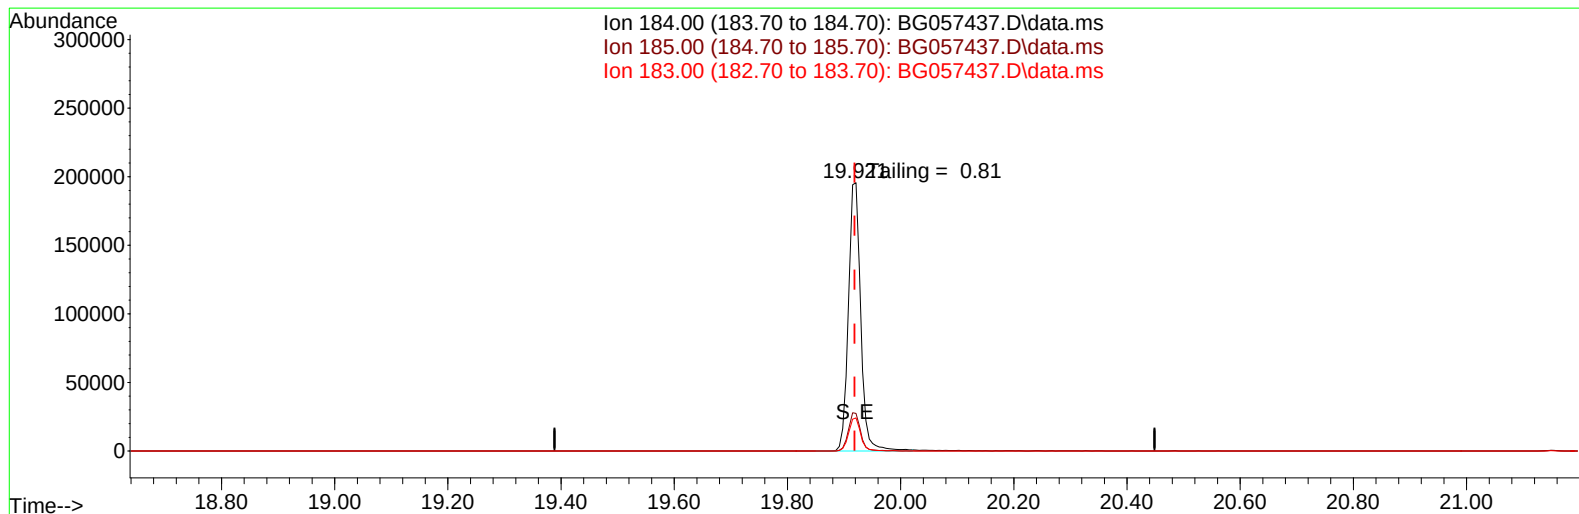

TIC: BG057437.D\data.ms

(77) Benzidine

19.921min (+ 0.003) 50191.30 ng

response 296234

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.04
183.00	12.40	12.39
0.00	0.00	0.00