
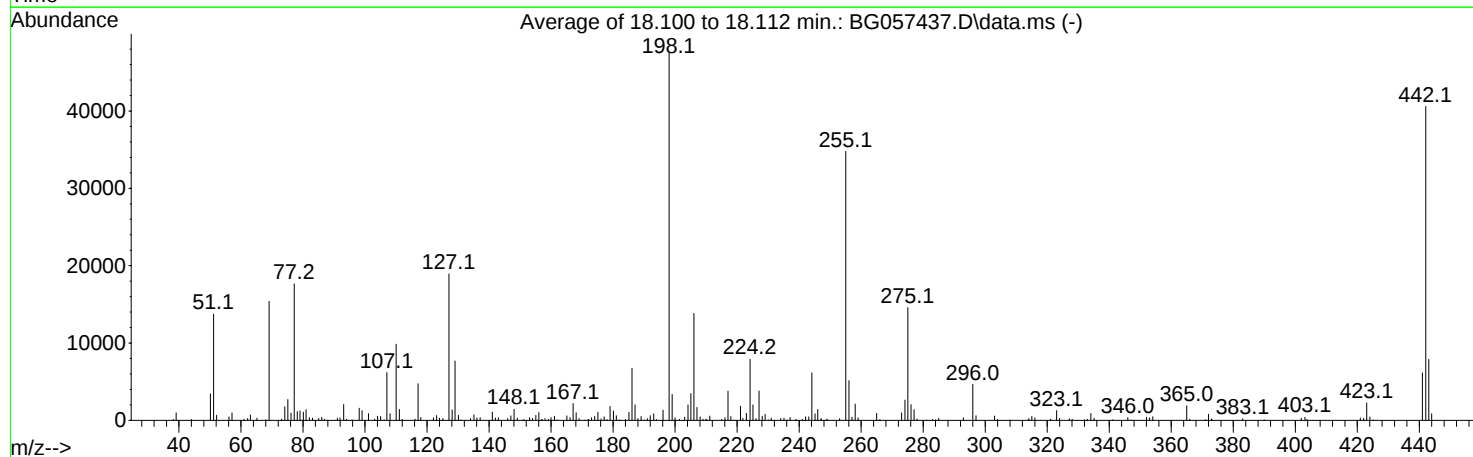


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051623\
 Data File : BG057437.D
 Acq On : 16 May 2023 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 12 22:04:03 2023

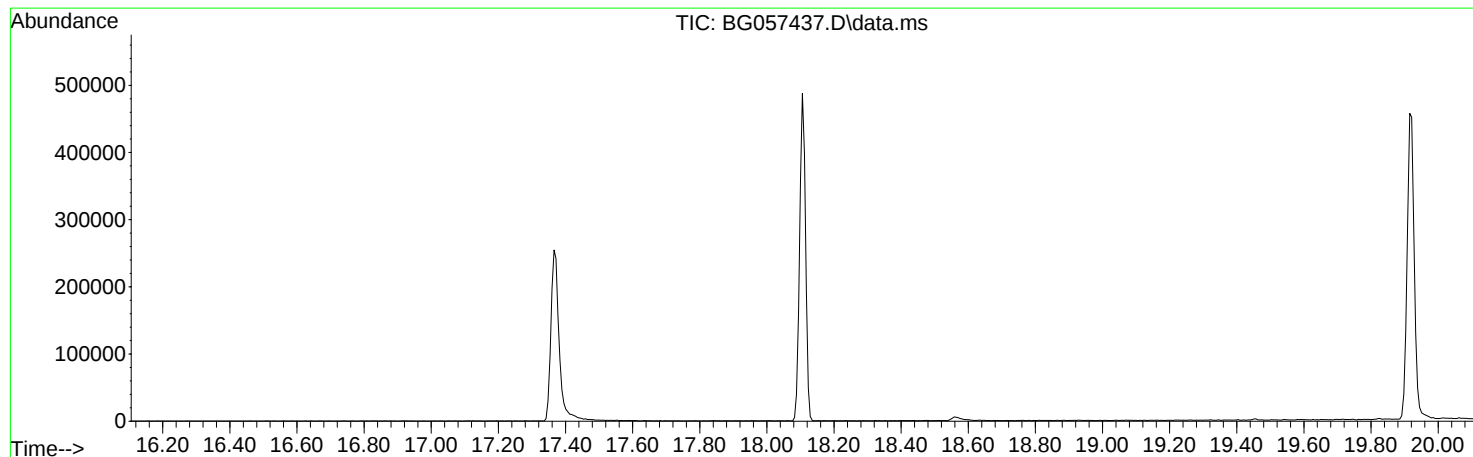




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	13732	PASS
68	69	0.00	2	0.5	77	PASS
69	198	0.00	100	32.4	15401	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.8	18925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47563	PASS
199	198	5	9	7.1	3360	PASS
275	198	10	60	30.7	14585	PASS
365	198	1	100	3.9	1877	PASS
441	198	0.01	100	12.9	6141	PASS
442	442	50	100	100.0	40589	PASS
443	442	15	24	19.4	7885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051623\
Data File : BG057437.D
Acq On : 16 May 2023 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 16 12:58:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

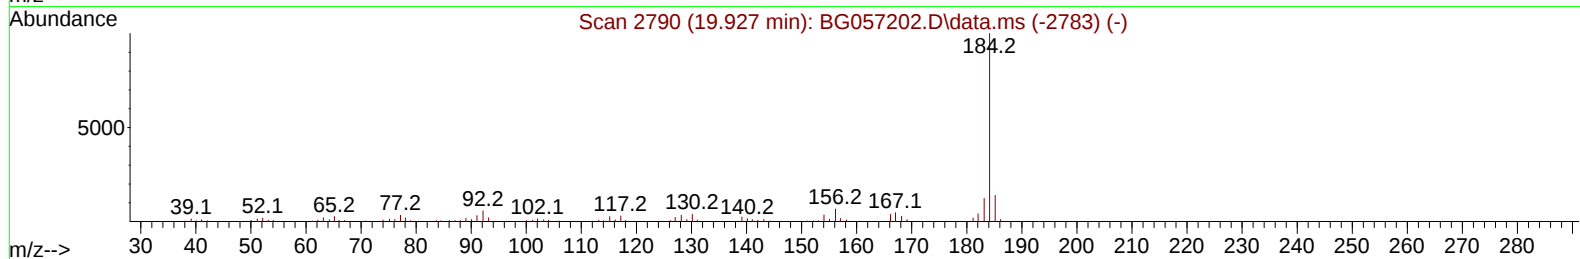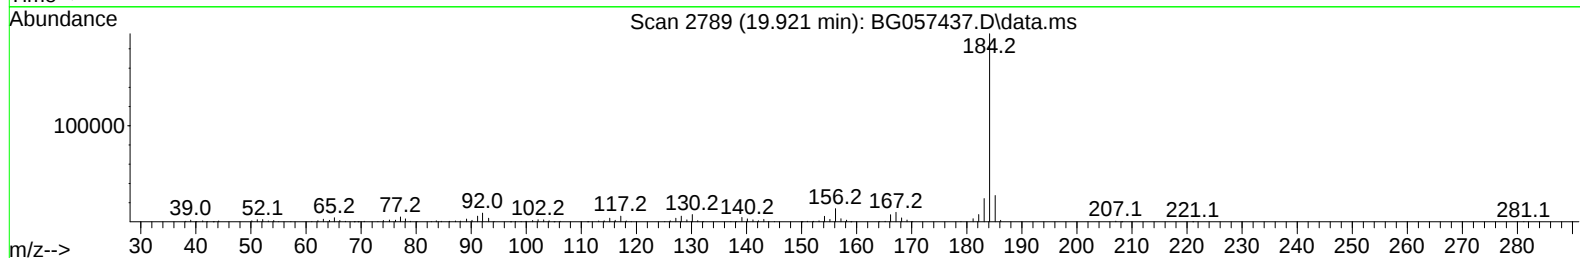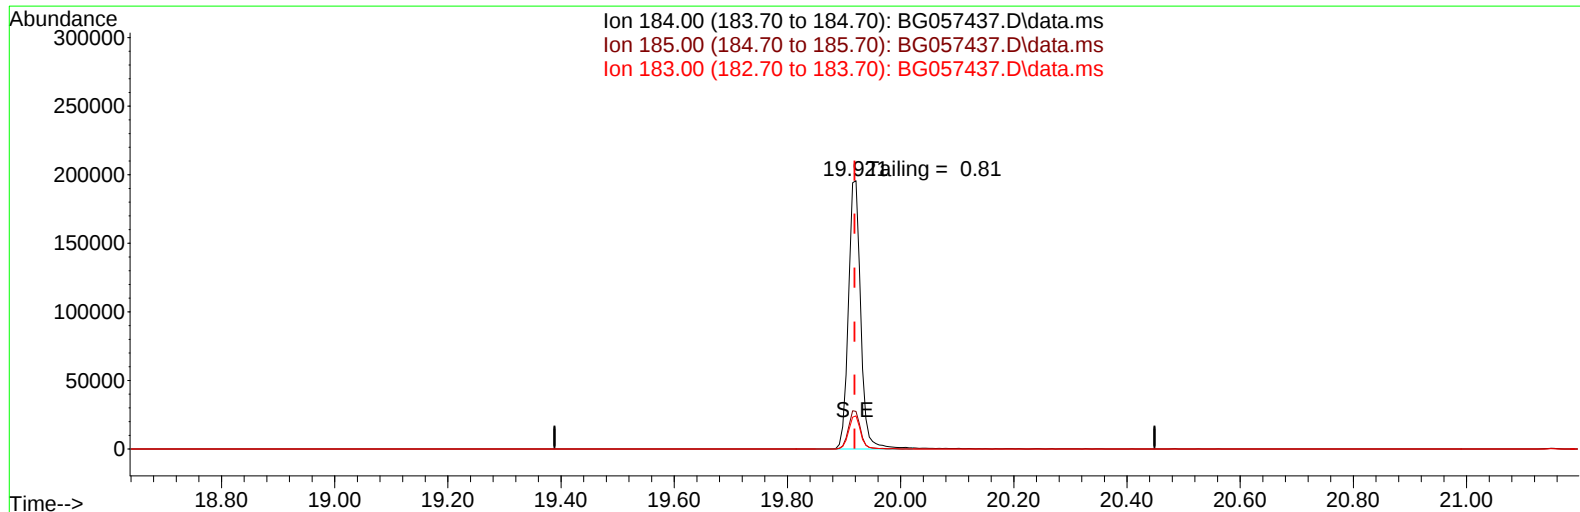

TIC: BG057437.D\data.ms

(77) Benzidine

19.921min (+ 0.003) 50191.30 ng

response 296234

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.04
183.00	12.40	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/16/2023	BNA_G	<u>BG057437.D</u>
Compound Name	Response	Retention Time
DDT	158580	21.149
DDD	2978	20.749
DDE	54	20.197
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3032	161612	1.88

Instrument :
BNA_G
ClientSampleId :
DFTPP