
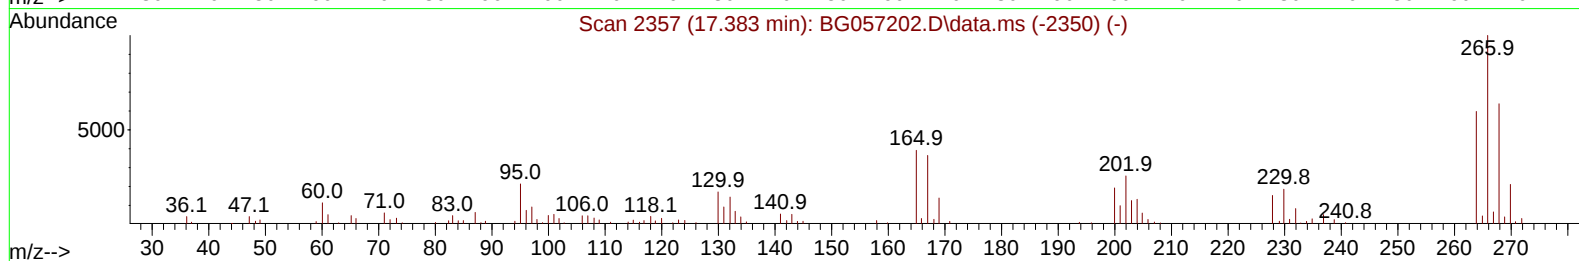
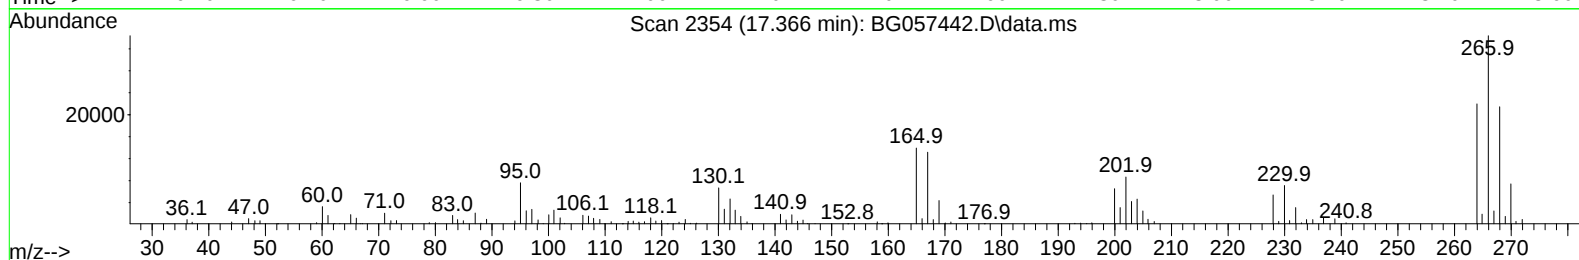


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051723\
Data File : BG057442.D
Acq On : 17 May 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 12:05:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

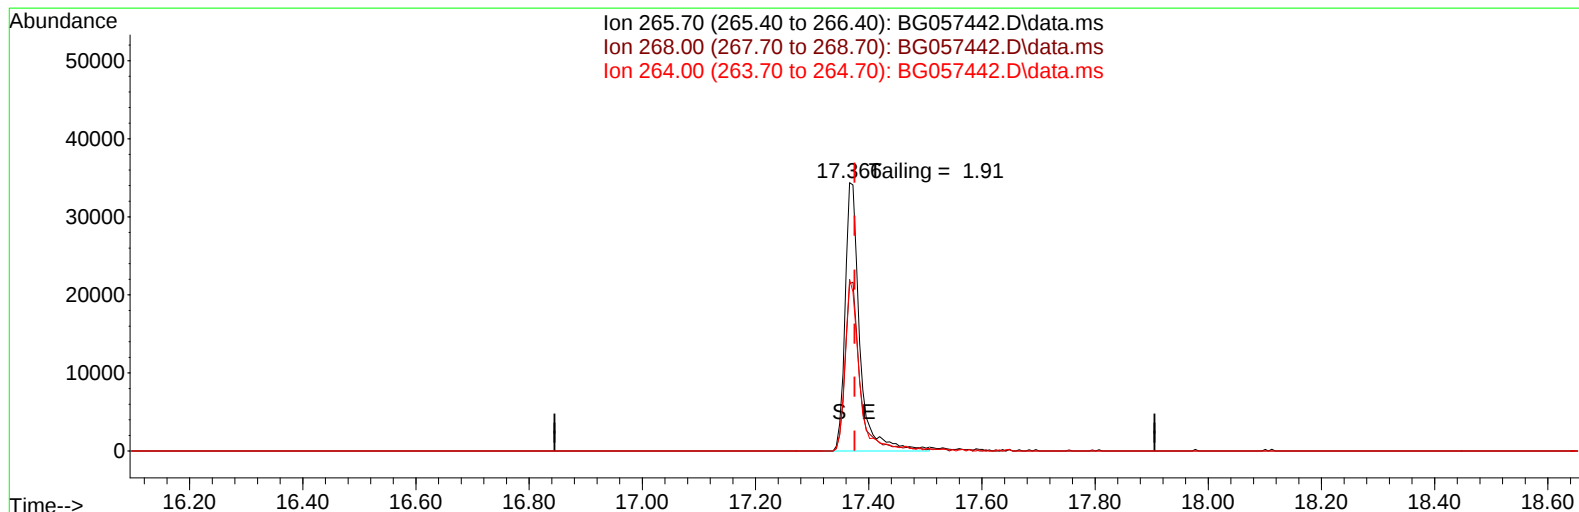

TIC: BG057442.D\data.ms

(70) Pentachlorophenol (C)




17.366min (-0.008) 36671.86 ng m

response 62178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.38
264.00	59.70	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051723\
Data File : BG057442.D
Acq On : 17 May 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 12:05:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

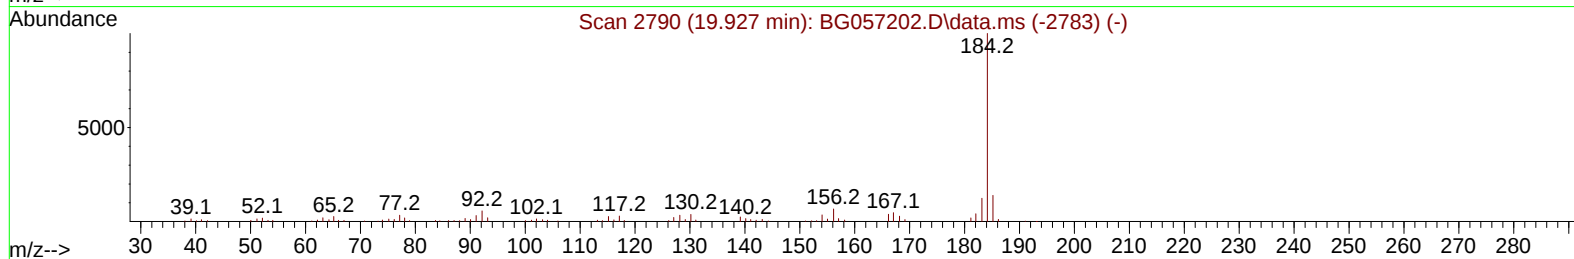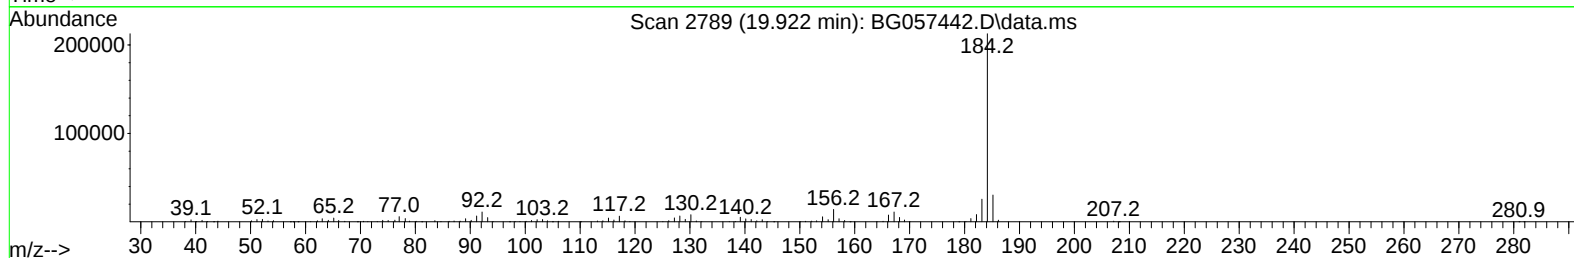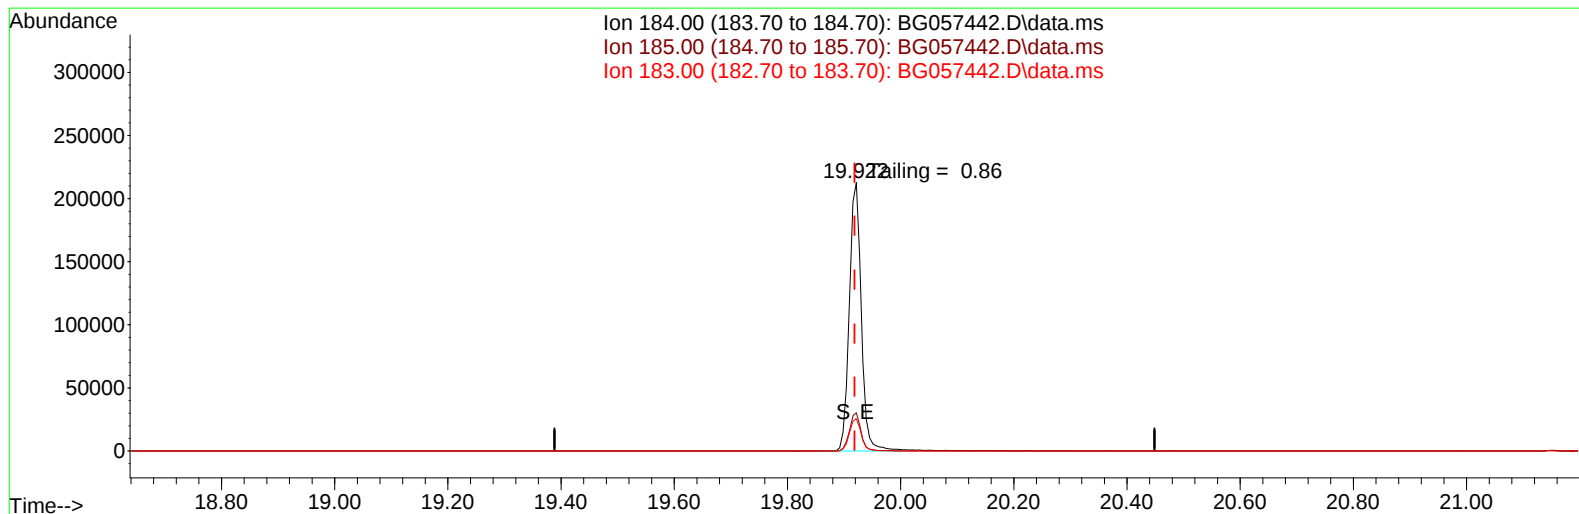

TIC: BG057442.D\data.ms

(77) Benzidine**19.922min (+ 0.003) 59355.19 ng****response 314492**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.28
183.00	12.40	12.07
0.00	0.00	0.00