
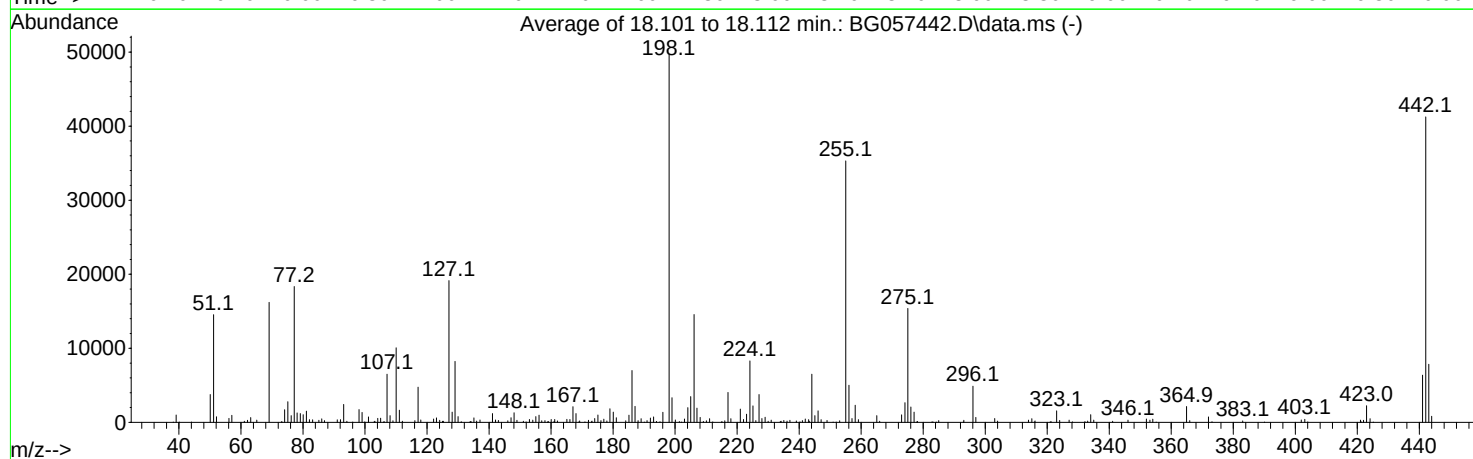


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051723\
Data File : BG057442.D
Acq On : 17 May 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 12 22:04:03 2023

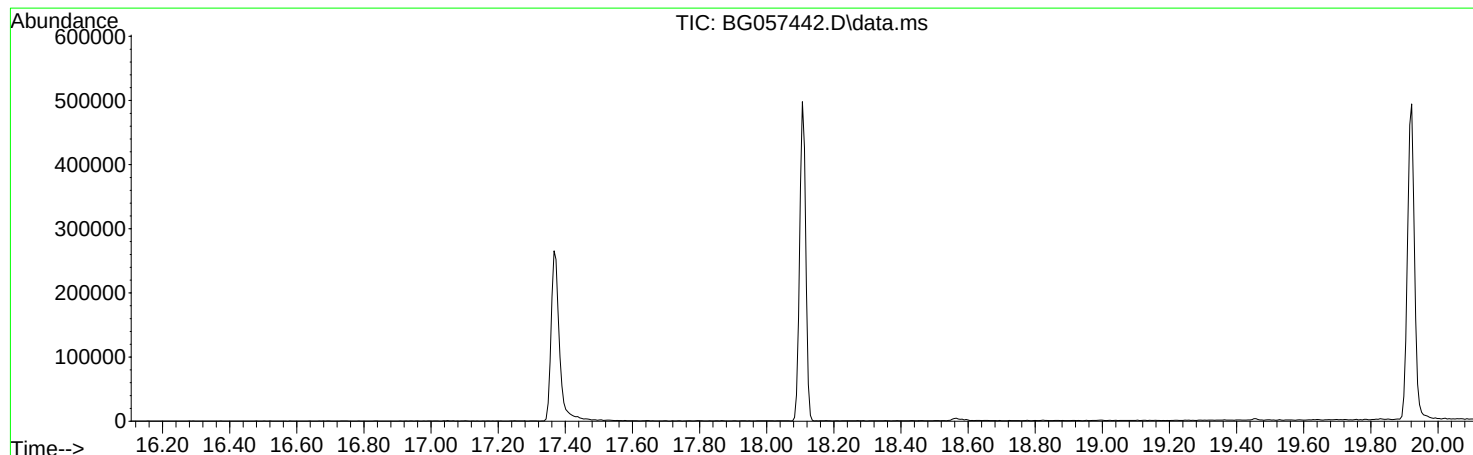

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	14537	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	16199	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.5	19149	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49677	PASS
199	198	5	9	6.7	3323	PASS
275	198	10	60	31.0	15379	PASS
365	198	1	100	4.3	2133	PASS
441	198	0.01	100	12.8	6369	PASS
442	442	50	100	100.0	41253	PASS
443	442	15	24	19.0	7853	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/17/2023	BNA_G	<u>BG057442.D</u>
Compound Name	Response	Retention Time
DDT	166932	21.155
DDD	2683	20.75
DDE	177	20.198
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2860	169792	1.68

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051723\
Data File : BG057442.D
Acq On : 17 May 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 17 12:05:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

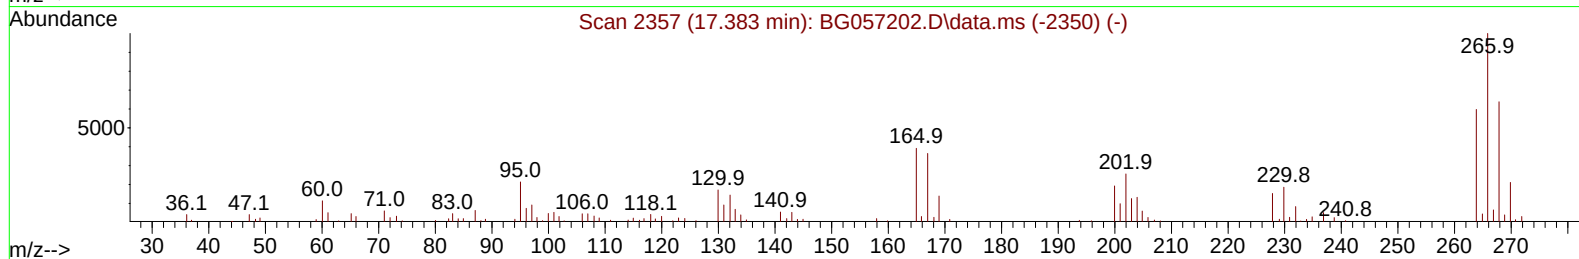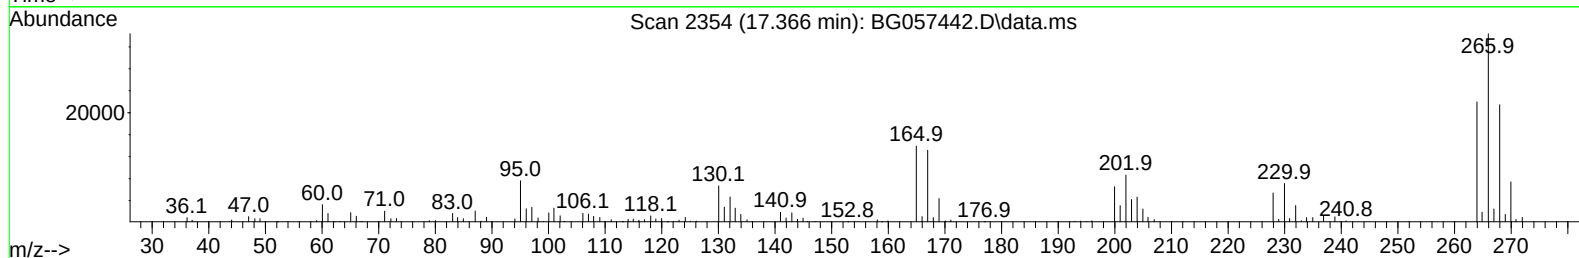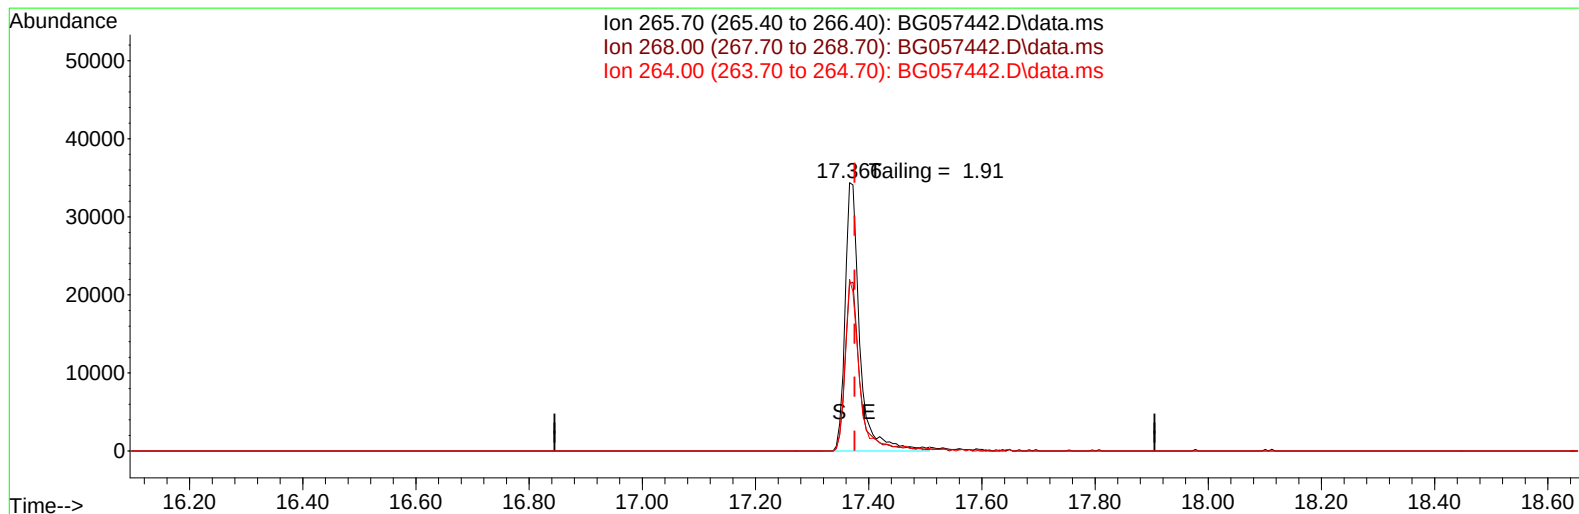

TIC: BG057442.D\data.ms

(70) Pentachlorophenol (C)

17.366min (-0.008) 36671.86 ng m




response 62178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.38
264.00	59.70	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051723\
Data File : BG057442.D
Acq On : 17 May 2023 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 17 12:05:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

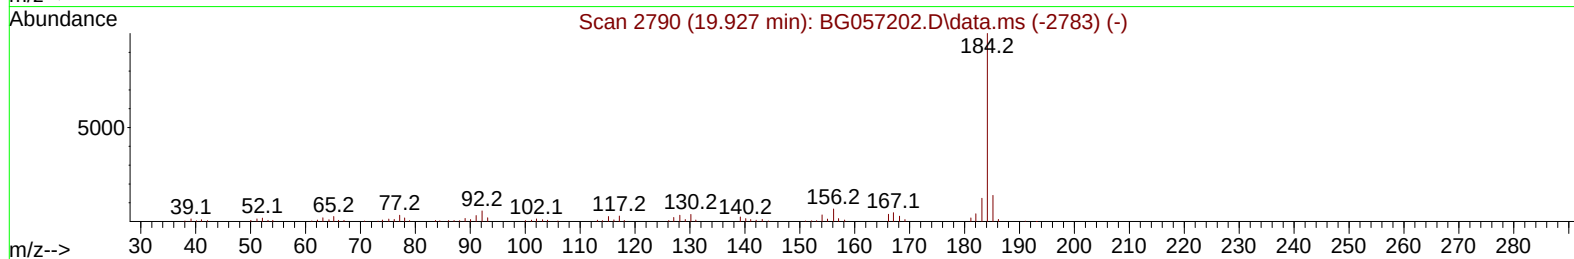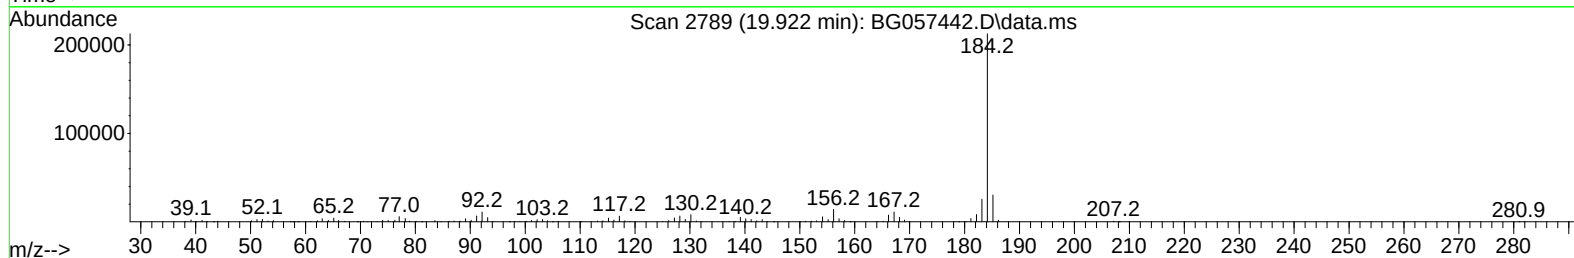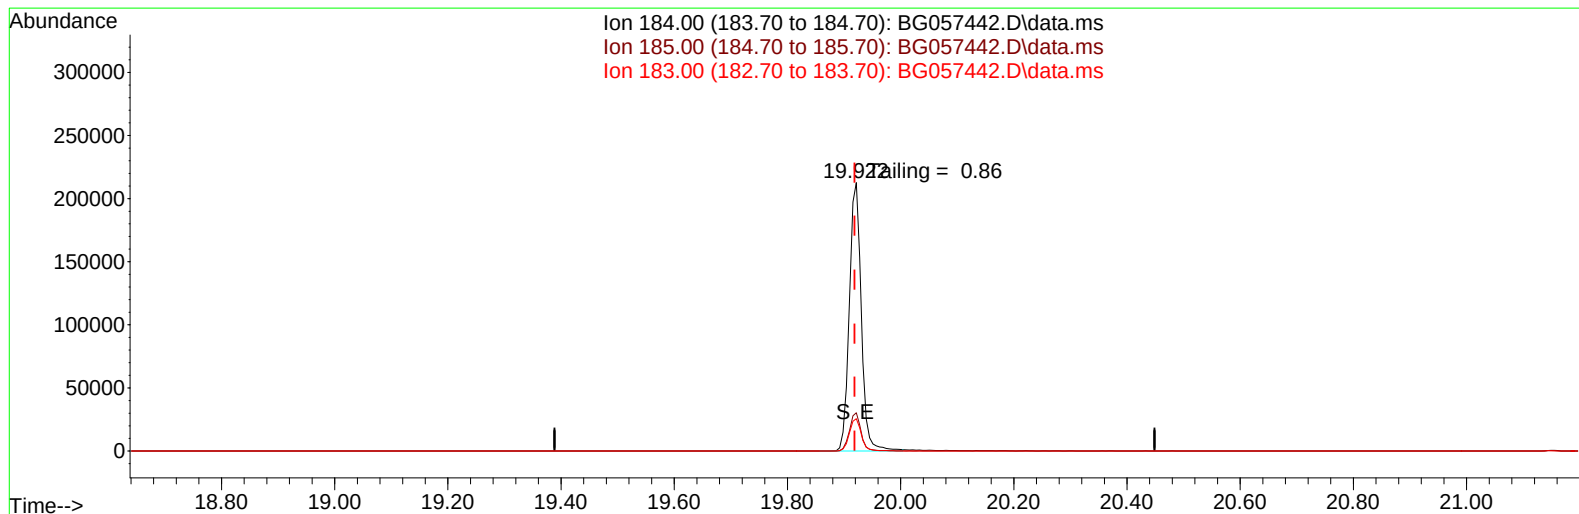

TIC: BG057442.D\data.ms

(77) Benzidine

19.922min (+ 0.003) 59355.19 ng

response 314492

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.28
183.00	12.40	12.07
0.00	0.00	0.00