

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051816\
 Data File : BG021950.D
 Acq On : 19 May 2016 2:37
 Operator : UM/SJ
 Sample : PB90727BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG051816.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.533	115	118	127	rVB2	7114	11919	1.06%	0.110%
2	4.056	205	207	212	rBV4	711	1193	0.11%	0.011%
3	4.286	243	246	247	rVV2	1131	1296	0.12%	0.012%
4	4.303	247	249	256	rVB5	2189	3475	0.31%	0.032%
5	4.391	260	264	269	rVB4	947	1635	0.15%	0.015%
6	7.311	753	761	773	rBV2	98655	205893	18.28%	1.908%
7	7.476	783	789	803	rBV	90006	179308	15.92%	1.662%
8	7.570	803	805	810	rVB4	1096	1448	0.13%	0.013%
9	7.687	817	825	838	rBV	115071	226485	20.11%	2.099%
10	8.058	886	888	891	rVB3	1264	1221	0.11%	0.011%
11	8.093	891	894	896	rBV2	1245	1234	0.11%	0.011%
12	8.163	899	906	918	rBV	93150	198703	17.64%	1.841%
13	8.375	939	942	946	rVB4	903	1171	0.10%	0.011%
14	8.863	1017	1025	1046	rBV	141197	307539	27.30%	2.850%
15	9.015	1049	1051	1057	rVB4	795	1703	0.15%	0.016%
16	9.327	1092	1104	1120	rBV	103792	231585	20.56%	2.146%
17	10.055	1219	1228	1244	rBV	80096	178693	15.86%	1.656%
18	10.596	1313	1320	1336	rBV	132519	291399	25.87%	2.700%
19	10.978	1377	1385	1395	rBV	180376	367741	32.65%	3.408%
20	11.113	1401	1408	1419	rBV	123982	291777	25.90%	2.704%
21	11.295	1438	1439	1444	rVB3	1333	1383	0.12%	0.013%
22	11.383	1452	1454	1459	rVB3	763	1238	0.11%	0.011%
23	12.558	1651	1654	1656	rBV3	1665	2088	0.19%	0.019%
24	13.657	1837	1841	1847	rVB	2015	3180	0.28%	0.029%
25	14.180	1923	1930	1942	rBV	340743	552125	49.02%	5.116%
26	14.291	1948	1949	1957	rVB2	898	1148	0.10%	0.011%
27	14.479	1972	1981	1993	rBV	403650	725196	64.38%	6.720%
28	14.785	2025	2033	2042	rBV2	300793	547887	48.64%	5.077%
29	14.979	2058	2066	2093	rBV	69142	213530	18.96%	1.979%
30	15.455	2146	2147	2154	rVB3	813	1366	0.12%	0.013%
31	15.772	2194	2201	2212	rBV	535886	916651	81.38%	8.494%
32	15.890	2214	2221	2232	rVB	112819	192763	17.11%	1.786%
33	16.013	2237	2242	2249	rVB3	5266	9252	0.82%	0.086%
34	16.724	2361	2363	2368	rVB2	947	1362	0.12%	0.013%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051816\
 Data File : BG021950.D
 Acq On : 19 May 2016 2:37
 Operator : UM/SJ
 Sample : PB90727BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG051816.M
 Title : SVOA CALIBRATION

35	17.311	2459	2463	2468	rVB2	825	1494	0.13%	0.014%
36	17.529	2492	2500	2509	rBV	368348	649426	57.65%	6.018%
37	17.623	2509	2516	2536	rVB	575806	1004013	89.13%	9.304%
38	18.316	2631	2634	2637	rBV3	994	1134	0.10%	0.011%
39	18.669	2688	2694	2696	rVB2	596	1225	0.11%	0.011%
40	19.432	2821	2824	2829	rBV5	1190	1850	0.16%	0.017%
41	19.474	2829	2831	2835	rBV2	1016	1348	0.12%	0.012%
42	19.538	2835	2842	2847	rBV2	5649	9271	0.82%	0.086%
43	19.626	2855	2857	2862	rVB4	1200	1406	0.12%	0.013%
44	19.797	2881	2886	2890	rBV3	5865	9306	0.83%	0.086%
45	19.903	2896	2904	2917	rBV	702939	1126412	100.00%	10.438%
46	20.179	2948	2951	2952	rBV3	1541	1822	0.16%	0.017%
47	20.396	2986	2988	2990	rBV2	2590	2839	0.25%	0.026%
48	20.537	3010	3012	3014	rBV3	2072	1555	0.14%	0.014%
49	20.578	3017	3019	3022	rBV4	1650	1530	0.14%	0.014%
50	20.613	3023	3025	3026	rVB2	2102	1248	0.11%	0.012%
51	20.631	3026	3028	3029	rBV2	2531	2044	0.18%	0.019%
52	20.666	3032	3034	3035	rBV2	2194	1240	0.11%	0.011%
53	20.725	3042	3044	3046	rBV3	1657	1606	0.14%	0.015%
54	20.837	3060	3063	3068	rVB7	4903	5792	0.51%	0.054%
55	20.937	3079	3080	3084	rBV4	2030	1507	0.13%	0.014%
56	20.966	3084	3085	3086	rVV	2400	1156	0.10%	0.011%
57	20.984	3086	3088	3090	rVB3	2879	2136	0.19%	0.020%
58	21.036	3095	3097	3098	rBV2	2109	1386	0.12%	0.013%
59	21.172	3118	3120	3123	rBV4	1851	1535	0.14%	0.014%
60	21.266	3134	3136	3137	rBV2	2306	1335	0.12%	0.012%
61	21.806	3221	3228	3240	rBV	328231	659287	58.53%	6.109%
62	22.082	3272	3275	3279	rBV6	2617	3970	0.35%	0.037%
63	22.400	3327	3329	3330	rBV2	2317	1292	0.11%	0.012%
64	23.481	3511	3513	3514	rBV2	2567	1384	0.12%	0.013%
65	24.145	3622	3626	3627	rBV4	3653	4419	0.39%	0.041%
66	24.908	3741	3756	3769	rBV3	284397	933255	82.85%	8.648%
67	25.132	3782	3794	3807	rBV	200849	635976	56.46%	5.893%
68	25.478	3851	3853	3854	rBV2	2746	1593	0.14%	0.015%
69	25.772	3902	3903	3905	rBV2	3151	2476	0.22%	0.023%
70	25.895	3922	3924	3925	rBV2	3667	2707	0.24%	0.025%
71	26.442	4015	4017	4019	rBV3	2632	2180	0.19%	0.020%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051816\
Data File : BG021950.D
Acq On : 19 May 2016 2:37
Operator : UM/SJ
Sample : PB90727BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK27

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG051816.M
Title : SVOA CALIBRATION

72	26.495	4025	4026	4028	rVB2	2619	1560	0.14%	0.014%
73	26.642	4049	4051	4053	rBV2	2263	1619	0.14%	0.015%
74	27.188	4142	4144	4145	rBV2	2683	1242	0.11%	0.012%
75	27.517	4198	4200	4201	rBV2	2286	1619	0.14%	0.015%
76	27.646	4220	4222	4224	rBV3	2335	2298	0.20%	0.021%
77	27.670	4224	4226	4227	rBV2	2823	2715	0.24%	0.025%
78	27.688	4227	4229	4230	rBV2	3559	2595	0.23%	0.024%
79	28.087	4295	4297	4298	rVB2	2748	1398	0.12%	0.013%
80	28.604	4384	4385	4389	rBV4	3211	2879	0.26%	0.027%
81	29.021	4454	4456	4459	rBV3	2275	2008	0.18%	0.019%
82	29.092	4466	4468	4470	rBV3	2218	2239	0.20%	0.021%
83	29.685	4567	4569	4571	rVB3	2305	1275	0.11%	0.012%
84	30.331	4677	4679	4680	rBV	2190	1310	0.12%	0.012%
85	30.461	4700	4701	4702	rBV	3196	1275	0.11%	0.012%
86	30.907	4776	4777	4779	rBV2	2590	2089	0.19%	0.019%
87	31.401	4859	4861	4862	rBV2	2691	1896	0.17%	0.018%
88	31.418	4862	4864	4865	rBV2	2386	1730	0.15%	0.016%
89	32.382	5026	5028	5030	rBV3	2297	1155	0.10%	0.011%


Sum of corrected areas: 10791644

Data Path : Z:\HPCHEM1\BNA G\DATA\BG051816\
Data File : BG021950.D
Acq On : 19 May 2016 2:37
Operator : UM/SJ
Sample : PB90727BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK27

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG051816.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

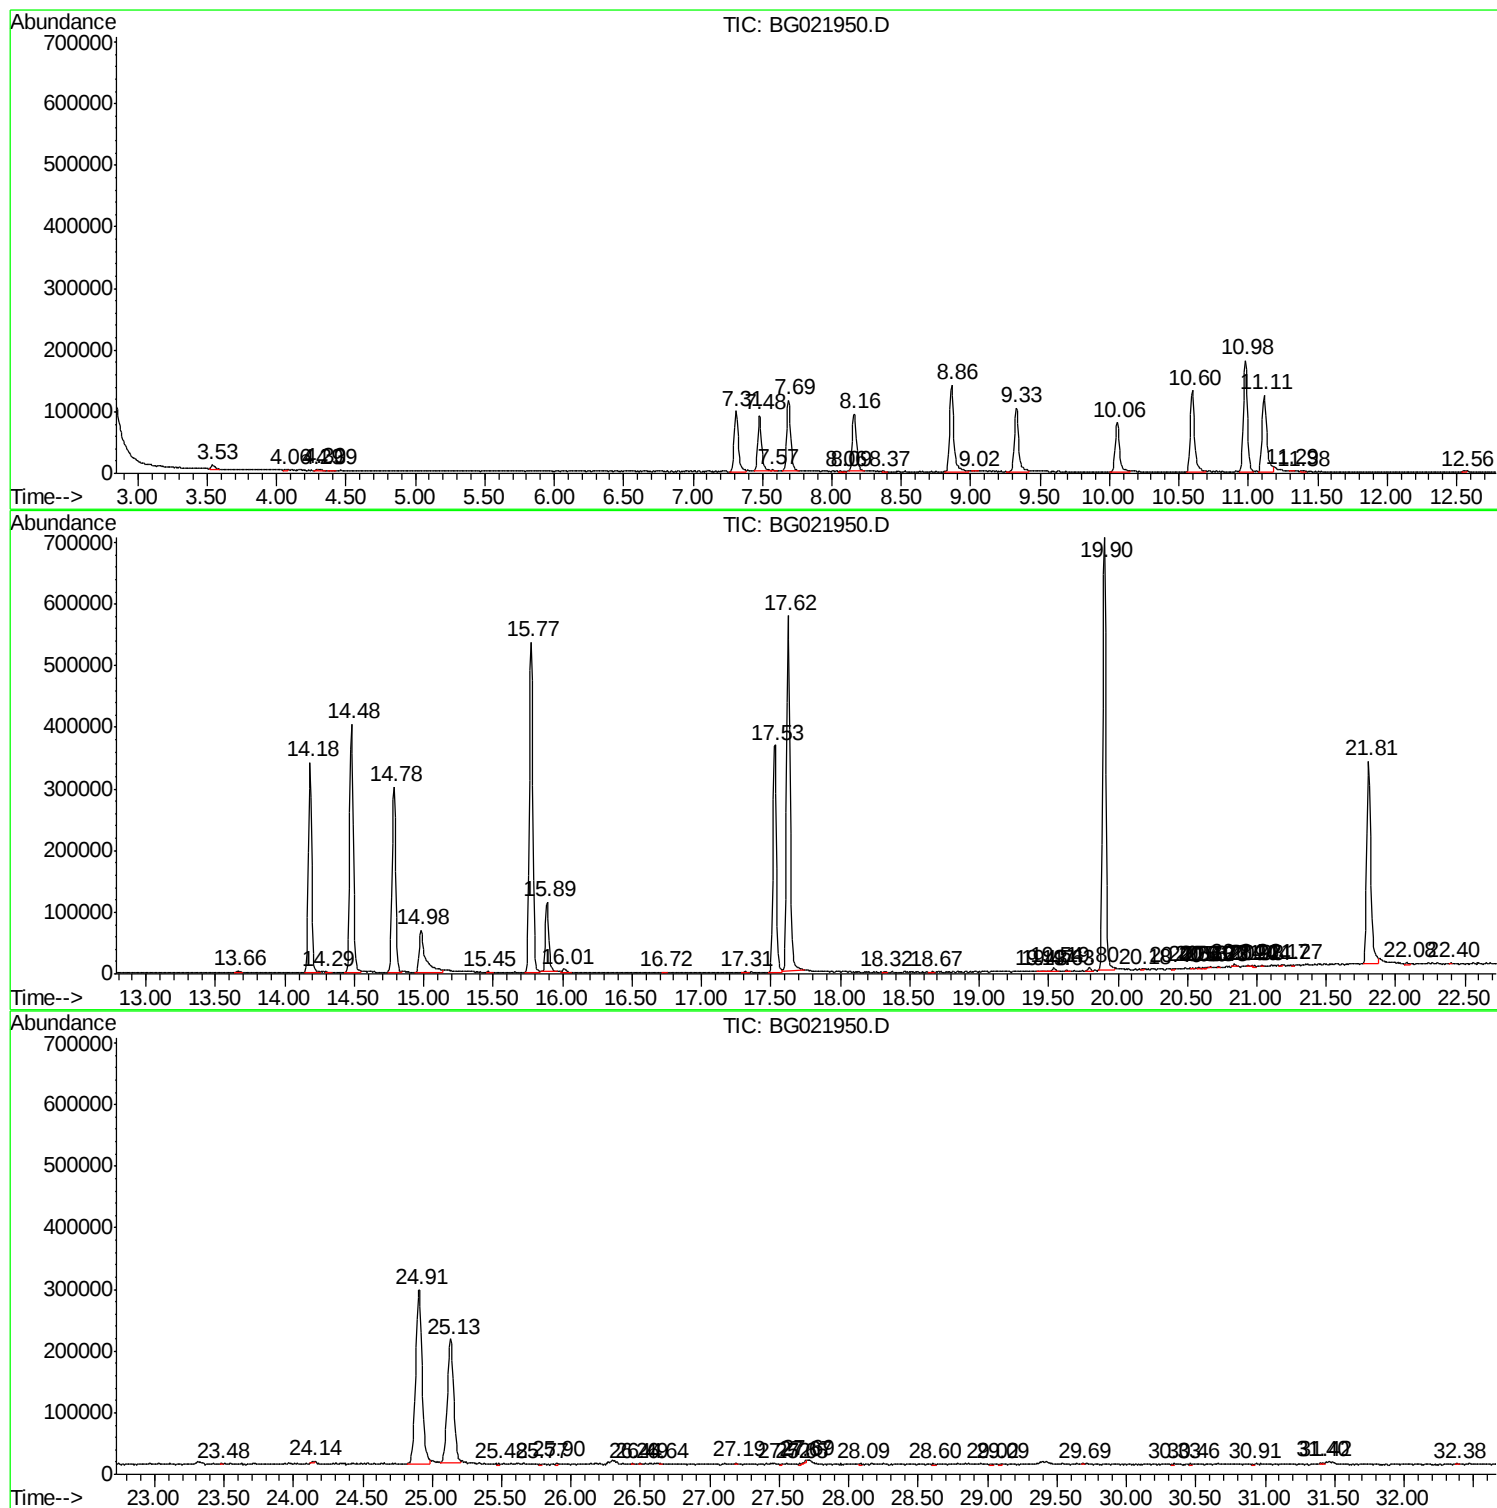

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051816\
Data File : BG021950.D
Acq On : 19 May 2016 2:37
Operator : UM/SJ
Sample : PB90727BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK27

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG051816.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051816\
Data File : BG021950.D
Acq On : 19 May 2016 2:37
Operator : UM/SJ
Sample : PB90727BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK27

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG051816.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc