
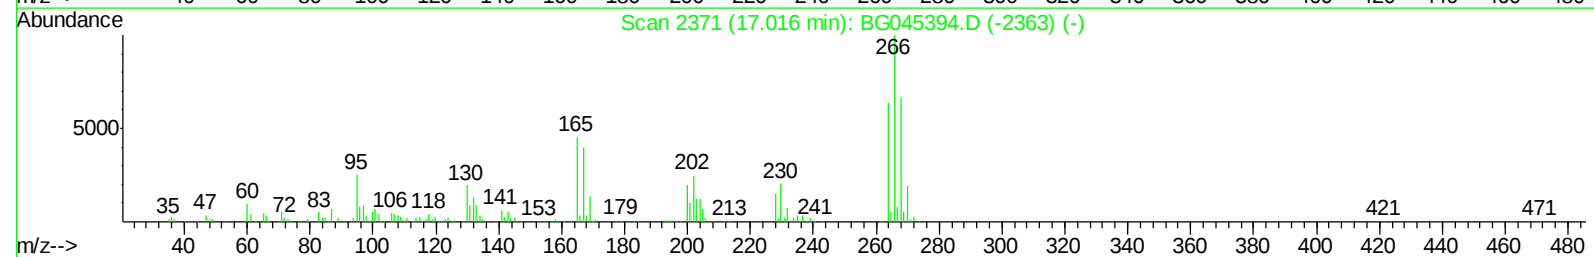
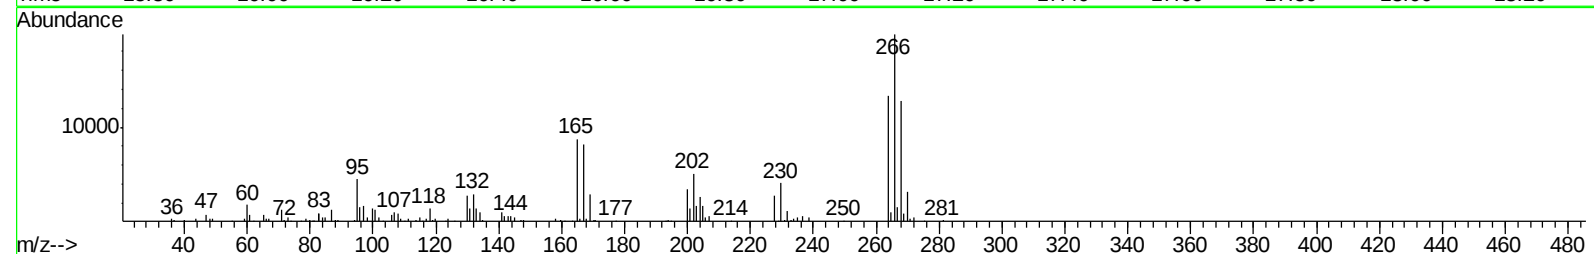


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG051820\
 Data File : BG045412.D
 Acq On : 18 May 2020 13:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 06:35:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 18 15:47:17 2020
 Response via : Initial Calibration

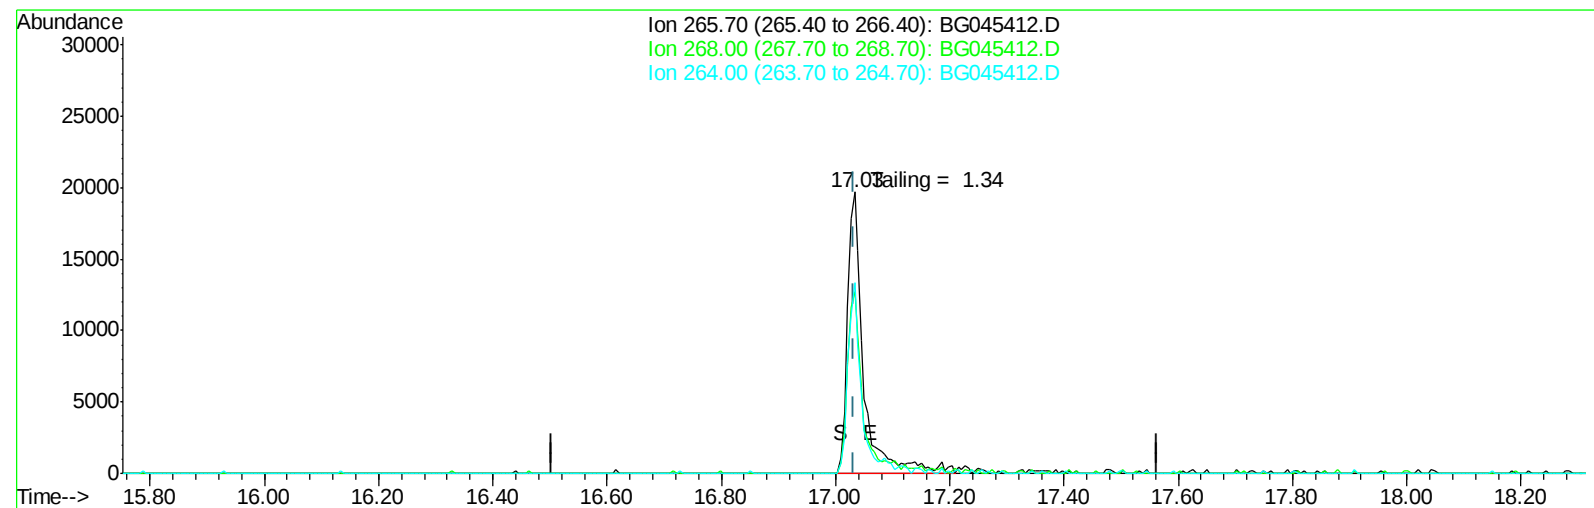

TIC: BG045412.D

(70) Pentachlorophenol (C)




17.033min (-0.001) 17377.25ng

response 35460

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.77
264.00	63.70	67.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG051820\
 Data File : BG045412.D
 Acq On : 18 May 2020 13:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 06:35:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 18 15:47:17 2020
 Response via : Initial Calibration

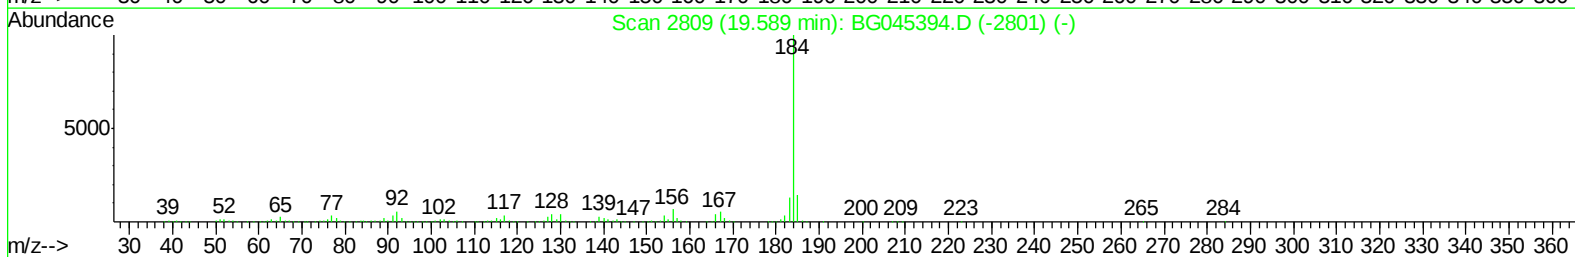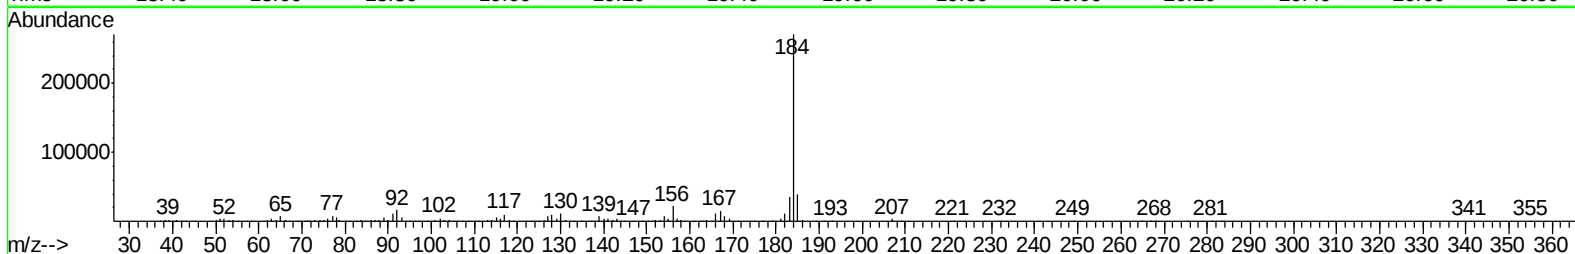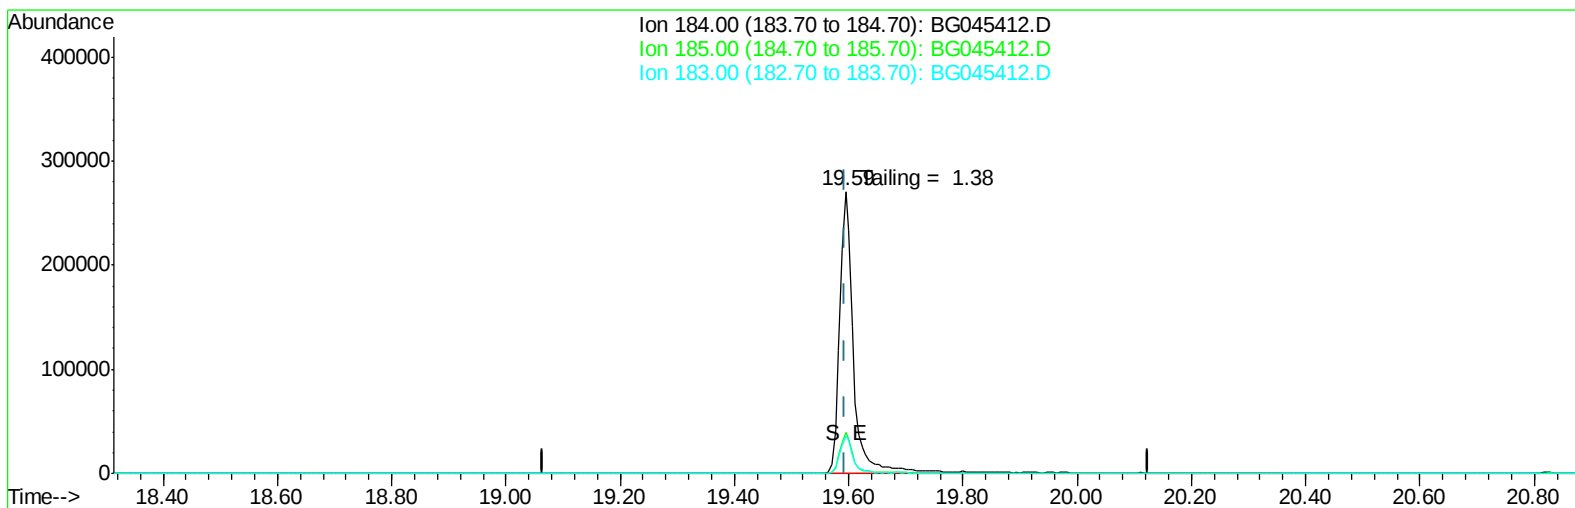

TIC: BG045412.D

(77) Benzidine

19.594min (-0.001) 122345.63ng m

response 477623

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.43
183.00	12.80	13.16
0.00	0.00	0.00