
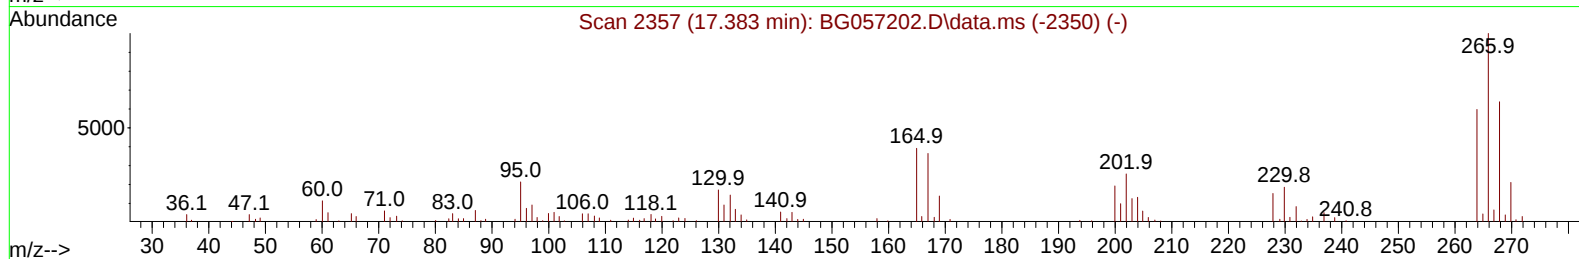
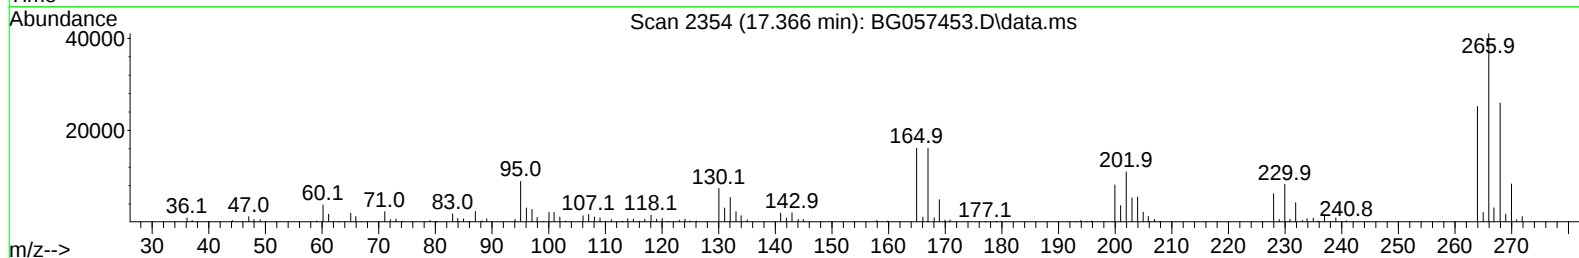


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051823\
Data File : BG057453.D
Acq On : 18 May 2023 9:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 17:10:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 22:04:03 2023
Response via : Initial Calibration

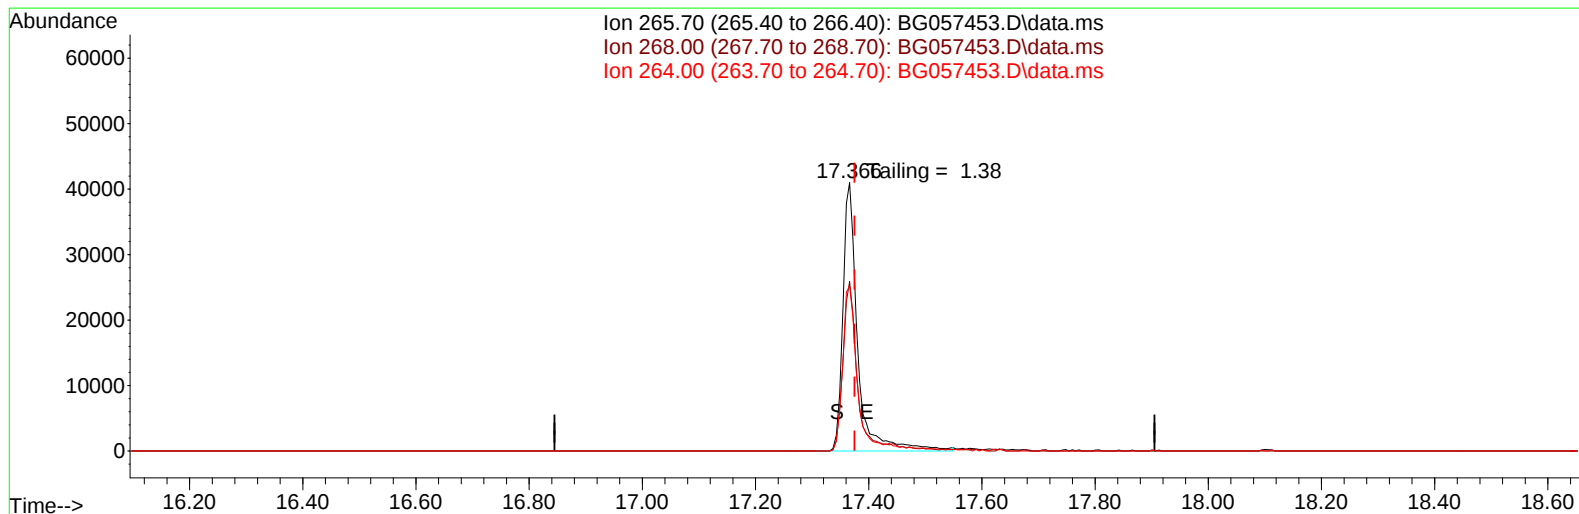

TIC: BG057453.D\data.ms

(70) Pentachlorophenol (C)




17.366min (-0.009) 41136.49 ng

response 74529

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.29
264.00	59.70	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051823\
 Data File : BG057453.D
 Acq On : 18 May 2023 9:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 17:10:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 12 22:04:03 2023
 Response via : Initial Calibration

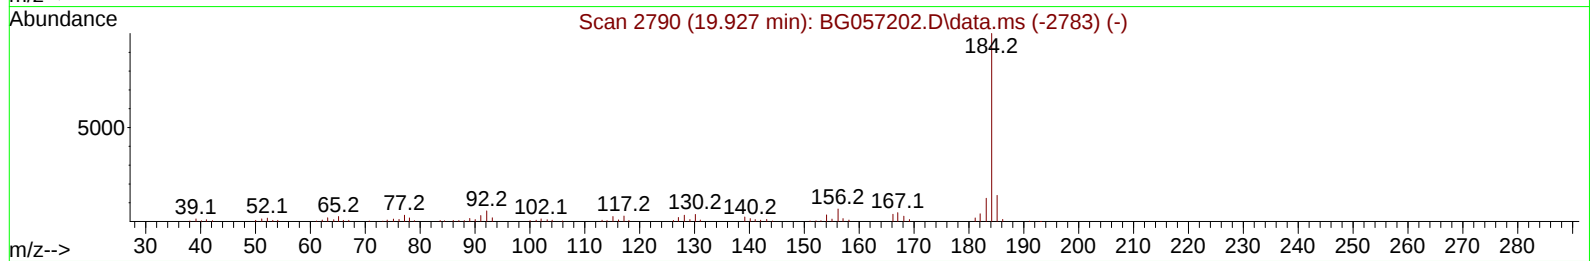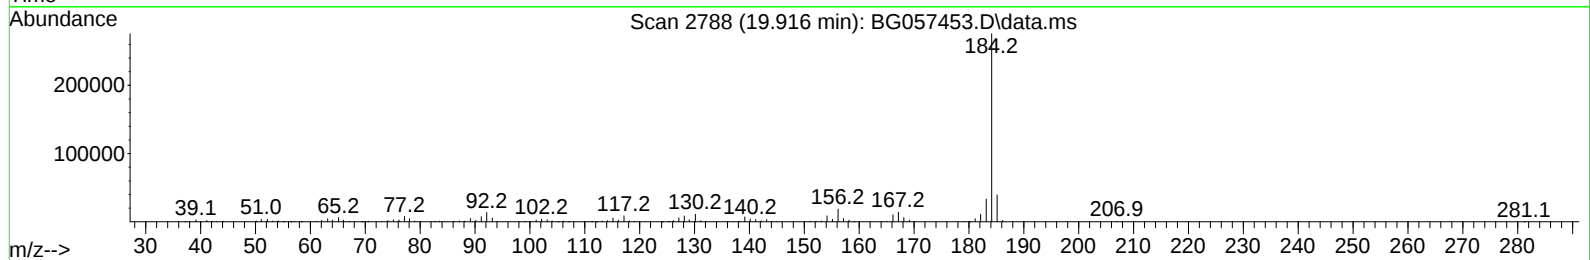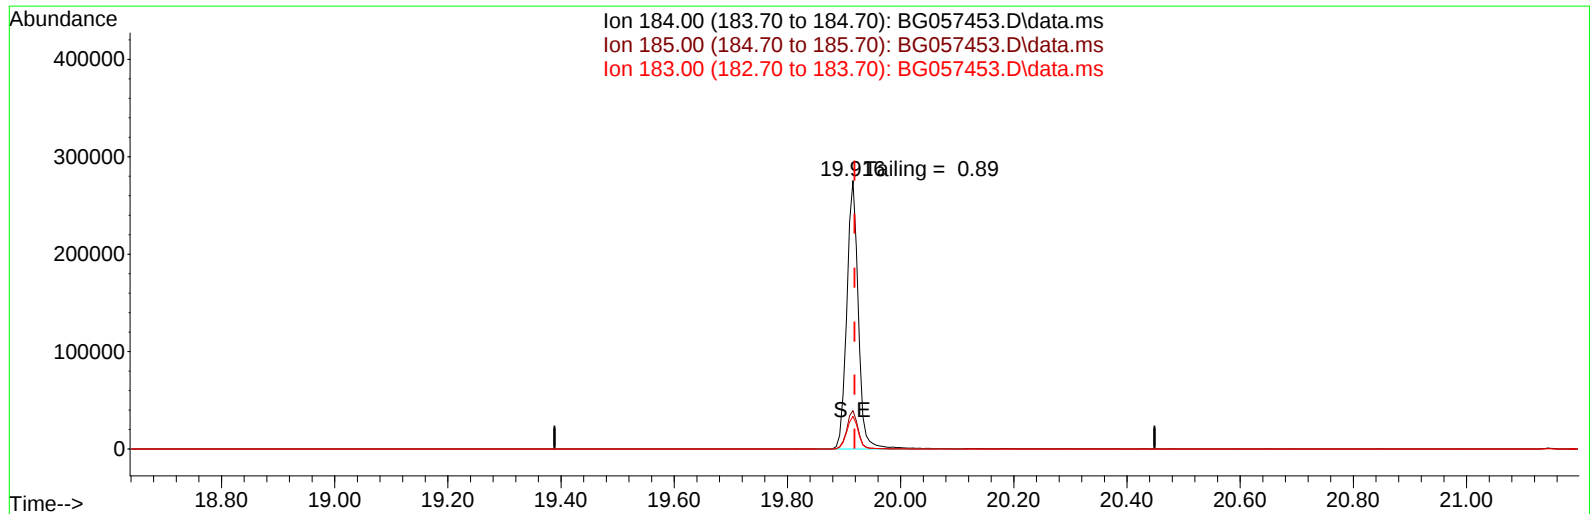

TIC: BG057453.D\data.ms

(77) Benzidine

19.916min (-0.003) 0.00 ng

response 391693

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.32
183.00	12.40	12.15
0.00	0.00	0.00