
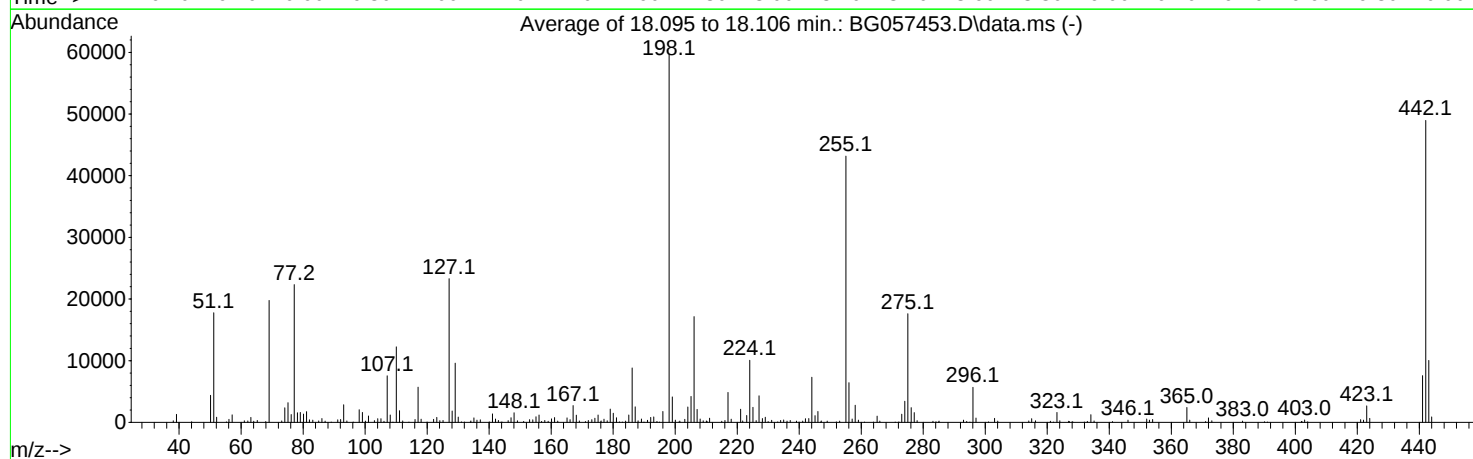


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG051823\  
 Data File : BG057453.D  
 Acq On : 18 May 2023 9:03  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 12 22:04:03 2023

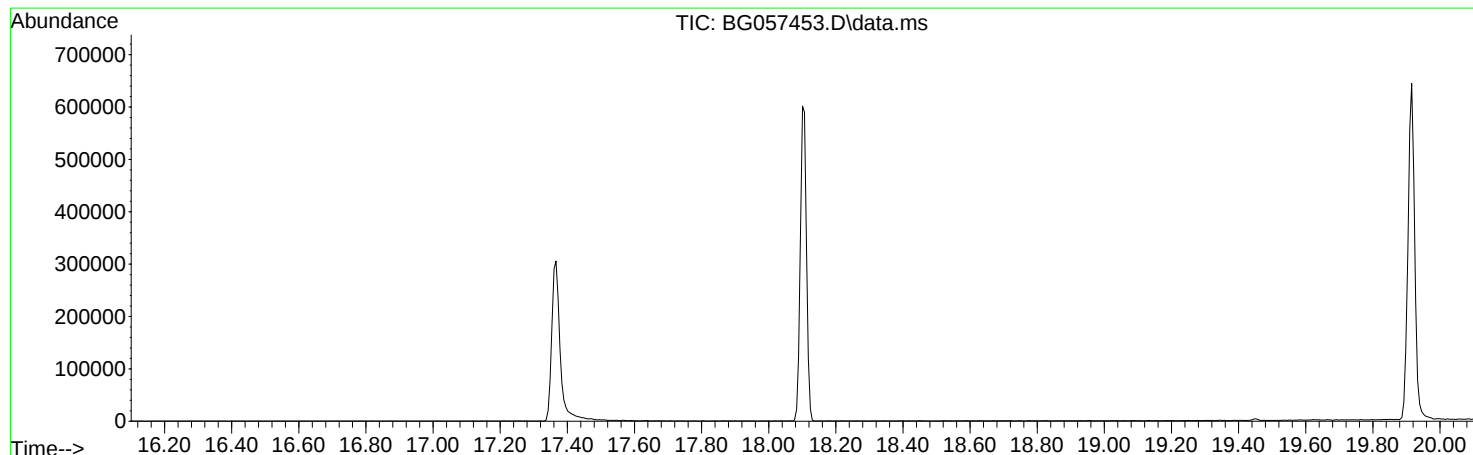

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.8         | 17773      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.6          | 126        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.1         | 19768      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 39.1         | 23304      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 59651      | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 4116       | PASS                |
| 275            | 198             | 10              | 60              | 29.5         | 17618      | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 2402       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.7         | 7582       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 48973      | PASS                |
| 443            | 442             | 15              | 24              | 20.5         | 10042      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/18/2023     | BNA_G            | <u>BG057453.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 205256           | 21.143             |
| DDD           | 3585             | 20.738             |
| DDE           | 174              | 20.192             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3759          | 209015           | 1.80               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG051823\  
Data File : BG057453.D  
Acq On : 18 May 2023 9:03  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: May 18 17:10:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 12 22:04:03 2023  
Response via : Initial Calibration

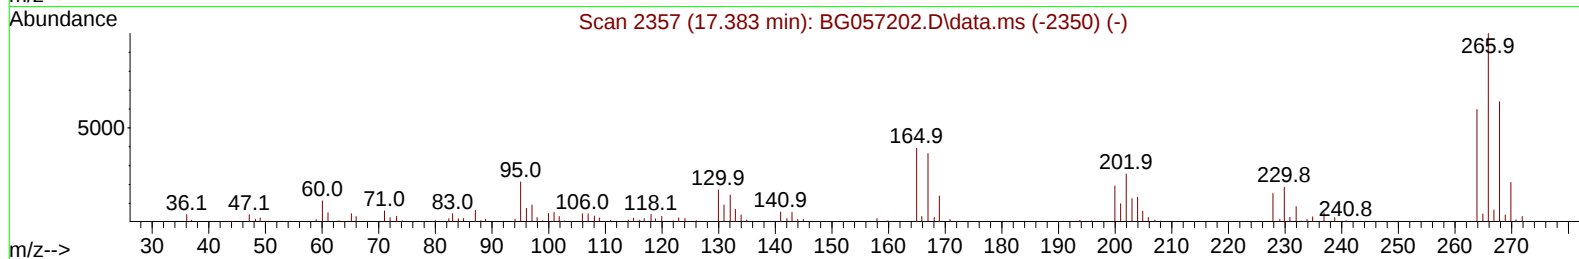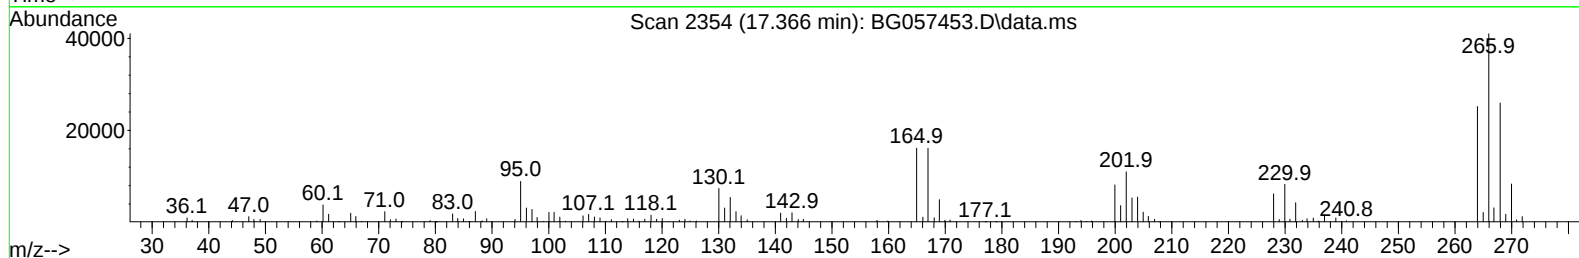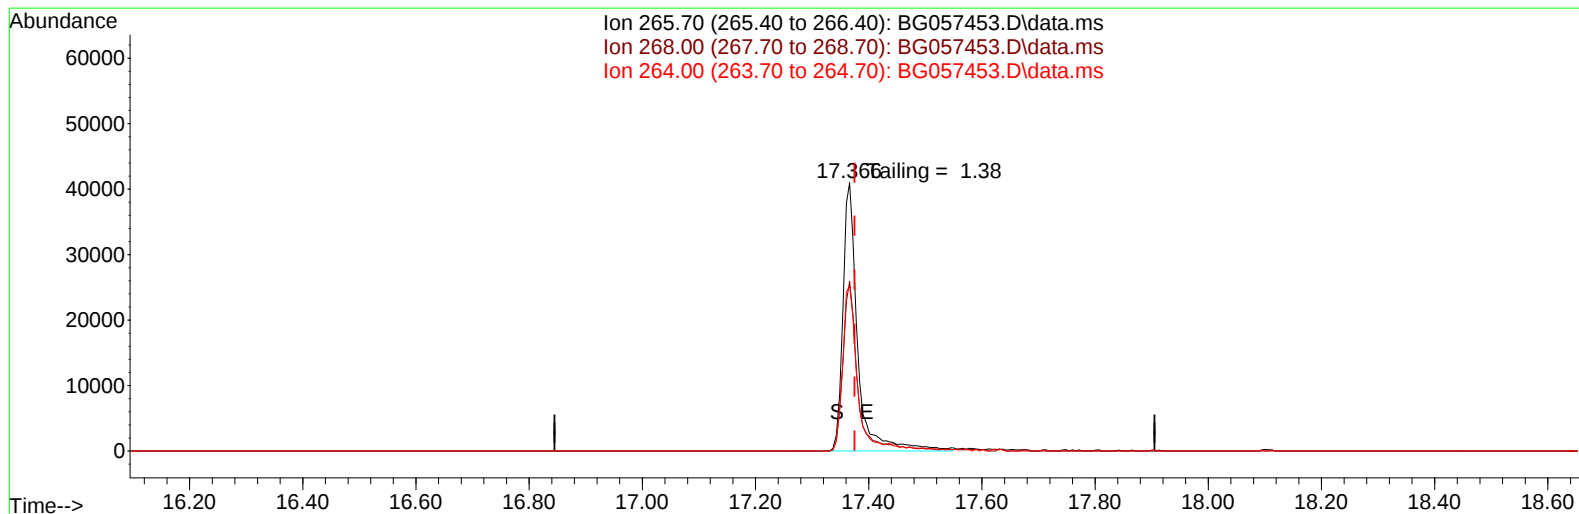

TIC: BG057453.D\data.ms

(70) Pentachlorophenol (C)

17.366min (-0.009) 41136.49 ng




response 74529

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.29  |
| 264.00 | 59.70  | 61.46  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG051823\  
Data File : BG057453.D  
Acq On : 18 May 2023 9:03  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: May 18 17:10:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG042723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 12 22:04:03 2023  
Response via : Initial Calibration

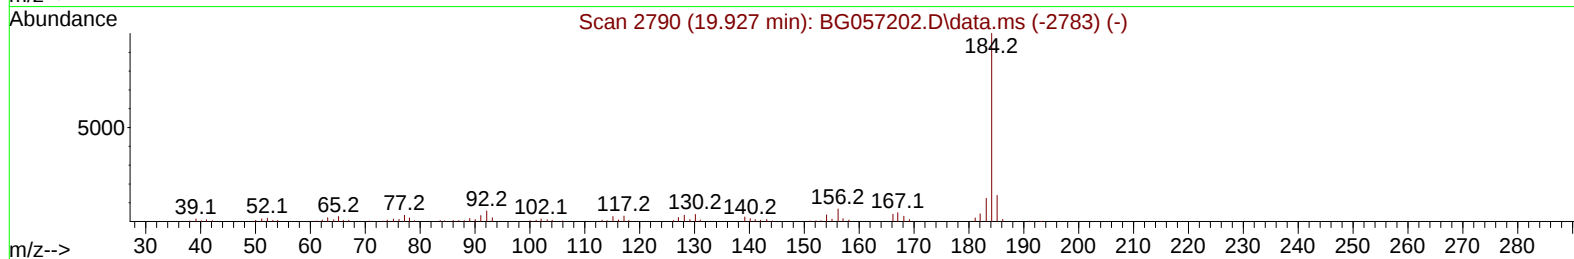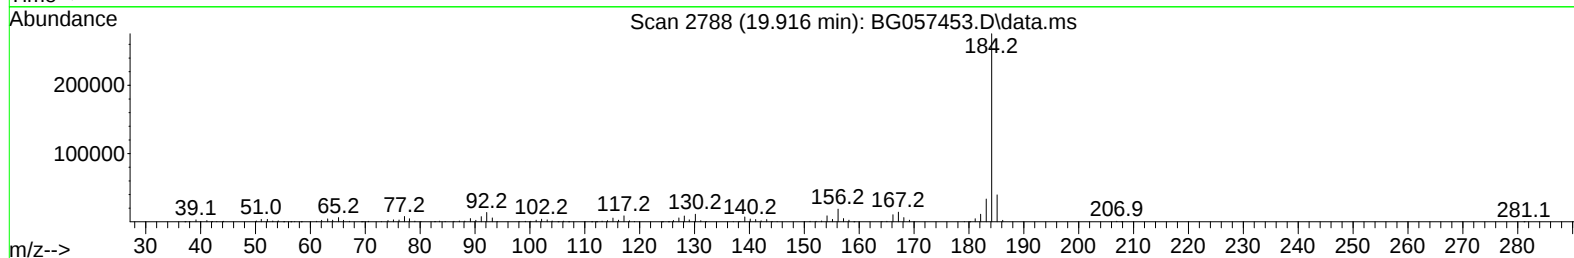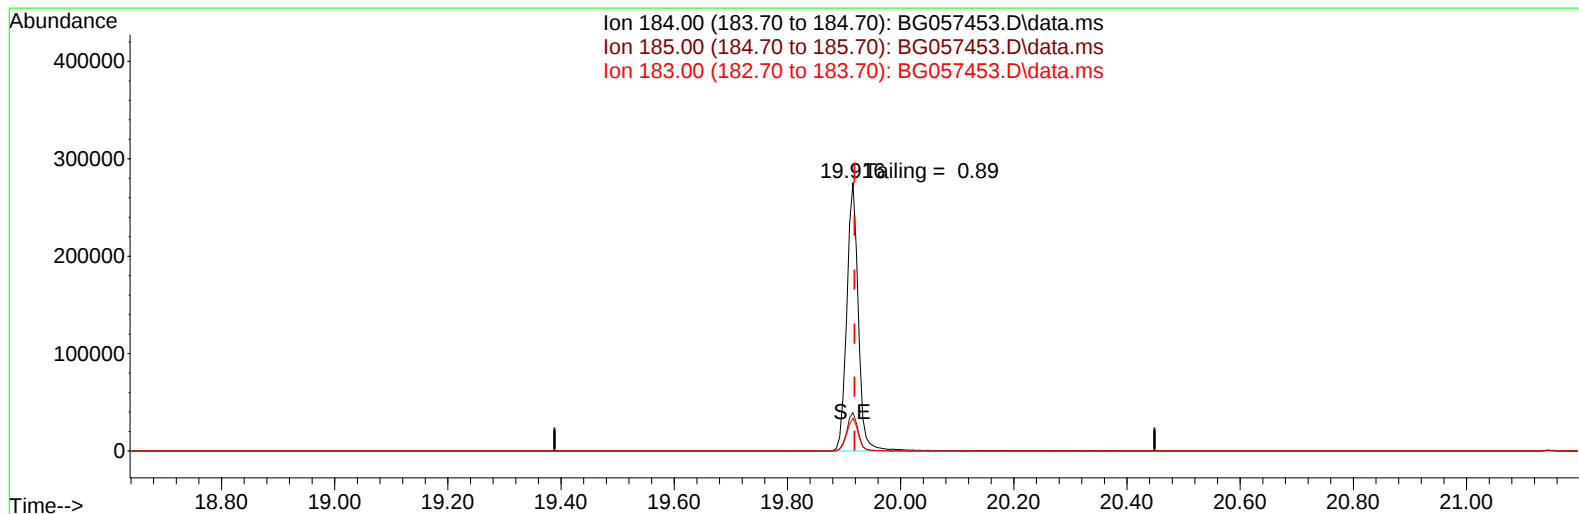

TIC: BG057453.D\data.ms

(77) Benzidine

19.916min (-0.003) 0.00 ng

response 391693

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.32  |
| 183.00 | 12.40  | 12.15  |
| 0.00   | 0.00   | 0.00   |