
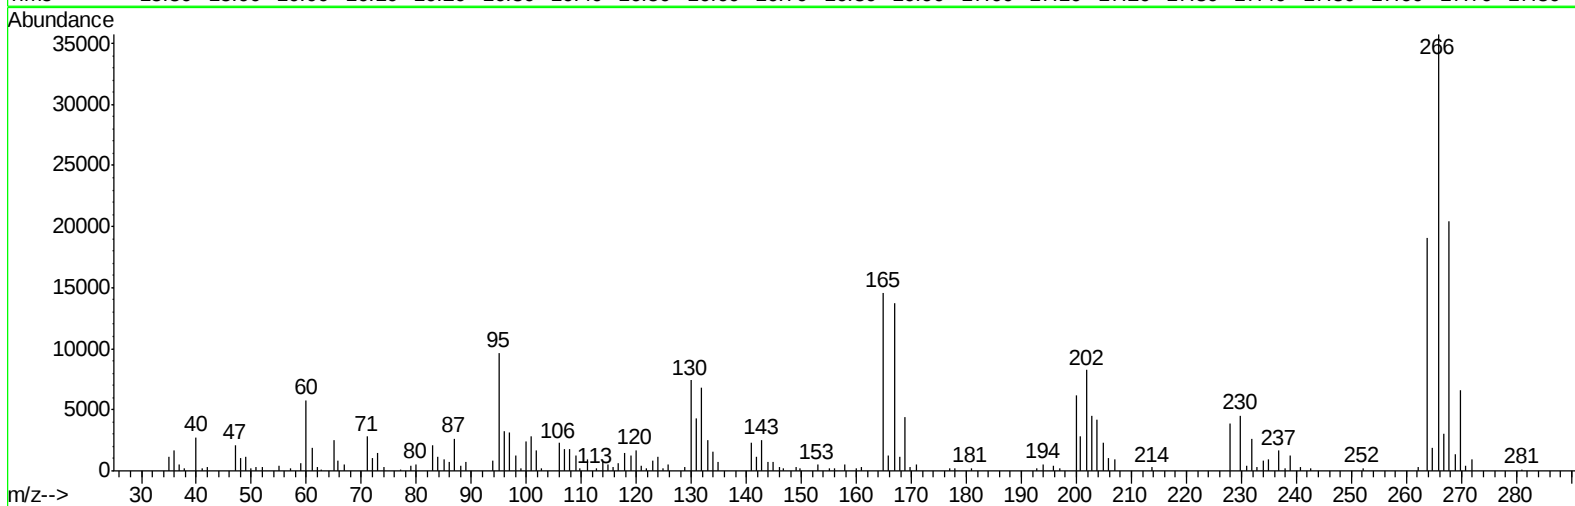


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051915\
Data File : BG017199.D
Acq On : 19 May 2015 14:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 07:02:27 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

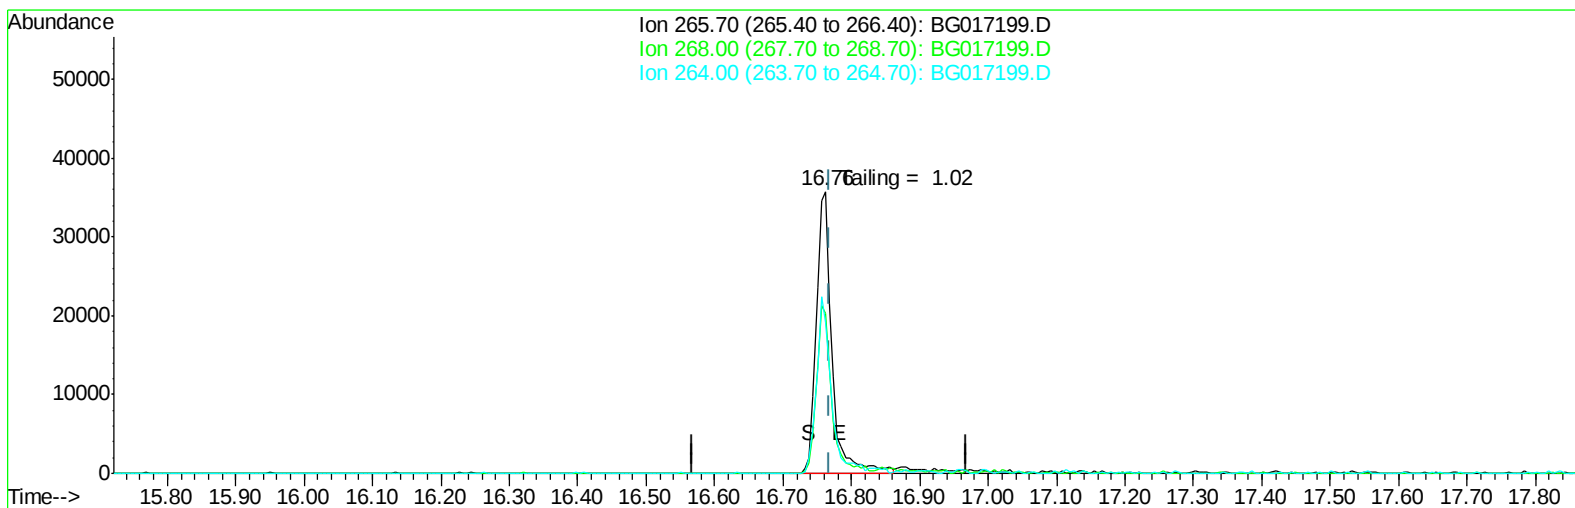

TIC: BG017199.D

(69) Pentachlorophenol (C)



16.762min (-0.006) 3059.53ng

response 56997

Ion	Exp%	Act%
265.70	100	100
268.00	70.70	57.05
264.00	61.70	53.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG051915\
Data File : BG017199.D
Acq On : 19 May 2015 14:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 07:02:27 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 16:12:13 2015
Response via : Initial Calibration

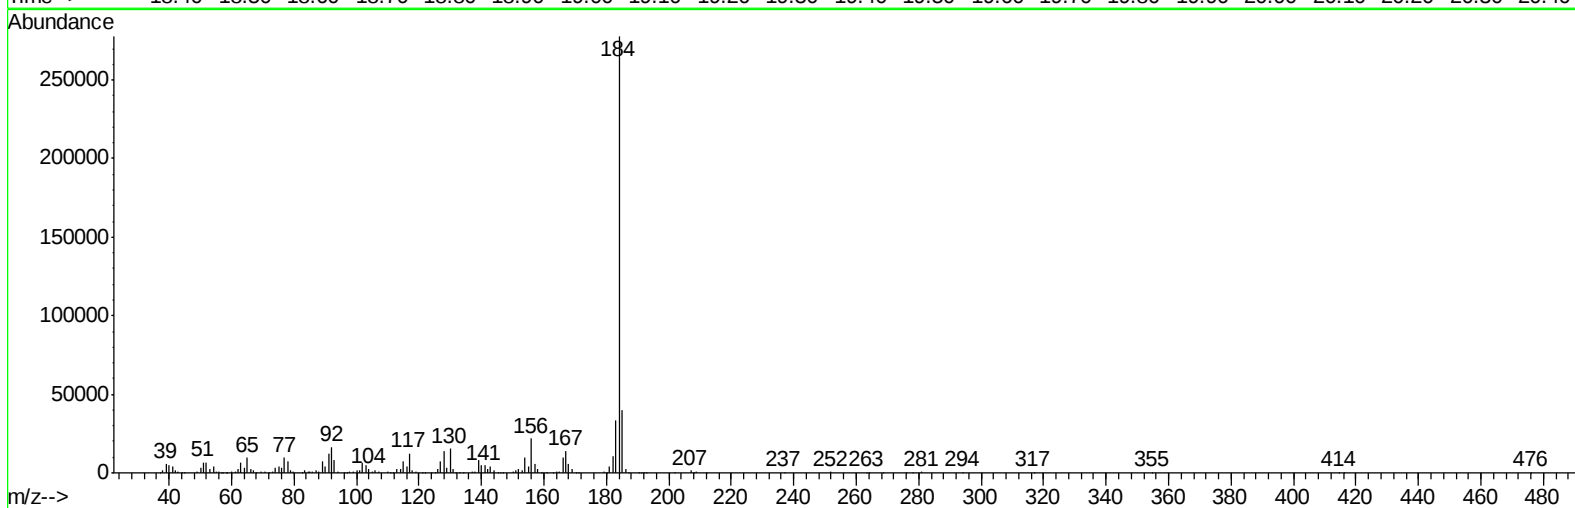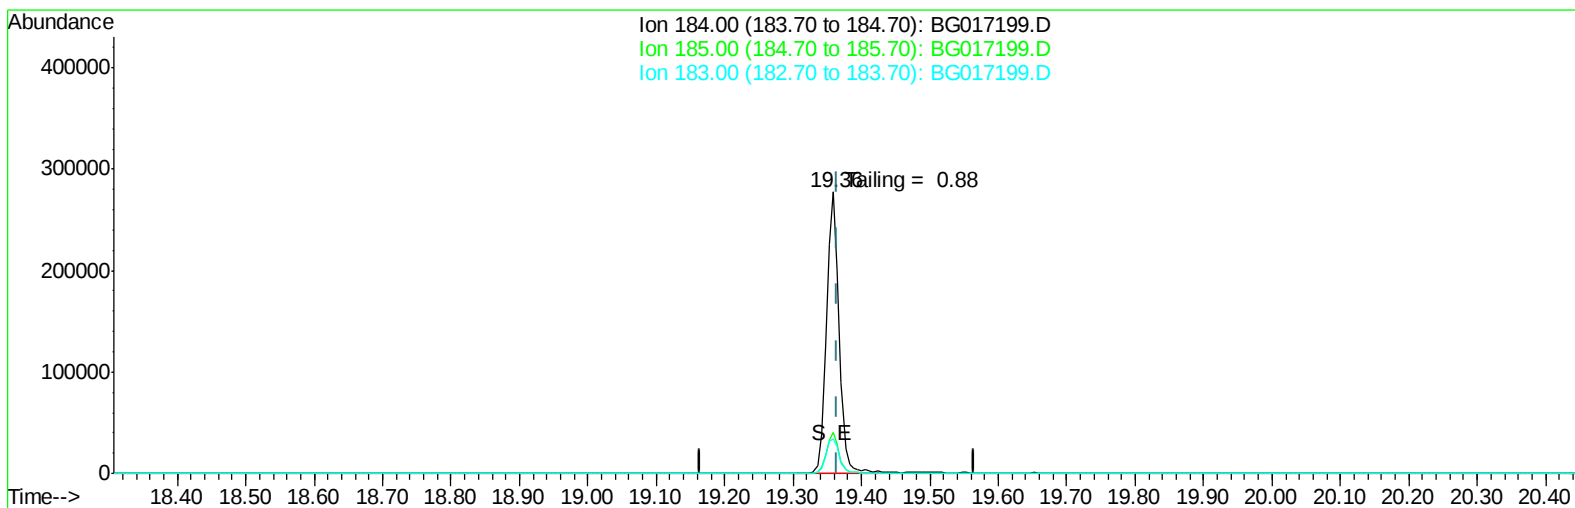

TIC: BG017199.D

(76) Benzidine

19.359min (-0.006) 170533.90ng

response 361913

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.43
183.00	14.30	12.16
0.00	0.00	0.00