
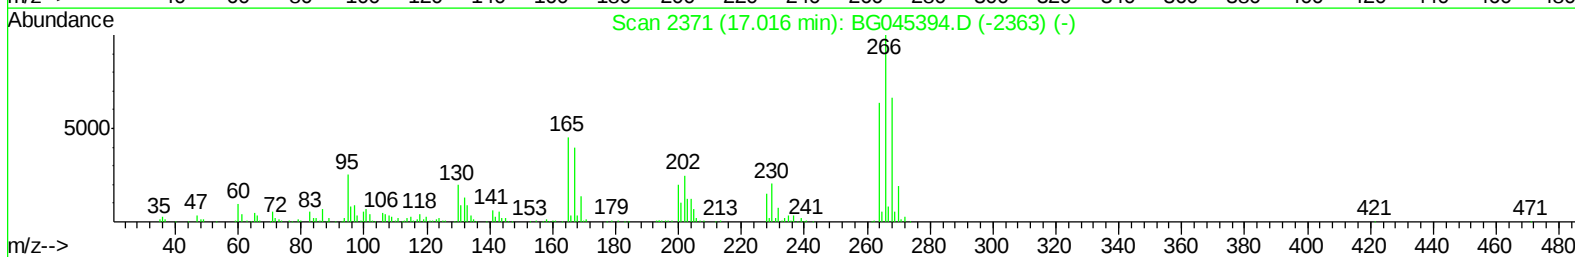
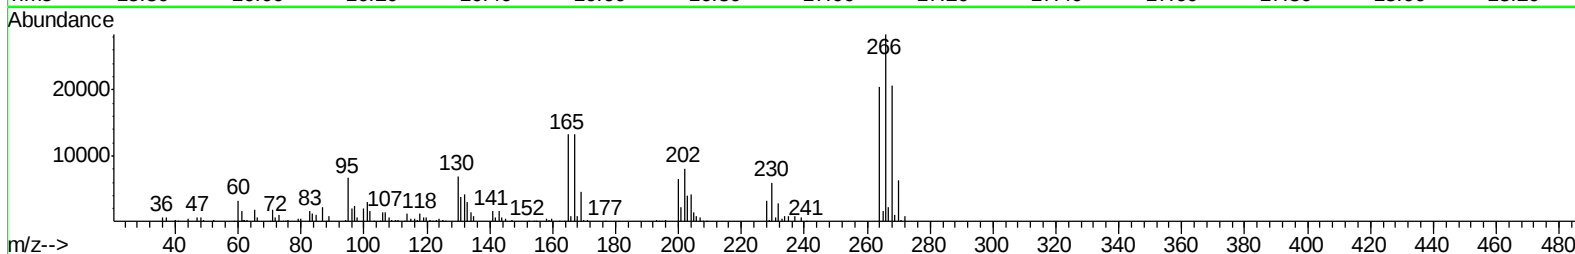


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051920\
 Data File : BG045421.D
 Acq On : 19 May 2020 9:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 02:31:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 19 12:10:36 2020
 Response via : Initial Calibration

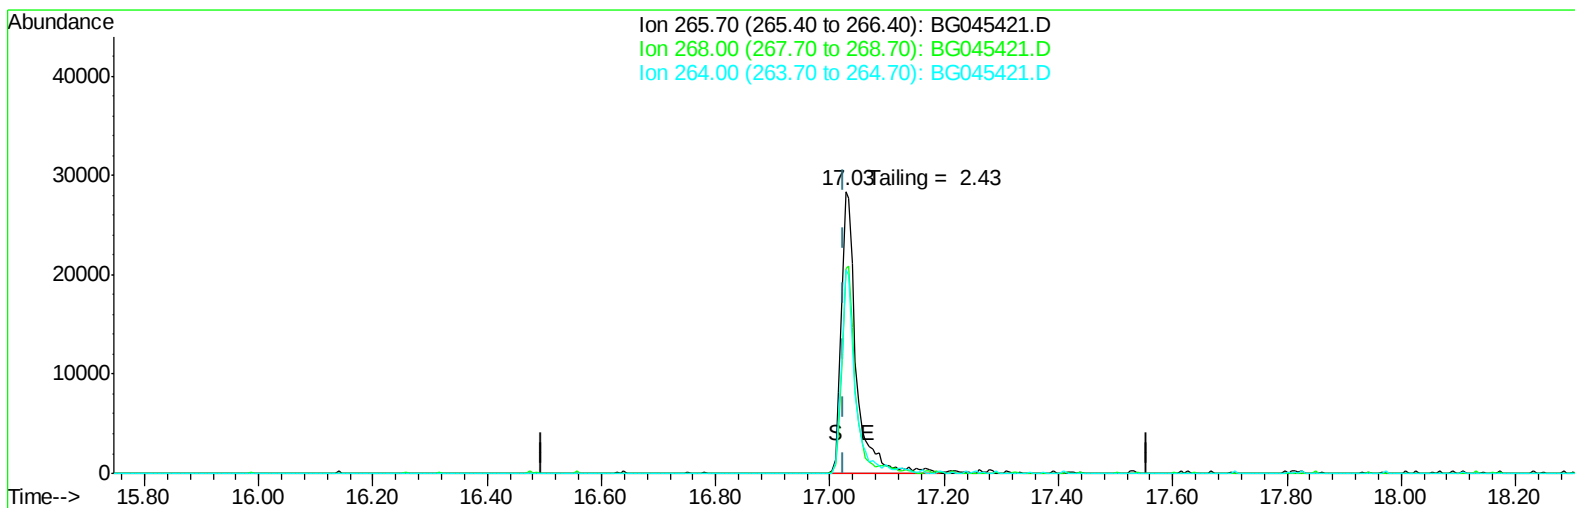

TIC: BG045421.D

(70) Pentachlorophenol (C)




17.027min (+0.002) 134060.69ng

response 51244

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	72.62
264.00	63.70	72.40
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG051920\
Data File : BG045421.D
Acq On : 19 May 2020 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 02:31:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 19 12:10:36 2020
Response via : Initial Calibration

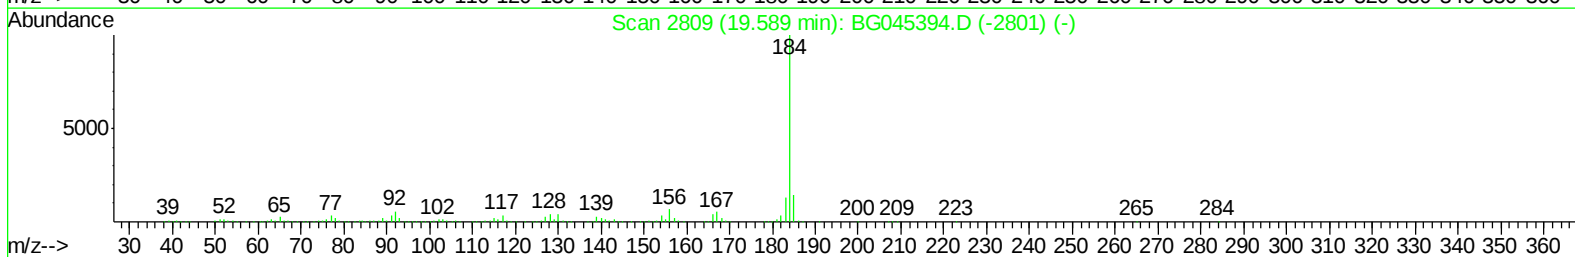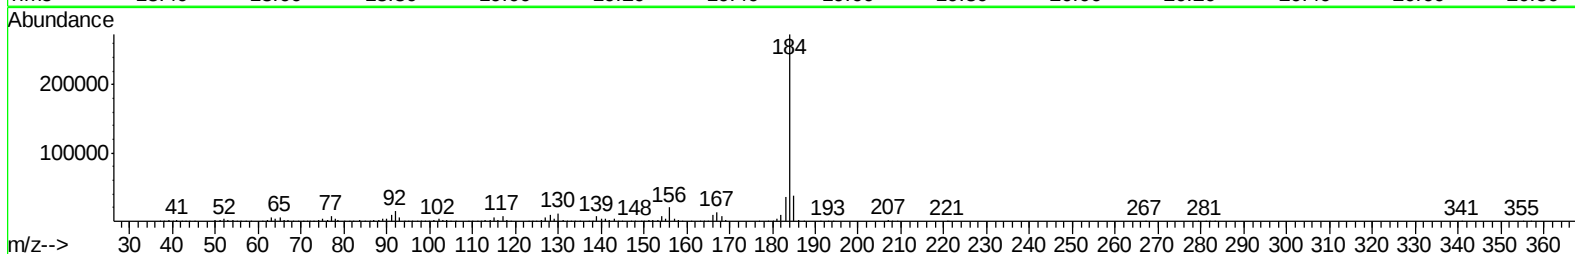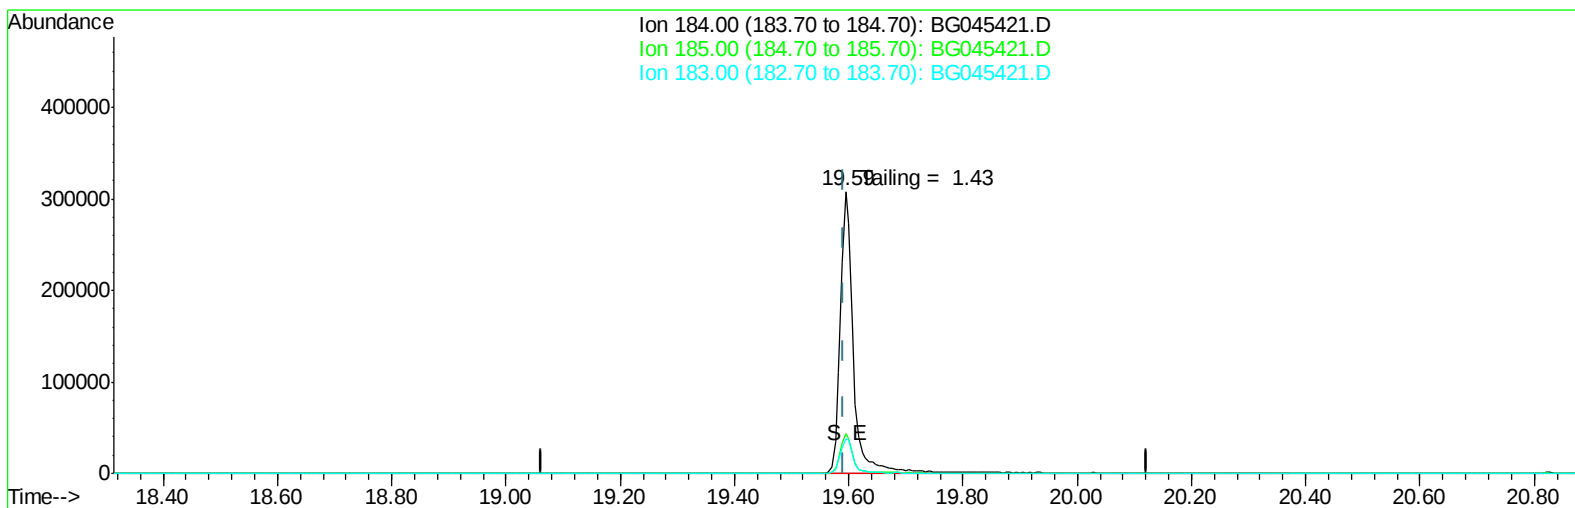

TIC: BG045421.D

(77) Benzidine

19.594min (+0.002) 12846.15ng

response 492118

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.32
183.00	12.80	12.38
0.00	0.00	0.00