


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG051920\
 Data File : BG045421.D
 Acq On : 19 May 2020 9:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 19 12:10:36 2020

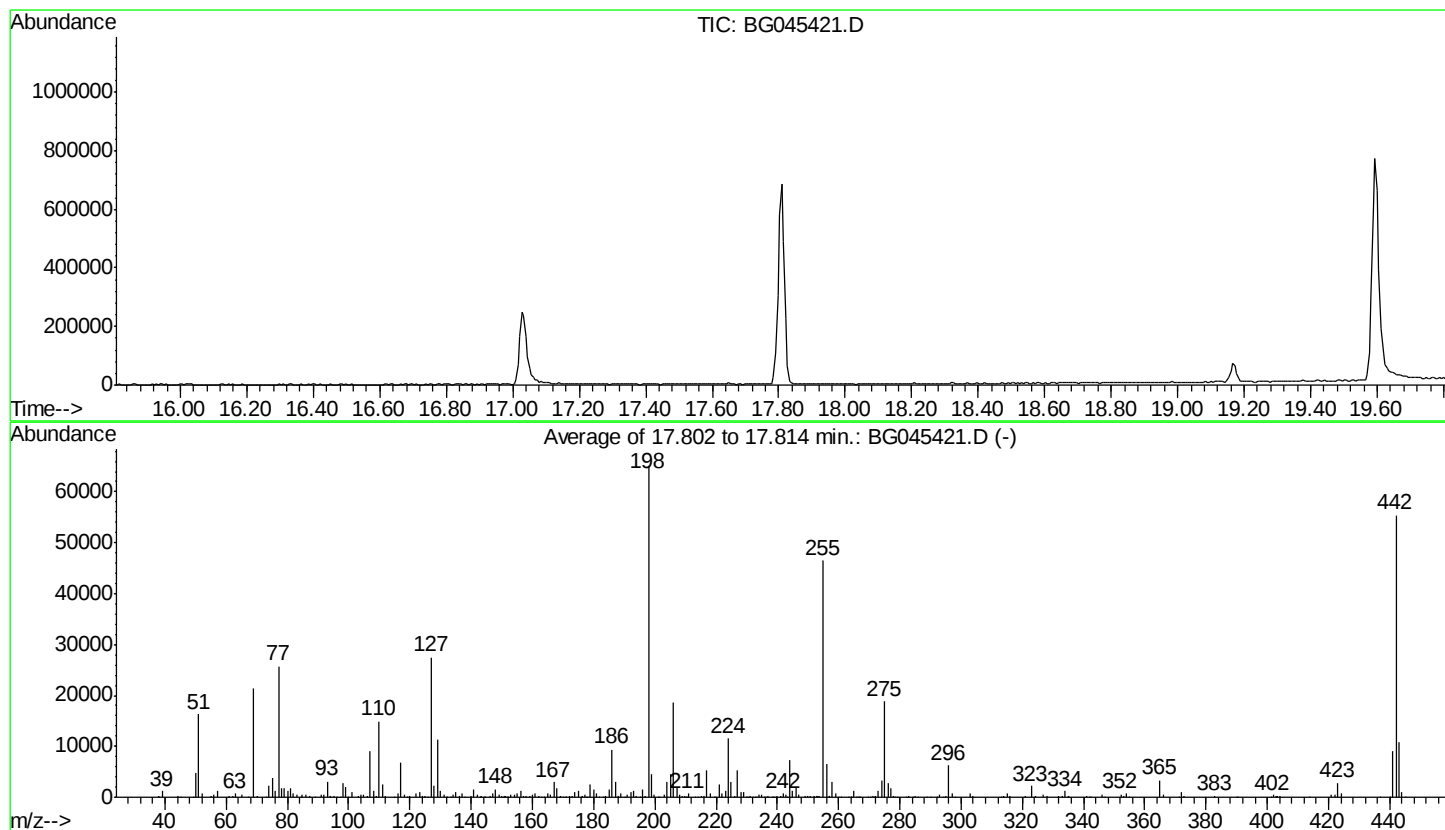

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	16239	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.8	21382	PASS
70	69	0.00	2	1.0	211	PASS
127	198	10	80	42.2	27504	PASS
197	198	0.00	2	0.4	258	PASS
198	198	100	100	100.0	65149	PASS
199	198	5	9	7.0	4585	PASS
275	198	10	60	28.8	18761	PASS
365	198	1	100	5.1	3324	PASS
441	198	0.01	100	14.0	9121	PASS
442	198	50	100	85.0	55349	PASS
443	442	15	24	19.7	10891	PASS