
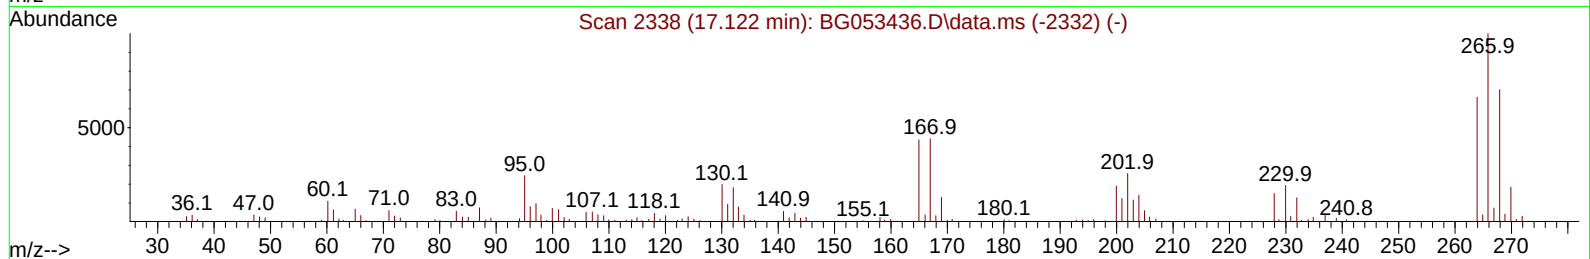
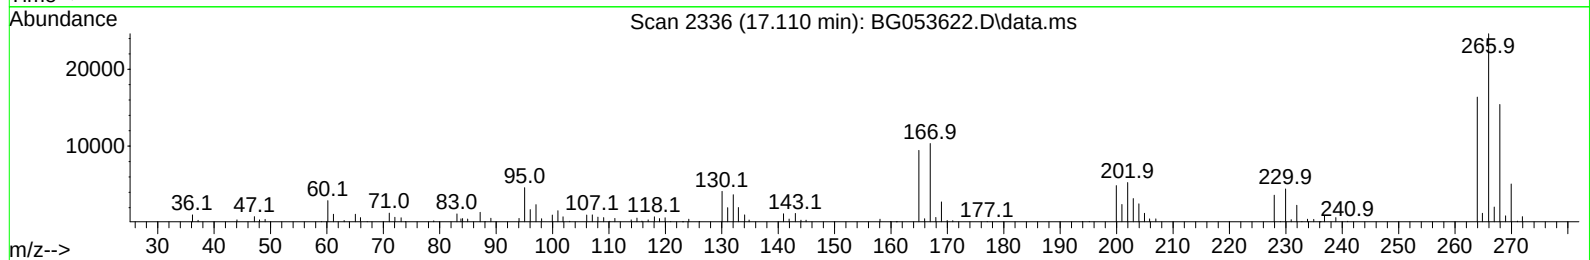


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053622.D
Acq On : 19 May 2022 12:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 12:46:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

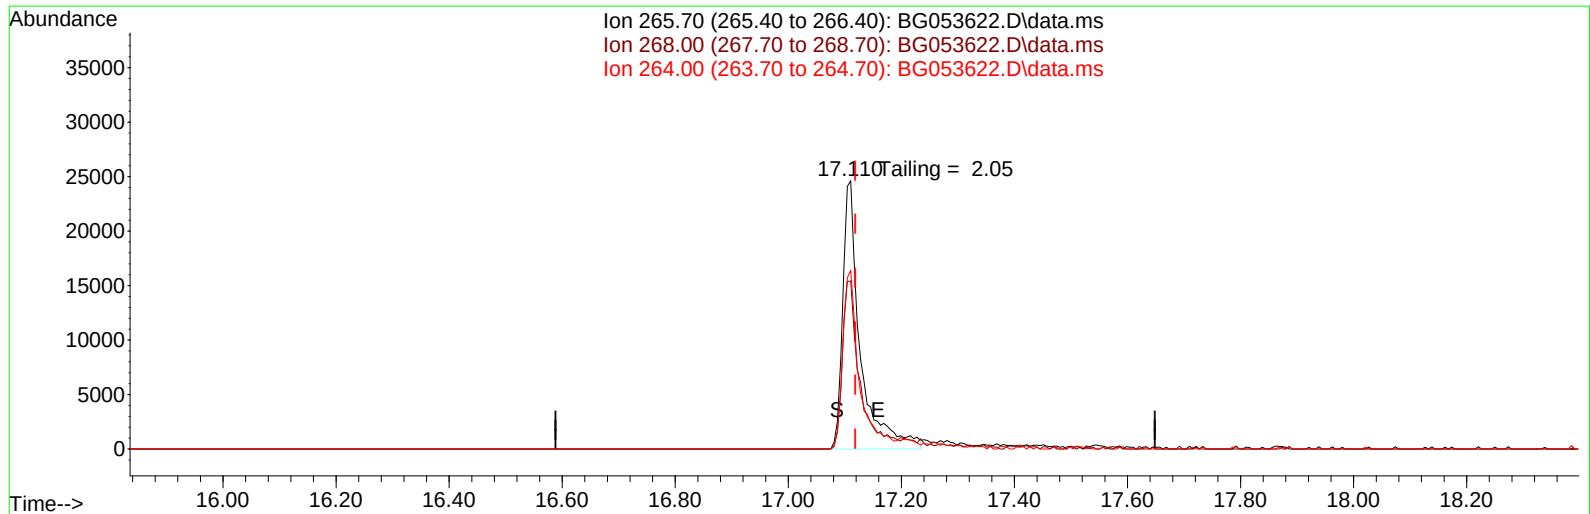

TIC: BG053622.D\data.ms

(70) Pentachlorophenol (C)




17.110min (-0.008) 28571.60 ng

response 52229

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.61
264.00	66.20	66.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053622.D
Acq On : 19 May 2022 12:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 12:46:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

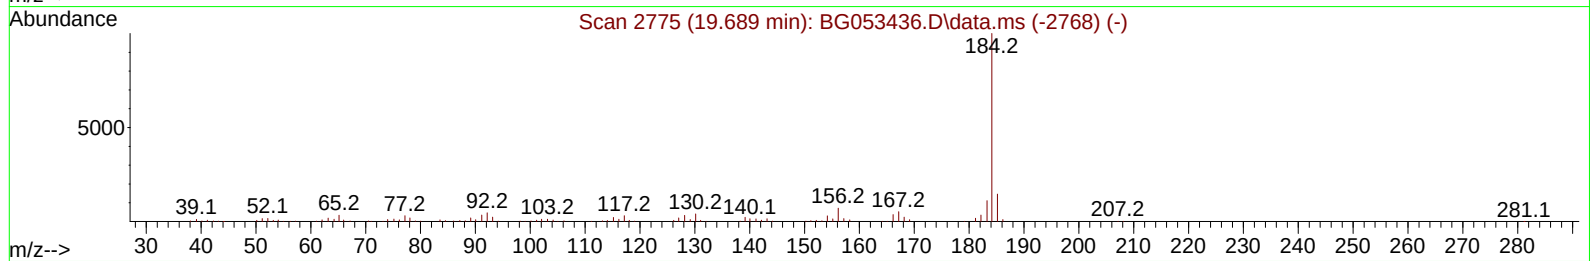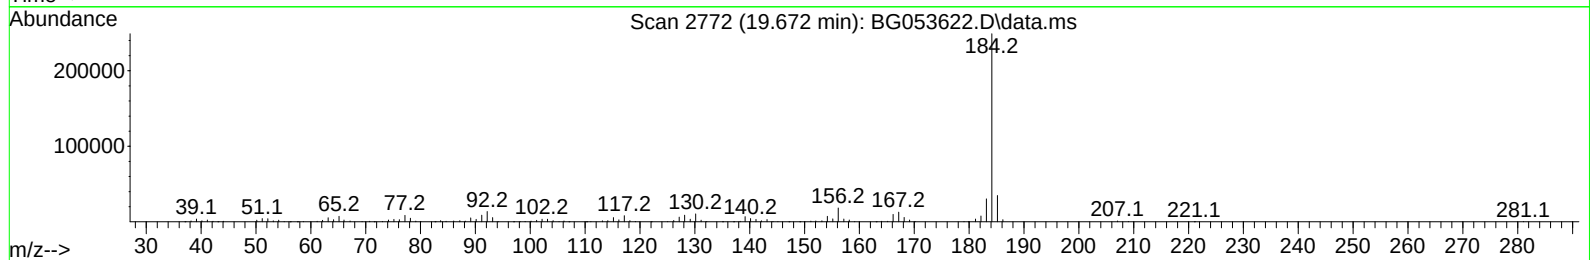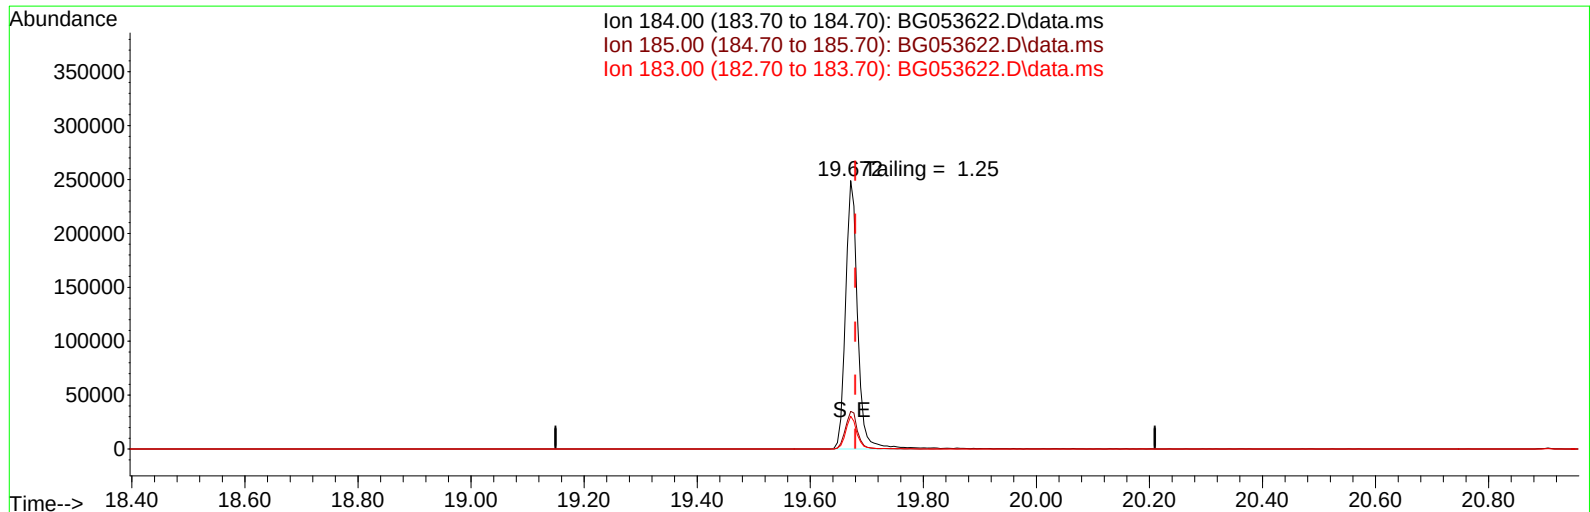

TIC: BG053622.D\data.ms

(77) Benzidine

19.672min (-0.008) 0.00 ng

response 371538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.04
183.00	11.10	12.24
0.00	0.00	0.00