

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
 Data File : BG053634.D
 Acq On : 19 May 2022 20:12
 Operator : CG/JU
 Sample : N2935-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-03-051822

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/20/2022
 Supervised By : Jagrut Upadhyay 05/20/2022

Quant Time: May 20 03:58:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 03:55:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	33862	20.000	ng	0.00
21) Naphthalene-d8	10.889	136	137851	20.000	ng	0.00
39) Acenaphthene-d10	14.701	164	96074	20.000	ng	0.00
64) Phenanthrene-d10	17.450	188	194683	20.000	ng	0.00
76) Chrysene-d12	21.733	240	163239	20.000	ng	0.00
86) Perylene-d12	25.011	264	169882	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.655	112	13895m	6.964	ng	0.01
7) Phenol-d6	7.253	99	19704m	6.507	ng	0.01
23) Nitrobenzene-d5	9.238	82	13848	4.276	ng	0.00
42) 2,4,6-Tribromophenol	16.199	330	7181	5.068	ng	0.00
45) 2-Fluorobiphenyl	13.327	172	32833	4.994	ng	0.00
79) Terphenyl-d14	20.053	244	47062	5.370	ng	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053634.D
Acq On : 19 May 2022 20:12
Operator : CG/JU
Sample : N2935-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
OK-03-051822

Quant Time: May 20 03:58:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 03:55:28 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

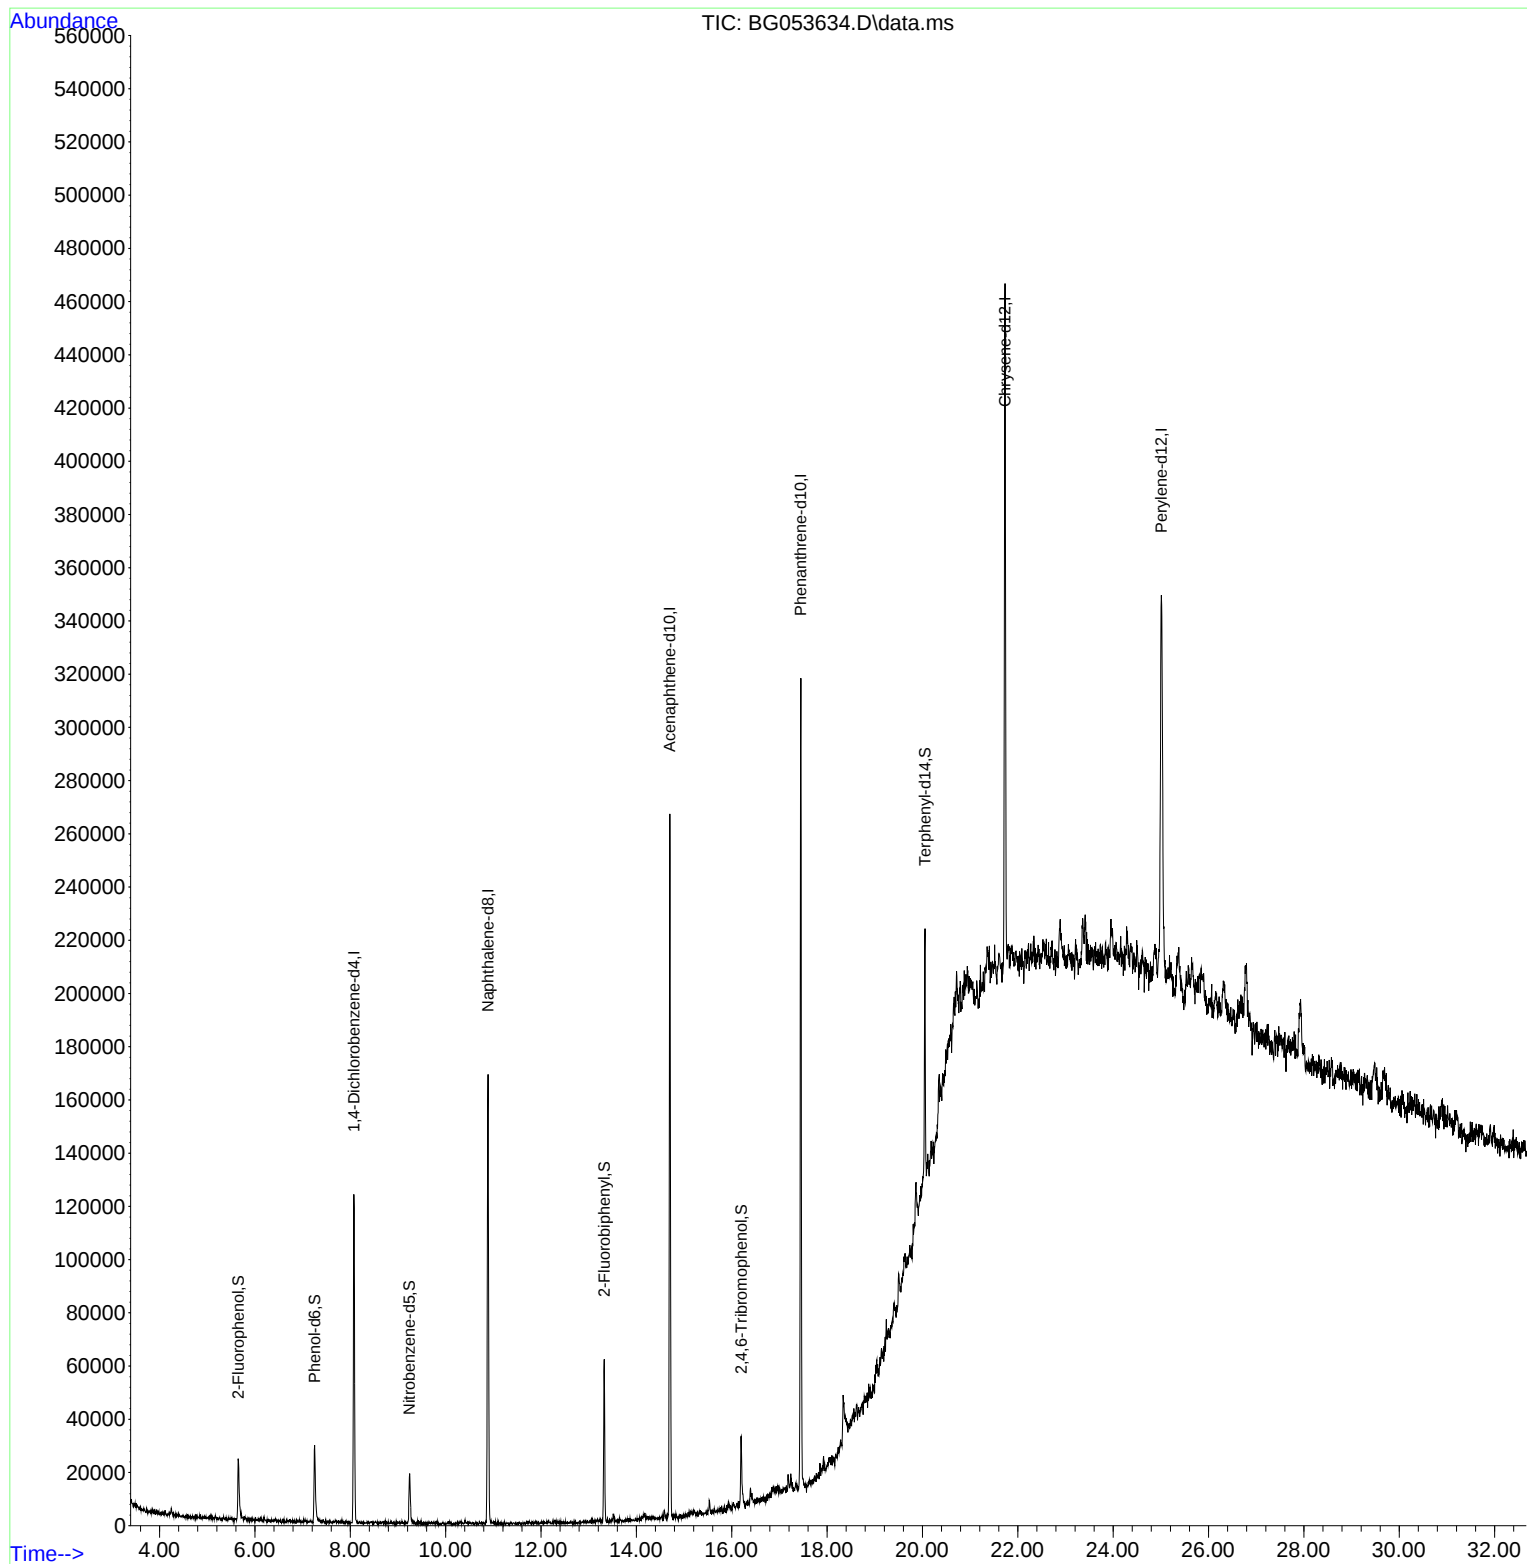




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.075 min Scan# 798
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

Instrument :

BNA_G

ClientSampleId :

OK-03-051822






Tgt Ion:152 Resp: 33862
Ion Ratio Lower Upper
152 100
150 145.4 131.6 197.4
115 56.2 50.9 76.3


Manual Integrations

APPROVED



Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

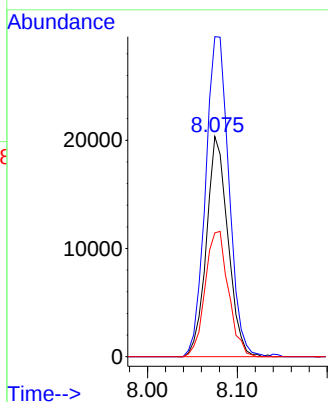


#5
2-Fluorophenol
Concen: 6.964 ng m
RT: 5.655 min Scan# 386
Delta R.T. 0.012 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

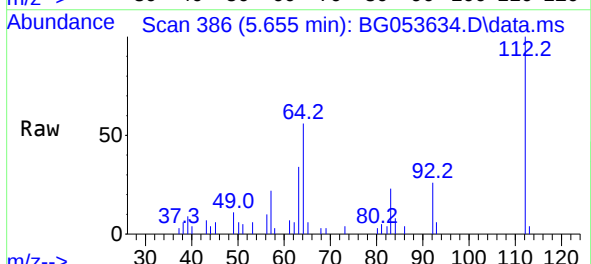


Tgt Ion:112 Resp: 13895
Ion Ratio Lower Upper
112 100
64 55.6 55.1 82.7
63 33.6 30.4 45.6

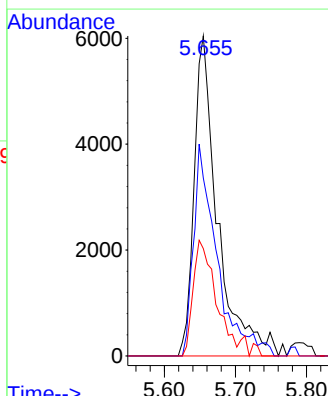



#7
Phenol-d6
Concen: 6.507 ng m
RT: 7.253 min Scan# 61
Delta R.T. 0.012 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12




Instrument :
BNA_G
ClientSampleId :
OK-03-051822




Tgt Ion: 99 Resp: 19704
Ion Ratio Lower Upper
99 100
42 17.6 17.0 25.6
71 44.6 33.8 50.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

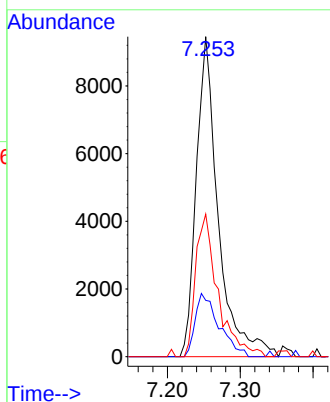


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.889 min Scan# 1277
Delta R.T. 0.006 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

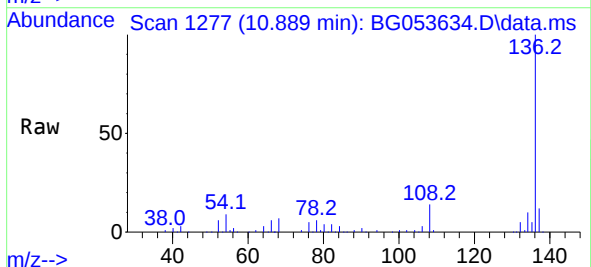

Tgt Ion:136 Resp: 137851
Ion Ratio Lower Upper
136 100
137 11.8 8.5 12.7
54 9.0 7.4 11.2
68 7.1 4.9 7.3

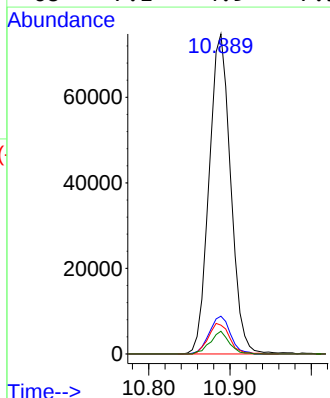




#23
Nitrobenzene-d5
Concen: 4.276 ng
RT: 9.238 min Scan# 91
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

Instrument :

BNA_G

ClientSampleId :




OK-03-051822




Tgt Ion: 82 Resp: 1384
Ion Ratio Lower Upper
82 100
128 30.3 27.9 41.9
54 50.0 41.2 61.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

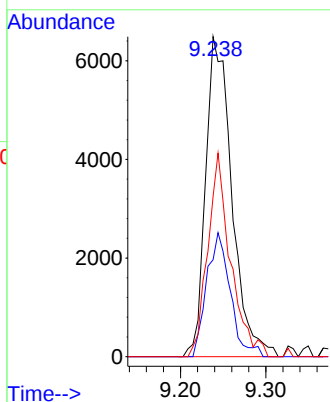


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.701 min Scan# 1926
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

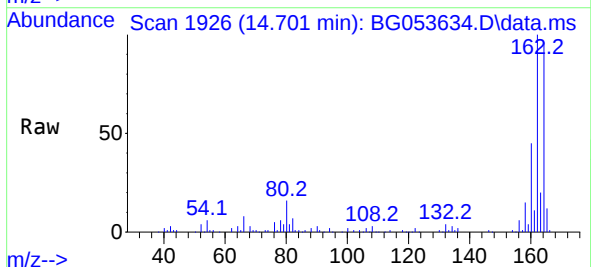

Tgt Ion:164 Resp: 96074
Ion Ratio Lower Upper
164 100
162 103.8 82.3 123.5
160 47.1 34.2 51.2

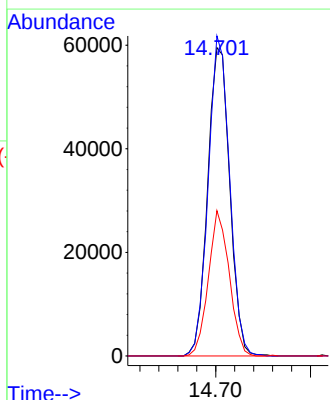




#42
2,4,6-Tribromophenol
Concen: 5.068 ng
RT: 16.199 min Scan# 2183
Delta R.T. 0.006 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

Instrument :

BNA_G

ClientSampleId :

OK-03-051822






Tgt Ion:330 Resp: 718
Ion Ratio Lower Upper
330 100
332 86.0 76.0 114.0
141 37.0 27.1 40.7


Manual Integrations

APPROVED



Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

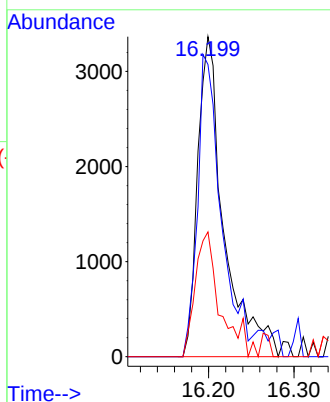


#45
2-Fluorobiphenyl
Concen: 4.994 ng
RT: 13.327 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12



Tgt Ion:172 Resp: 32833
Ion Ratio Lower Upper
172 100
171 32.0 28.5 42.7
170 19.9 18.9 28.3

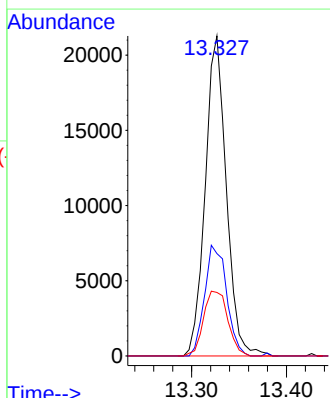




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.450 min Scan# 2194
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

Instrument :

BNA_G

ClientSampleId :

OK-03-051822






Tgt Ion:188 Resp: 19468
Ion Ratio Lower Upper
188 100
94 6.2 5.4 8.0
80 7.7 6.8 10.2


Manual Integrations

APPROVED



Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

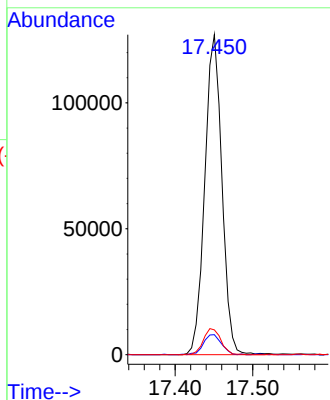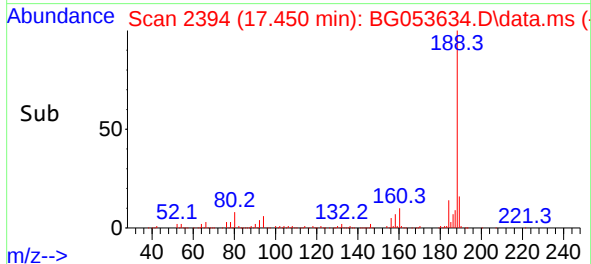


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.733 min Scan# 3123
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

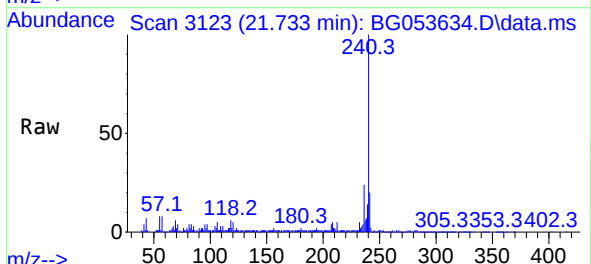

Tgt Ion:240 Resp: 163239
Ion Ratio Lower Upper
240 100
120 5.3 4.6 7.0
236 24.5 20.2 30.4

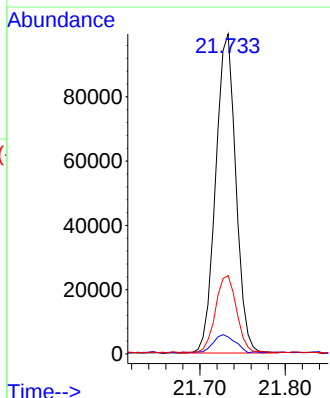



#79
Terphenyl-d14
Concen: 5.370 ng
RT: 20.053 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

Instrument :

BNA_G

ClientSampleId :





OK-03-051822

Tgt Ion:244 Resp: 47062
Ion Ratio Lower Upper
244 100
212 9.1 6.5 9.7
122 5.1 5.0 7.4

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 05/20/2022
Supervised By :Jagrut Upadhyay 05/20/2022

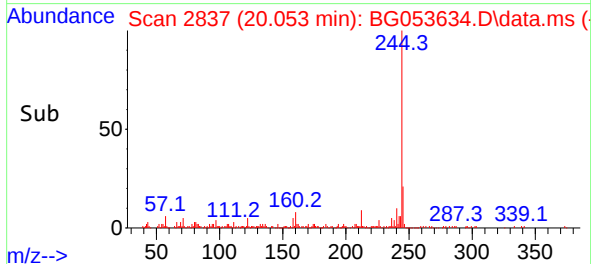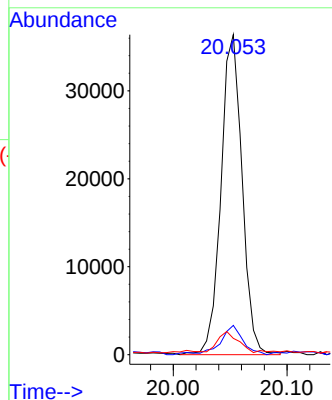

#86
Perylene-d12
Concen: 20.000 ng
RT: 25.011 min Scan# 3681
Delta R.T. 0.006 min
Lab File: BG053634.D
Acq: 19 May 2022 20:12

Tgt Ion:264 Resp: 169882
Ion Ratio Lower Upper
264 100
260 23.4 19.0 28.6
265 23.1 17.4 26.2

