

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
 Data File : BG053634.D
 Acq On : 19 May 2022 20:12
 Operator : CG/JU
 Sample : N2935-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-03-051822

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.649	379	385	395	rBV2	23243	51546	11.09%	2.235%
2	7.253	652	658	667	rBV	29278	62526	13.46%	2.711%
3	8.075	791	798	809	rBV	123469	215951	46.47%	9.362%
4	9.244	990	997	1003	rBV2	18718	38210	8.22%	1.657%
5	10.889	1270	1277	1286	rBV	168634	307533	66.18%	13.332%
6	13.327	1686	1692	1698	rBV	60941	94721	20.38%	4.106%
7	14.584	1902	1906	1909	rBV3	4119	6874	1.48%	0.298%
8	14.701	1920	1926	1933	rVB	263672	417428	89.83%	18.097%
9	15.530	2064	2067	2071	rVB3	4546	5500	1.18%	0.238%
10	16.199	2174	2181	2191	rBV4	27057	56892	12.24%	2.466%
11	16.393	2210	2214	2218	rBV5	6435	10157	2.19%	0.440%
12	17.180	2346	2348	2354	rBV6	6380	9394	2.02%	0.407%
13	17.239	2356	2358	2363	rVB5	5705	5869	1.26%	0.254%
14	17.450	2388	2394	2400	rBV	302385	464679	100.00%	20.145%
15	18.338	2541	2545	2547	rBV5	19232	27071	5.83%	1.174%
16	20.053	2833	2837	2842	rVB	93032	117218	25.23%	5.082%
17	21.733	3118	3123	3130	rVB	253992	415096	89.33%	17.996%


Sum of corrected areas: 2306665

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053634.D
Acq On : 19 May 2022 20:12
Operator : CG/JU
Sample : N2935-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-03-051822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

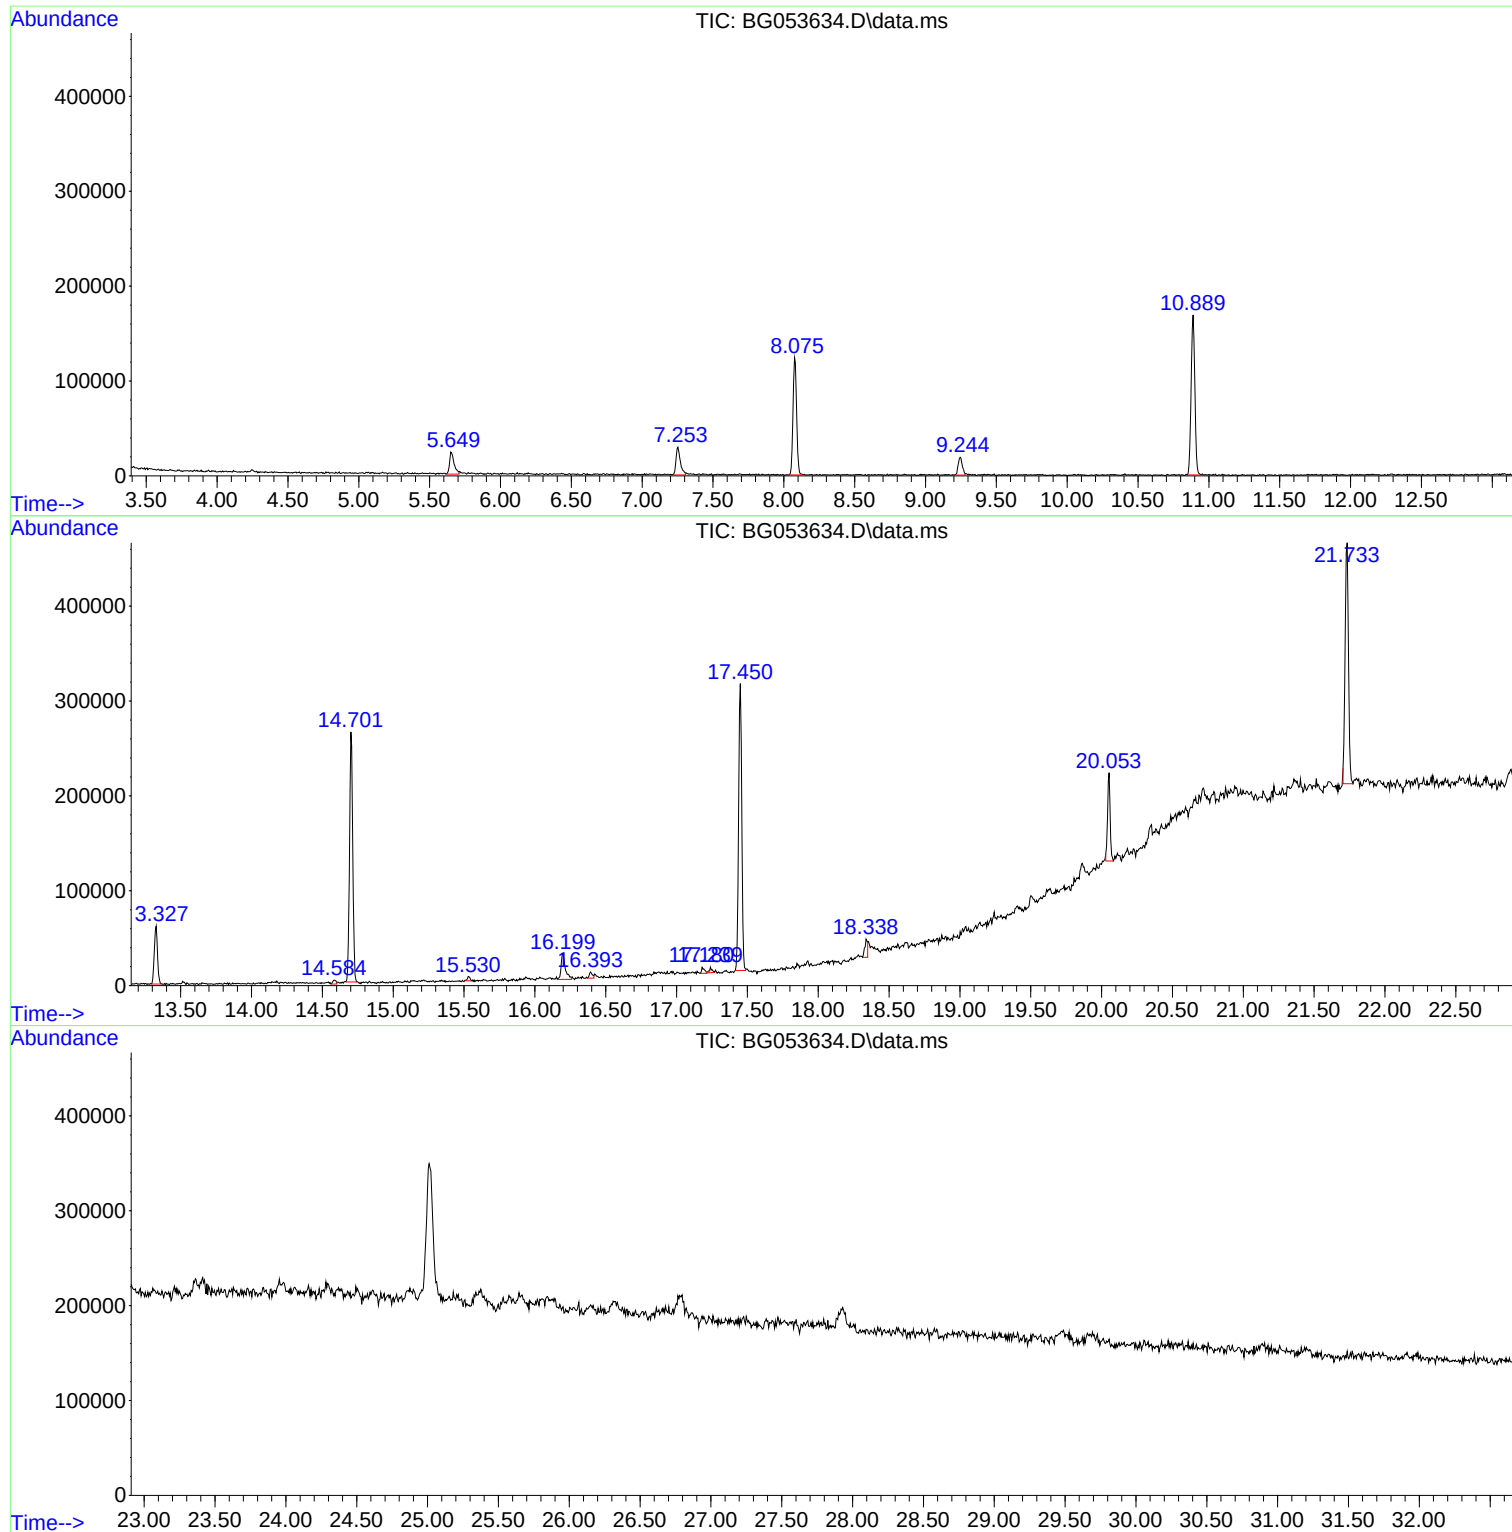

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053634.D
Acq On : 19 May 2022 20:12
Operator : CG/JU
Sample : N2935-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-03-051822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053634.D
Acq On : 19 May 2022 20:12
Operator : CG/JU
Sample : N2935-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-03-051822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------