


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
 Data File : BG053622.D
 Acq On : 19 May 2022 12:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 03:55:28 2022

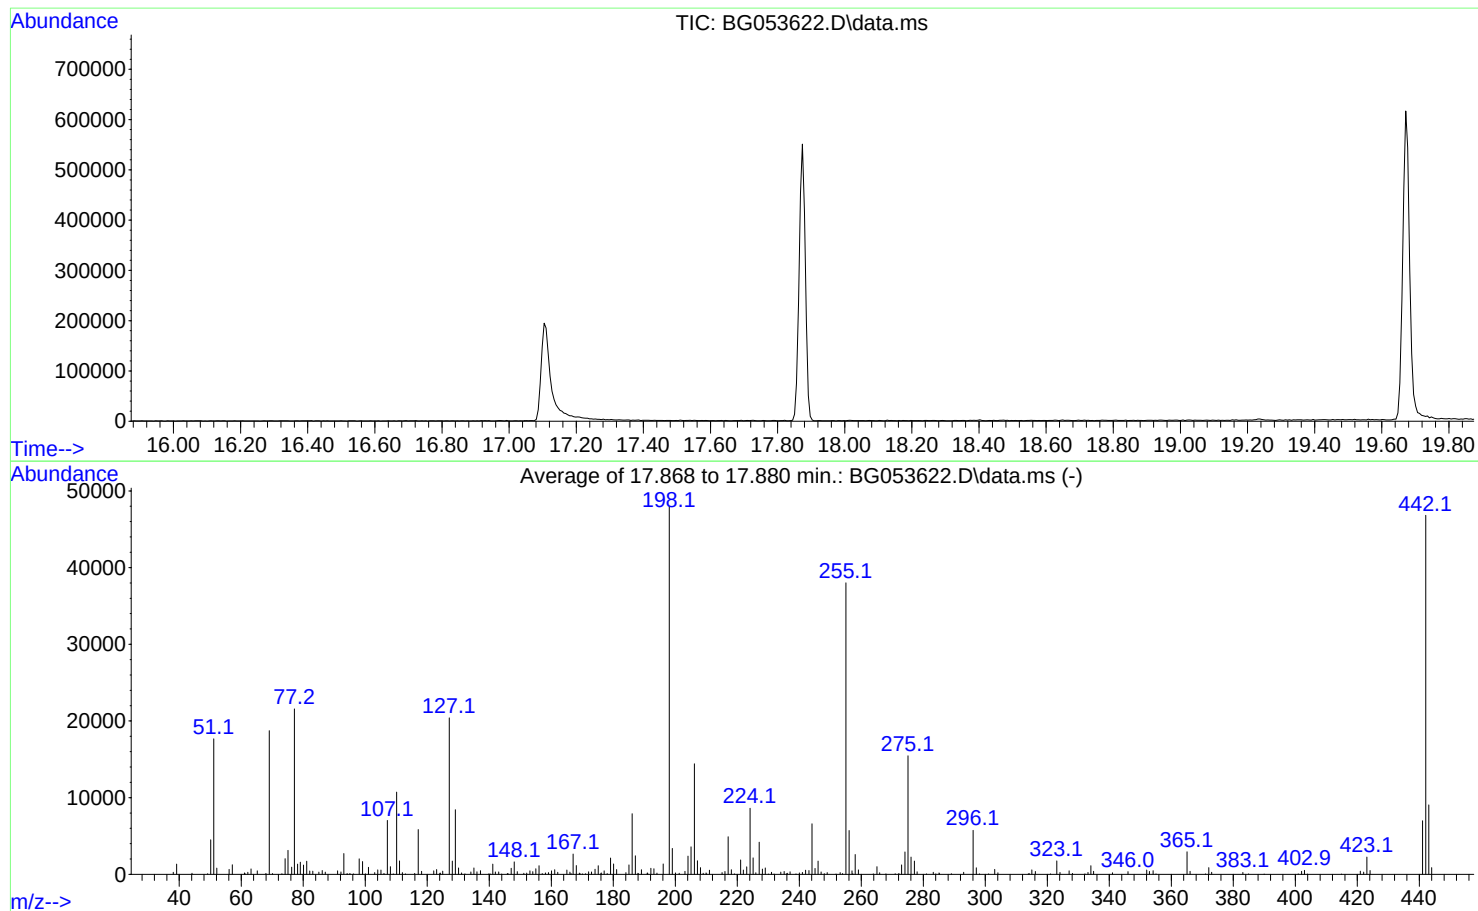




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	17675	PASS
68	69	0.00	2	0.6	120	PASS
69	198	0.00	100	39.0	18731	PASS
70	69	0.00	2	0.6	111	PASS
127	198	10	80	42.5	20403	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47968	PASS
199	198	5	9	7.0	3372	PASS
275	198	10	60	32.2	15456	PASS
365	198	1	100	6.1	2950	PASS
441	198	0.01	100	14.6	6996	PASS
442	442	50	100	100.0	46813	PASS
443	442	15	24	19.4	9062	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053622.D
Acq On : 19 May 2022 12:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 19 12:46:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

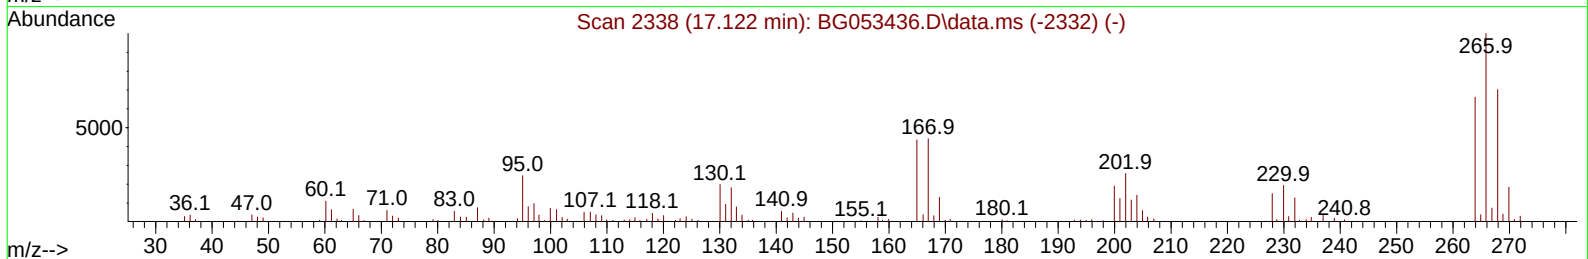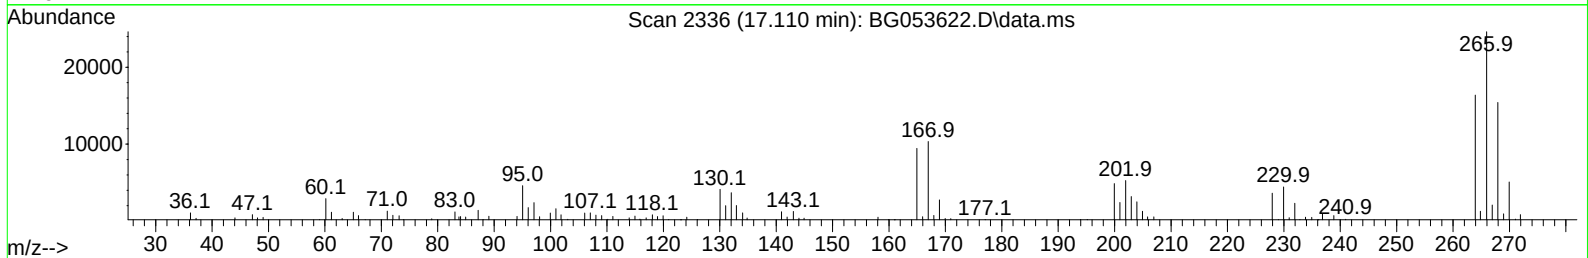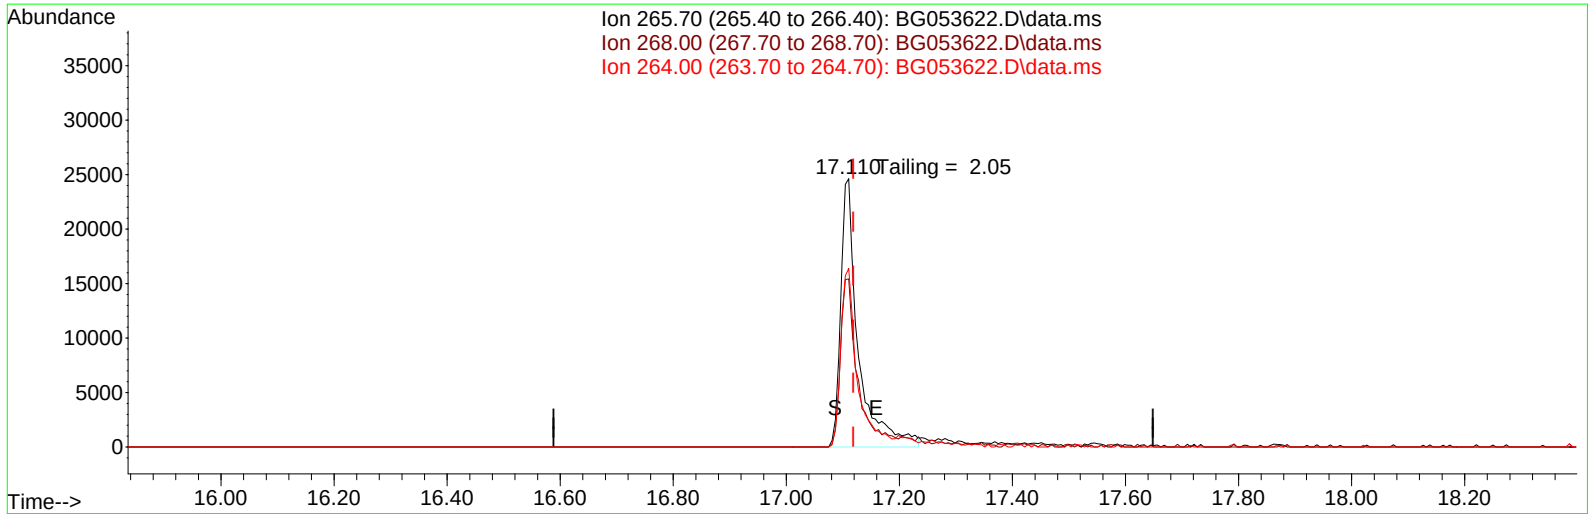

TIC: BG053622.D\data.ms

(70) Pentachlorophenol (C)

17.110min (-0.008) 28571.60 ng




response 52229

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.61
264.00	66.20	66.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG051922\
Data File : BG053622.D
Acq On : 19 May 2022 12:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 19 12:46:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 11 06:00:46 2022
Response via : Initial Calibration

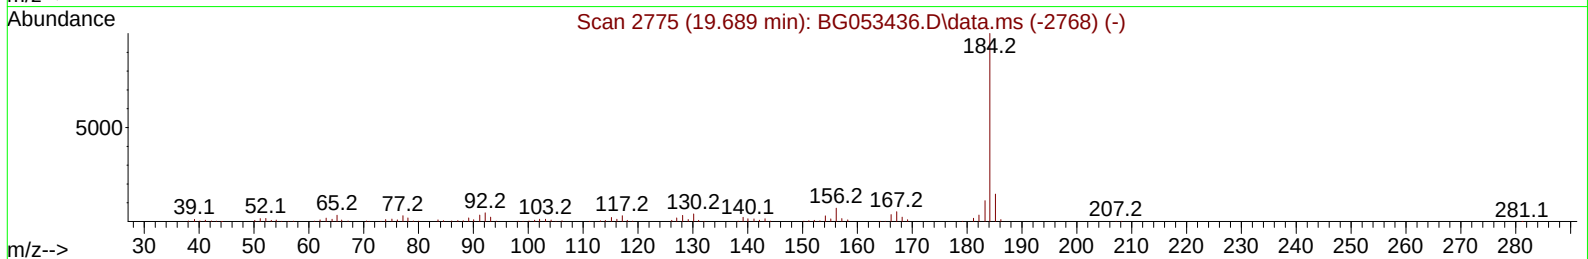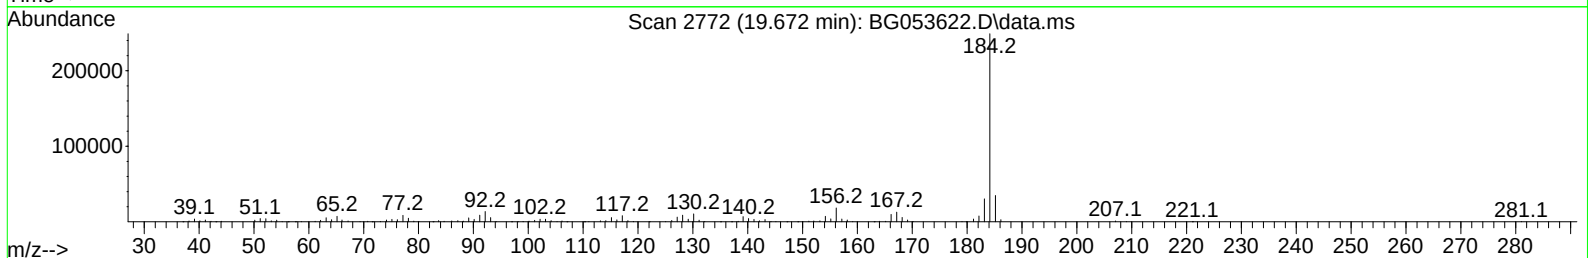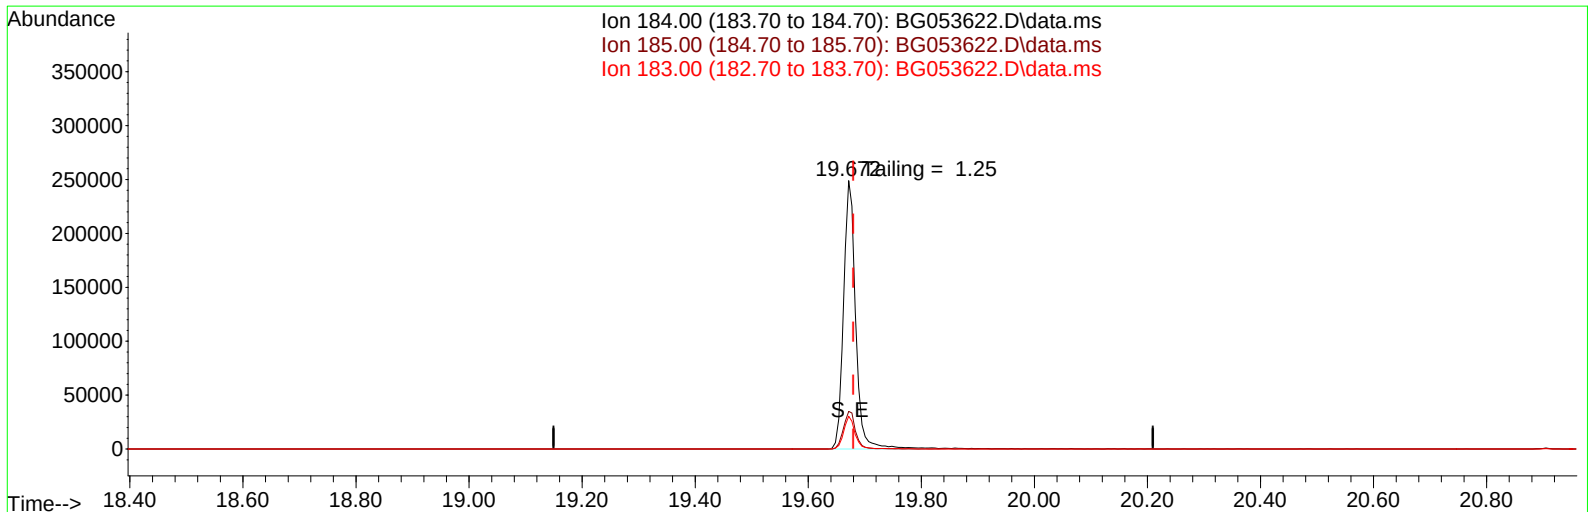

TIC: BG053622.D\data.ms

(77) Benzidine

19.672min (-0.008) 0.00 ng

response 371538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.04
183.00	11.10	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2022	BNA_G	<u>BG053622.D</u>
Compound Name	Response	Retention Time
DDT	190904	20.905
DDD	1675	20.517
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1675	192579	0.87

Instrument :
BNA_G
ClientSampleId :
DFTPP